

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
 Data File : VU049243.D
 Acq On : 17 Jun 2022 13:54
 Operator : SY/MD
 Sample : N3277-15DL 50000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0BB4DL

Quant Time: Jun 18 04:13:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 18 04:11:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	124642	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	115824	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	57754	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	53459	4.909	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.200%
7) Chloroethane-d5	1.912	69	37849	5.133	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	102.600%
11) 1,1-Dichloroethene-d2	2.565	65	21346	4.873	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	97.400%
20) 2-Butanone-d5	4.639	46	168011	57.776	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.560%
24) Chloroform-d	5.063	84	87098	5.097	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.703	65	49300	5.260	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.200%
32) Benzene-d6	5.729	84	177337	5.082	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.690	67	60433	5.103	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.899	98	155509	4.950	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
43) trans-1,3-Dichloroprop...	8.179	79	23208	4.411	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.200%
46) 2-Hexanone-d5	8.635	63	118614	55.889	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.780%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	48465	5.111	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	57074	5.150	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%
Target Compounds						
9) Trichlorofluoromethane	2.134	101	1519	0.125	ug/L	94
34) Trichloroethene	6.542	95	107874	12.245	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
Data File : VU049243.D
Acq On : 17 Jun 2022 13:54
Operator : SY/MD
Sample : N3277-15DL 50000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0BB4DL

Quant Time: Jun 18 04:13:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 18 04:11:00 2022
Response via : Initial Calibration




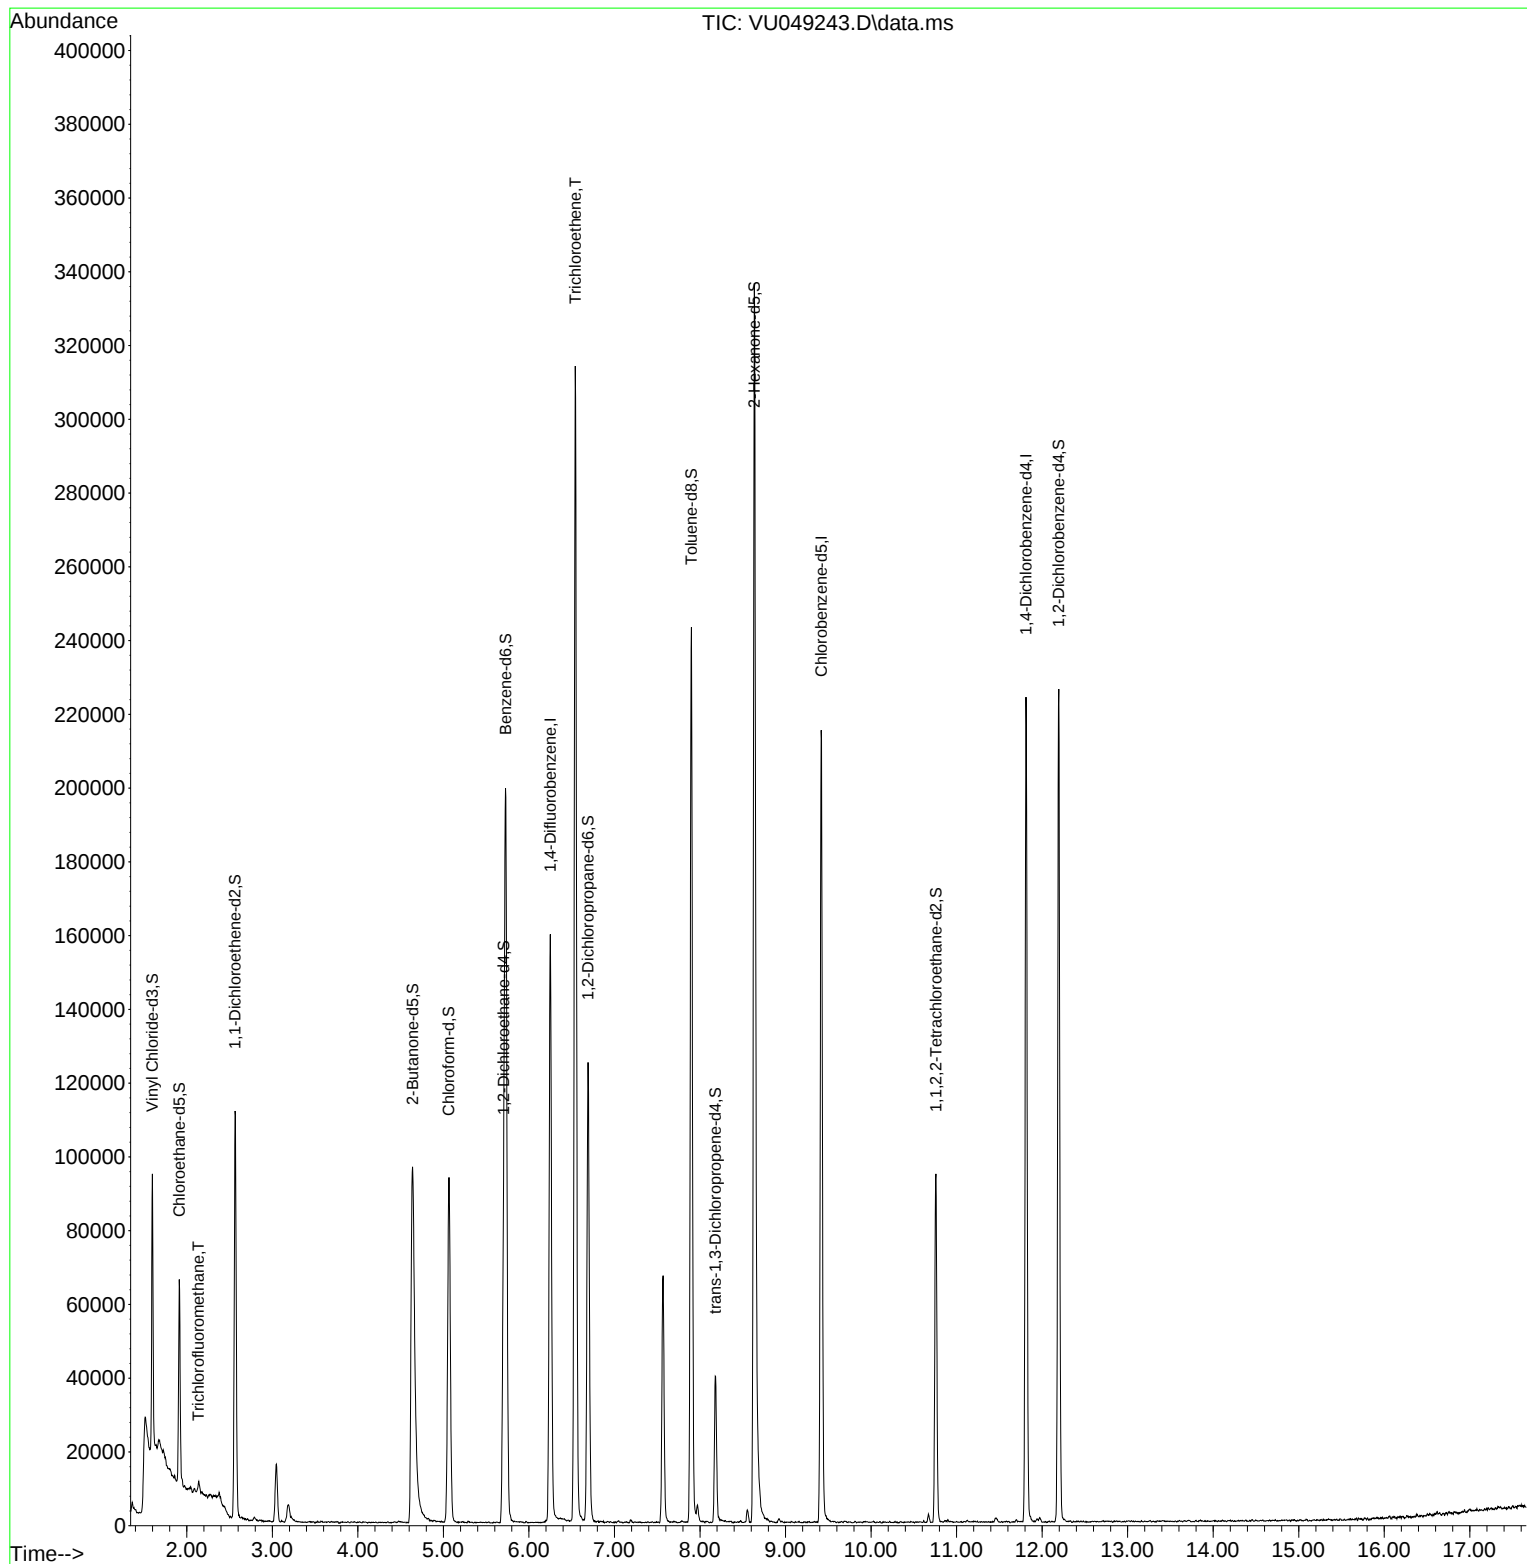


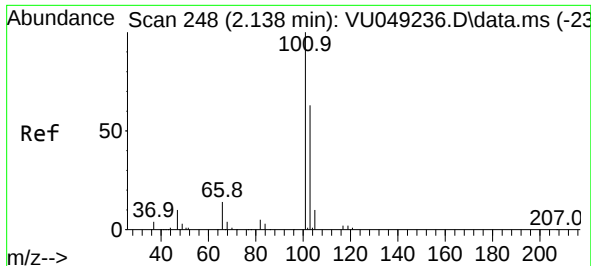

#9
Trichlorofluoromethane
Concen: 0.125 ug/L
RT: 2.134 min Scan# 248
Delta R.T. -0.003 min
Lab File: VU049243.D
Acq: 17 Jun 2022 13:54

Instrument :
MSVOA_U
ClientSampleId :
C0BB4DL

Tgt Ion:101 Resp: 1519
Ion Ratio Lower Upper
101 100
103 61.8 53.5 80.3

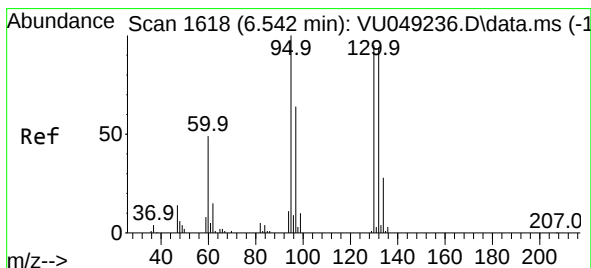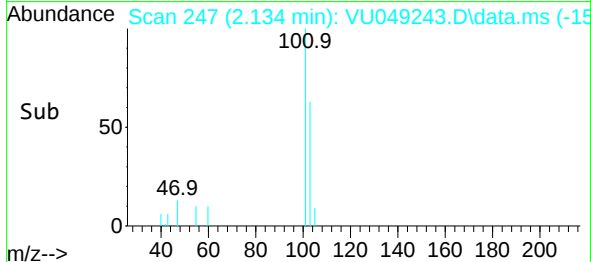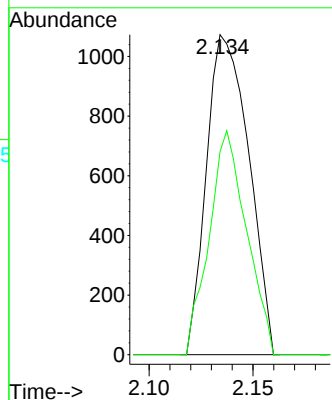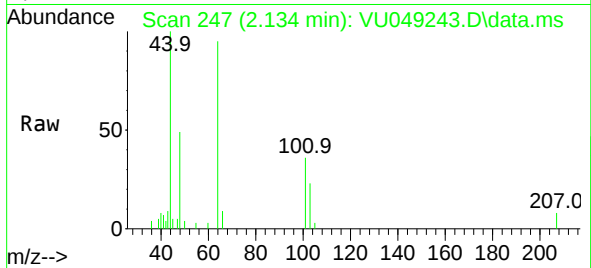

#34
Trichloroethene
Concen: 12.245 ug/L
RT: 6.542 min Scan# 1618
Delta R.T. -0.000 min
Lab File: VU049243.D
Acq: 17 Jun 2022 13:54

Tgt Ion: 95 Resp: 107874
Ion Ratio Lower Upper
95 100
97 65.0 45.3 84.1
132 91.6 61.5 114.3
130 94.8 65.6 121.8

