

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
 Data File : VU049237.D
 Acq On : 17 Jun 2022 11:26
 Operator : SY/MD
 Sample : VU0617WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK091

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU049237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rBV	75680	85894	15.44%	2.031%
2	1.913	170	178	190	rVB	55283	71545	12.86%	1.692%
3	2.568	370	382	399	rVB	108180	176827	31.78%	4.181%
4	3.048	518	531	541	rBV3	3609	6586	1.18%	0.156%
5	4.636	1012	1025	1062	rBV	76436	233414	41.95%	5.519%
6	5.067	1143	1159	1178	rBV	94138	203421	36.56%	4.810%
7	5.726	1344	1364	1389	rBV2	197146	503969	90.57%	11.917%
8	6.250	1511	1527	1550	rBV	161857	308014	55.36%	7.283%
9	6.690	1651	1664	1685	rBV	119770	236542	42.51%	5.593%
10	7.565	1922	1936	1958	rBV2	65441	117096	21.04%	2.769%
11	7.899	2025	2040	2057	rBV	241135	420334	75.54%	9.939%
12	7.970	2057	2062	2073	rVB3	3852	5939	1.07%	0.140%
13	8.179	2117	2127	2145	rBV2	38491	66917	12.03%	1.582%
14	8.636	2257	2269	2303	rBV2	281866	556423	100.00%	13.157%
15	9.417	2500	2512	2532	rBV	219995	366657	65.90%	8.670%
16	10.758	2917	2929	2945	rBV	88997	142151	25.55%	3.361%
17	11.812	3245	3257	3274	rBV	225499	361777	65.02%	8.555%
18	12.192	3360	3375	3396	rBV	218024	358981	64.52%	8.488%
19	14.092	3958	3966	3974	rBV2	4256	6591	1.18%	0.156%




Sum of corrected areas: 4229078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
Data File : VU049237.D
Acq On : 17 Jun 2022 11:26
Operator : SY/MD
Sample : VU0617WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK091

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

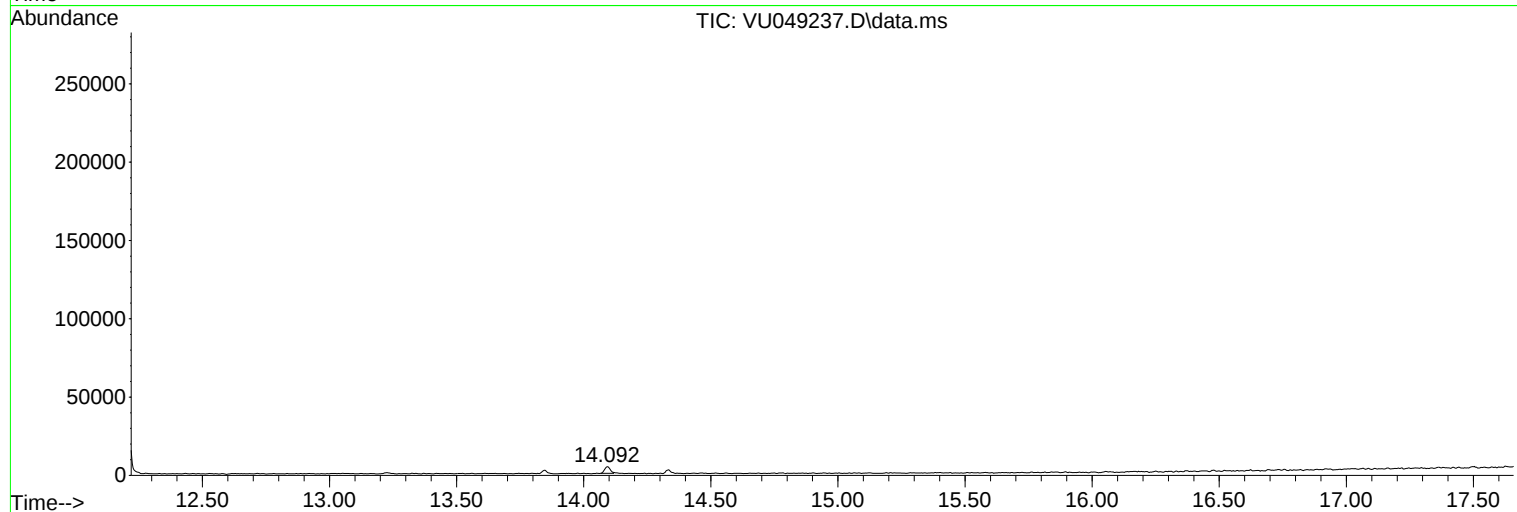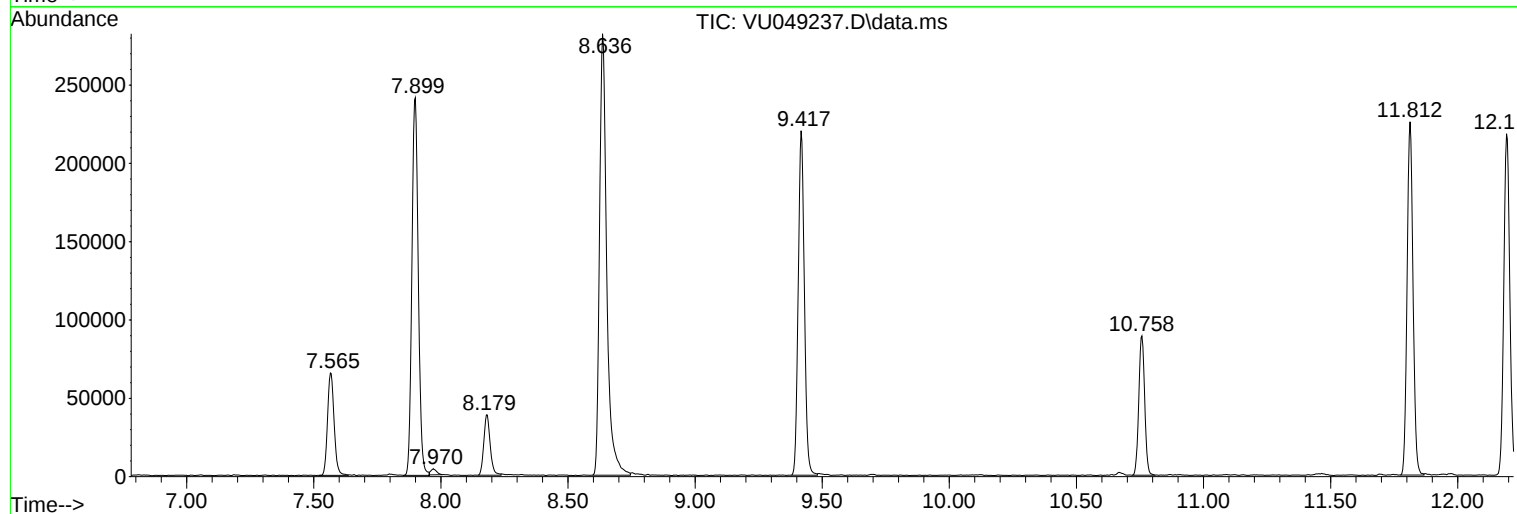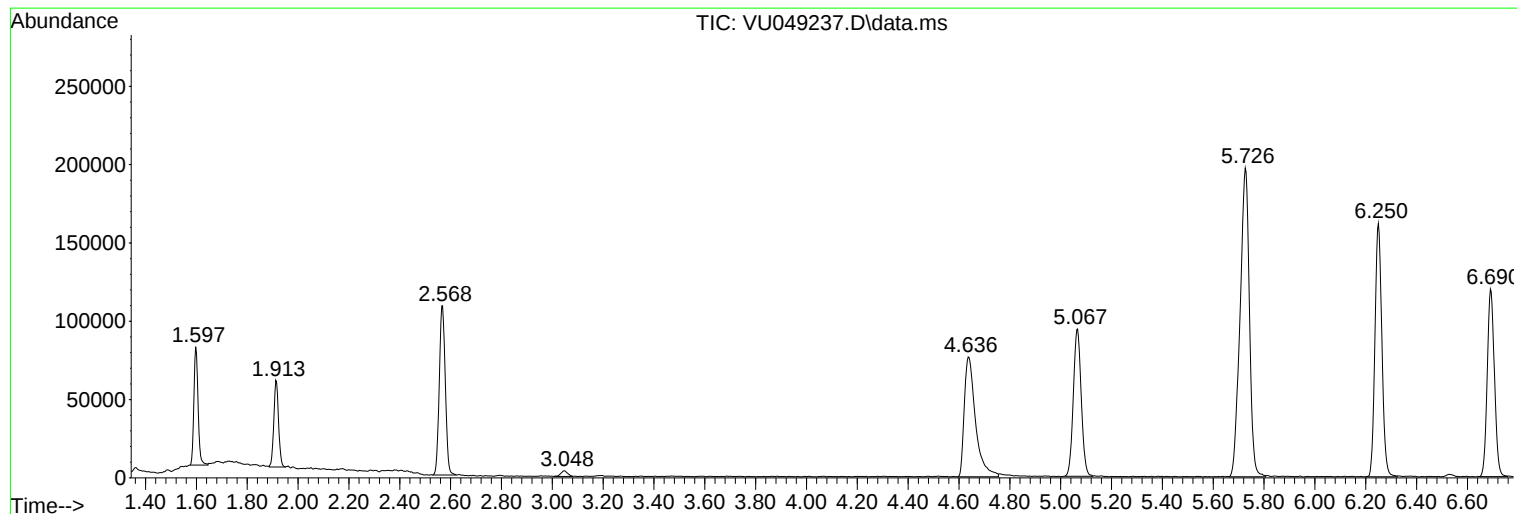

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
Data File : VU049237.D
Acq On : 17 Jun 2022 11:26
Operator : SY/MD
Sample : VU0617WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK091

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
Data File : VU049237.D
Acq On : 17 Jun 2022 11:26
Operator : SY/MD
Sample : VU0617WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK091

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc