


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061722\
 Data File : VU049235.D
 Acq On : 17 Jun 2022 08:49
 Operator : SY/MD
 Sample : BFB085
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB085

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jun 18 05:20:12 2022

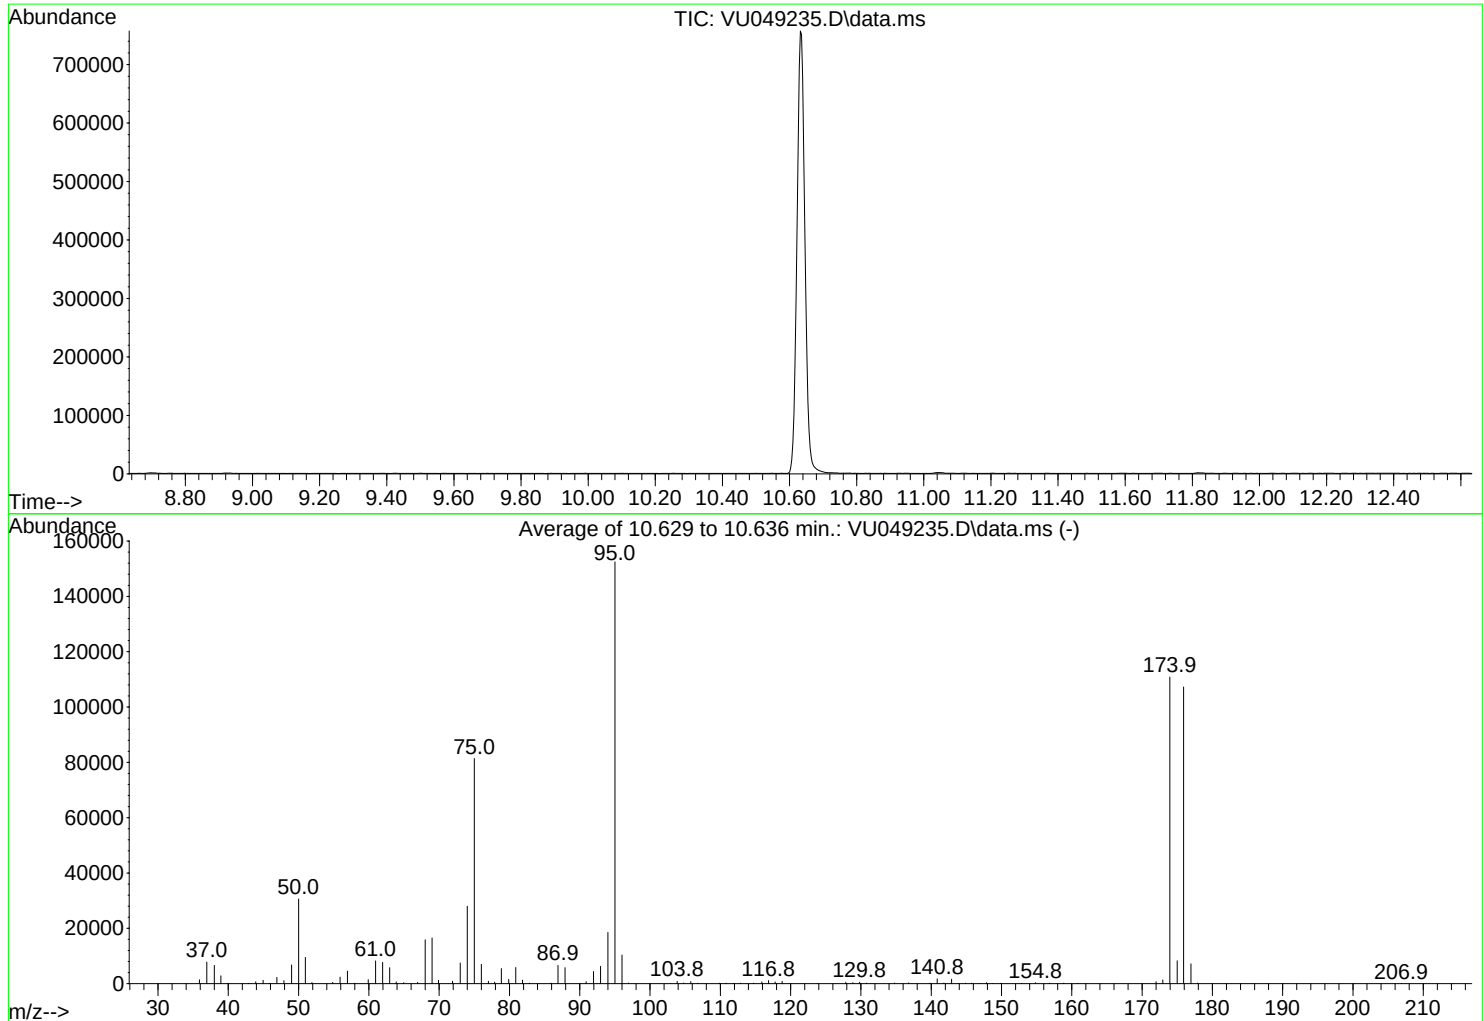

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	30603	PASS
75	95	30	80	53.4	81405	PASS
95	95	100	100	100.0	152491	PASS
96	95	5	9	6.8	10388	PASS
173	174	0.00	2	1.2	1366	PASS
174	95	50	120	72.7	110827	PASS
175	174	5	9	7.5	8263	PASS
176	174	95	101	96.8	107272	PASS
177	176	5	9	6.7	7179	PASS

Scan 2876 (10.587 min): VU049235.D\data.ms
BFB085

m/z	Abundance
39.90	152.0
43.80	655.0
207.10	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	1401.0
37.00	7641.0
38.00	6361.0
39.00	2764.0
39.80	244.0
42.90	111.0
43.90	1284.0
45.00	1130.0
45.90	143.0
46.90	2178.0
47.90	1049.0
49.00	6414.0
50.00	29504.0
50.90	8852.0
51.90	447.0
54.90	428.0
55.90	2269.0
56.90	4238.0
58.10	127.0
59.90	1415.0
60.90	7886.0
61.90	7474.0
62.90	5607.0
63.90	601.0
65.00	333.0
66.90	445.0
68.00	15104.0
69.00	15807.0
69.90	1206.0
71.90	798.0
73.00	7104.0
74.00	26888.0
75.00	77928.0
76.00	6939.0
77.00	880.0
77.90	658.0
78.80	5189.0
79.90	1508.0
80.90	5523.0
81.80	1273.0
82.90	163.0
85.80	129.0
86.00	129.0
86.90	6500.0
87.90	5568.0
90.90	607.0
92.00	4188.0
92.90	5696.0
94.00	17040.0
95.00	145344.0
96.00	10342.0
96.90	287.0
102.90	117.0
103.90	753.0
104.70	203.0
105.80	706.0
106.80	157.0
109.90	158.0
110.80	167.0
111.90	108.0
112.90	150.0
114.70	124.0
115.90	612.0
116.90	1049.0
117.80	683.0
118.80	769.0
127.90	507.0
128.90	333.0
129.80	543.0
130.80	223.0
134.80	217.0
136.80	292.0
139.80	136.0
140.80	1589.0
141.80	200.0
142.90	1449.0
144.90	187.0
145.80	144.0
146.90	107.0
147.90	340.0
148.70	106.0
149.80	135.0
152.80	139.0
154.90	394.0
156.80	198.0
158.80	165.0
160.90	118.0
172.00	664.0
173.00	1261.0
174.00	102296.0
175.00	7915.0
175.90	98960.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

177.00	6745.0
177.90	219.0
206.90	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	1422.0
37.00	8004.0
38.00	6771.0
39.00	2976.0
39.90	286.0
42.90	149.0
43.90	1377.0
45.00	1249.0
45.90	143.0
46.90	2301.0
47.90	1117.0
49.00	6978.0
50.00	31696.0
51.00	9806.0
51.90	441.0
54.90	454.0
55.90	2424.0
56.90	4636.0
58.00	160.0
59.90	1493.0
60.90	8427.0
61.90	7936.0
63.00	6004.0
63.90	663.0
65.00	340.0
66.90	462.0
68.00	16351.0
69.00	17008.0
69.90	1269.0
71.90	922.0
73.00	7724.0
74.00	28936.0
75.00	84096.0
76.00	7269.0
77.00	909.0
77.90	640.0
78.90	5567.0
79.90	1673.0
80.90	6045.0
81.80	1301.0
82.90	174.0
85.90	180.0
86.90	6879.0
87.90	5897.0
90.90	717.0
92.00	4544.0
92.90	6468.0
94.00	19136.0
95.00	157376.0
96.00	10686.0
96.90	264.0
102.90	116.0
103.90	831.0
104.80	206.0
105.80	726.0
106.80	153.0
109.80	163.0
110.80	198.0
111.90	104.0
112.90	185.0
114.80	177.0
115.90	640.0
116.80	1151.0
117.80	659.0
118.80	874.0
123.80	110.0
127.90	529.0
128.90	339.0
129.80	548.0
130.80	186.0
134.80	235.0
136.80	317.0
139.80	181.0
140.80	1785.0
141.80	212.0
142.90	1672.0
144.90	169.0
145.70	173.0
146.90	117.0
147.90	361.0
149.90	153.0
152.80	142.0
154.80	349.0
156.90	189.0
158.80	203.0
160.80	123.0
172.00	735.0
173.00	1414.0
173.90	114104.0
175.00	8610.0
175.90	110648.0
177.00	7417.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

177.90206.90

217.0126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

m/z	Abundance
35.90	1346.0
36.90	7718.0
38.00	6721.0
38.90	2831.0
39.90	313.0
42.90	165.0
44.00	1401.0
44.90	1323.0
45.80	112.0
46.90	2218.0
47.90	1094.0
49.00	6869.0
50.00	30608.0
51.00	9795.0
51.90	385.0
54.80	454.0
55.90	2386.0
57.00	4742.0
57.90	180.0
59.90	1502.0
61.00	8386.0
62.00	7631.0
63.00	5792.0
63.90	624.0
64.90	325.0
67.00	430.0
68.00	16031.0
69.00	16832.0
69.90	1203.0
71.90	953.0
73.00	7626.0
74.00	28104.0
75.00	82192.0
76.00	6883.0
77.00	888.0
77.90	544.0
78.90	5499.0
79.90	1591.0
80.90	6013.0
81.90	1275.0
82.80	187.0
86.00	206.0
86.90	6485.0
87.90	5878.0
90.90	717.0
91.90	4558.0
93.00	6625.0
94.00	19400.0
95.00	154752.0
96.00	10136.0
97.00	231.0
103.80	875.0
104.90	215.0
105.80	752.0
106.80	152.0
109.80	151.0
110.80	209.0
111.80	125.0
112.90	200.0
114.80	204.0
115.90	660.0
116.80	1205.0
117.80	633.0
118.80	935.0
123.80	107.0
127.80	539.0
128.80	328.0
129.80	524.0
130.80	146.0
134.80	270.0
136.80	331.0
139.80	160.0
140.90	1796.0
141.80	216.0
142.90	1769.0
143.80	100.0
144.90	132.0
145.80	199.0
147.80	389.0
149.90	152.0
152.90	101.0
154.80	289.0
156.90	196.0
158.90	227.0
160.90	138.0
172.00	654.0
172.90	1423.0
173.90	116080.0
175.00	8263.0
175.90	112208.0
176.90	7375.0
177.90	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085

207.10

133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB085