


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061725\
Data File : VU063406.D
Acq On : 17 Jun 2025 08:43
Operator : MD/SY
Sample : BFB025
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB025

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM061625.M
Title : TRACE VOA SOM01.0
Last Update : Tue Jun 17 11:04:00 2025

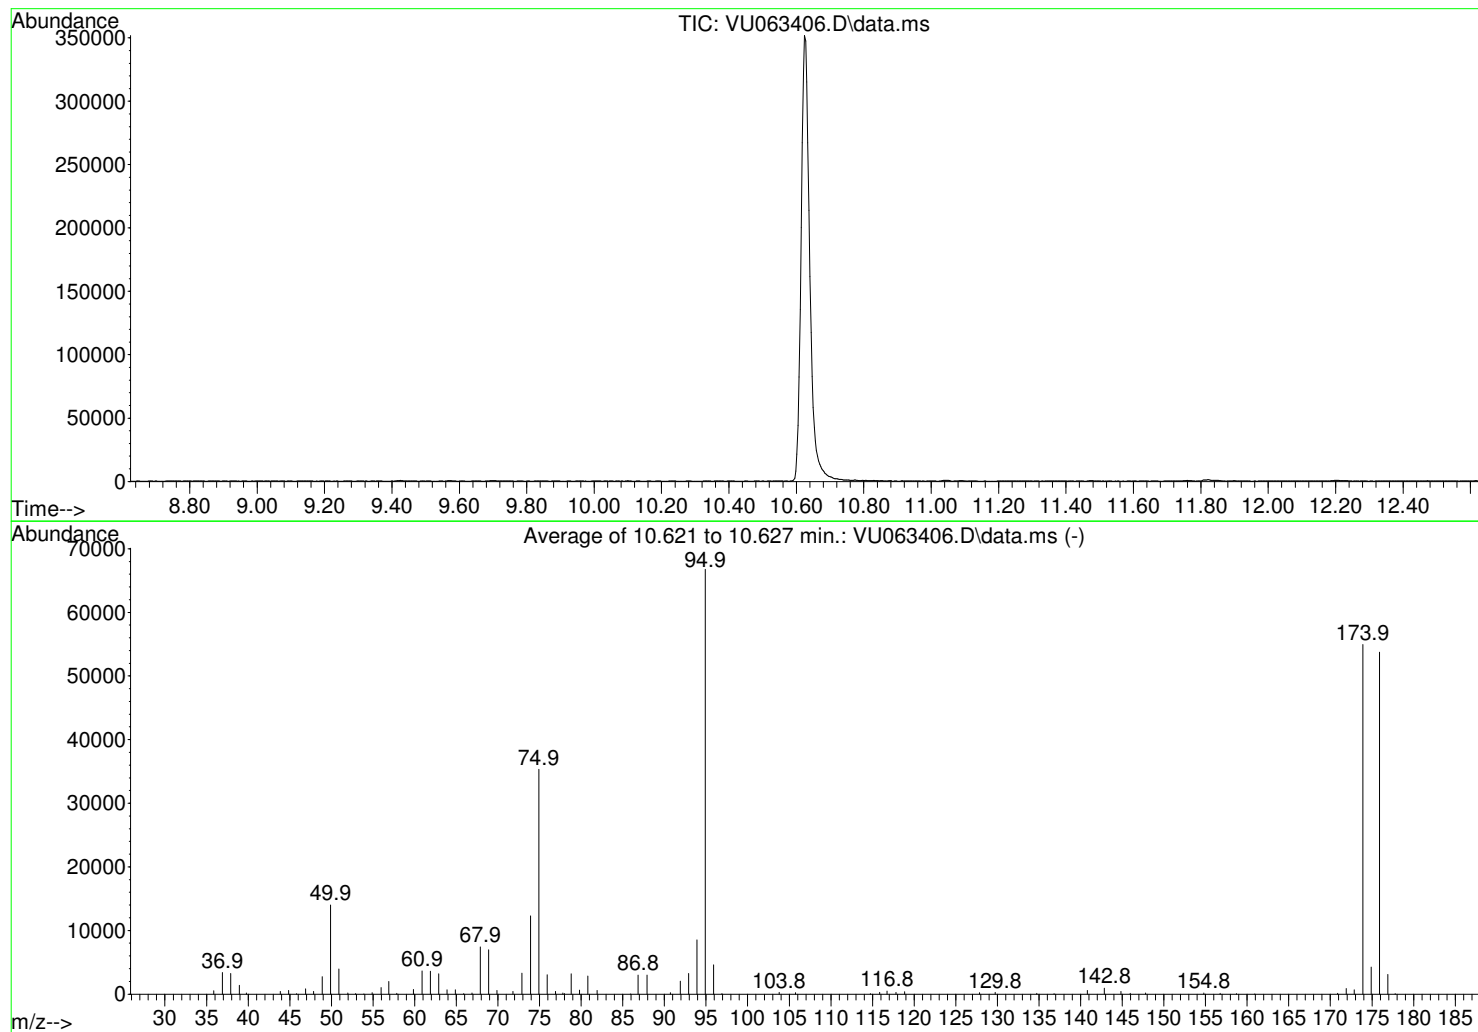

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	13997	PASS
75	95	30	80	52.9	35347	PASS
95	95	100	100	100.0	66776	PASS
96	95	5	9	6.9	4614	PASS
173	174	0.00	2	1.2	667	PASS
174	95	50	120	82.3	54968	PASS
175	174	5	9	7.7	4230	PASS
176	174	95	101	97.8	53741	PASS
177	176	5	9	5.8	3100	PASS

m/z	Abundance
43.80	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	550.0
36.90	3362.0
37.90	3270.0
39.00	1265.0
39.80	184.0
43.90	610.0
44.90	565.0
45.80	102.0
46.90	862.0
47.90	394.0
48.90	2532.0
49.90	13358.0
50.90	3852.0
51.90	215.0
52.90	130.0
53.90	103.0
54.90	218.0
56.00	953.0
56.90	2030.0
57.80	112.0
59.80	749.0
60.90	3401.0
61.90	3685.0
62.90	3009.0
63.90	678.0
64.90	644.0
66.90	165.0
67.90	7043.0
68.90	6361.0
69.90	547.0
71.80	453.0
72.90	3232.0
73.90	11775.0
74.90	33720.0
75.90	3046.0
76.90	430.0
77.80	275.0
78.80	2948.0
79.80	596.0
80.80	2714.0
81.90	507.0
86.80	3075.0
87.90	2797.0
90.70	202.0
91.90	1873.0
92.90	2997.0
93.90	8210.0
94.90	63336.0
95.90	4516.0
96.90	151.0
103.80	252.0
105.80	241.0
115.90	215.0
116.70	495.0
117.80	269.0
118.90	375.0
127.90	198.0
129.70	211.0
134.70	121.0
140.80	498.0
142.80	845.0
144.80	459.0
145.90	148.0
147.80	175.0
154.80	197.0
156.80	118.0
158.70	120.0
170.90	117.0
171.90	840.0
172.80	638.0
173.90	51520.0
174.90	3911.0
175.90	49840.0
176.90	2992.0
177.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.90	568.0
36.90	3506.0
37.90	3319.0
38.90	1446.0
39.80	186.0
43.90	671.0
44.80	559.0
45.80	120.0
46.90	818.0
47.80	411.0
48.90	2821.0
49.90	14553.0
50.90	4090.0
51.90	181.0
52.90	126.0
54.90	249.0
55.90	1060.0
56.90	2047.0
57.90	117.0
59.80	771.0
60.90	3766.0
61.90	3719.0
62.90	3275.0
63.90	702.0
64.90	720.0
65.90	111.0
66.90	184.0
67.90	7686.0
68.90	7169.0
69.90	585.0
71.80	463.0
72.90	3407.0
73.90	12673.0
74.90	36656.0
75.90	3164.0
76.90	444.0
77.80	312.0
78.80	3304.0
79.80	620.0
80.80	2944.0
81.90	573.0
86.80	3041.0
87.90	3135.0
90.70	215.0
91.90	2067.0
92.90	3406.0
93.90	8832.0
94.90	68808.0
95.90	4810.0
96.90	138.0
103.80	303.0
105.70	239.0
114.70	106.0
115.80	275.0
116.80	475.0
117.80	314.0
118.80	396.0
127.80	263.0
129.80	299.0
134.70	136.0
136.80	116.0
140.80	614.0
142.90	971.0
144.80	460.0
145.90	139.0
147.80	175.0
154.80	197.0
156.70	147.0
158.70	117.0
170.80	143.0
171.90	903.0
172.90	677.0
173.90	56696.0
174.90	4384.0
175.90	55536.0
176.90	3192.0
177.80	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025

m/z	Abundance
35.80	517.0
36.90	3388.0
37.90	3093.0
38.90	1477.0
39.80	216.0
43.90	688.0
44.80	572.0
46.90	794.0
47.90	406.0
48.90	2817.0
49.90	14079.0
50.90	3982.0
52.00	174.0
54.90	232.0
55.90	1098.0
56.90	1947.0
57.90	102.0
59.90	730.0
60.90	3755.0
61.90	3455.0
62.90	3303.0
63.90	681.0
64.90	738.0
65.90	115.0
66.90	197.0
67.90	7464.0
68.90	7404.0
69.90	554.0
71.80	398.0
72.90	3247.0
73.90	12399.0
74.90	35664.0
75.90	2937.0
76.90	400.0
78.00	285.0
78.80	3267.0
79.80	641.0
80.80	2940.0
81.90	645.0
85.90	108.0
86.90	2935.0
87.90	3103.0
90.70	226.0
91.90	2150.0
92.90	3333.0
93.90	8524.0
94.90	68184.0
95.90	4517.0
103.80	310.0
105.70	223.0
114.80	101.0
115.80	281.0
116.80	477.0
117.80	316.0
118.80	376.0
127.80	295.0
129.80	327.0
134.80	141.0
136.80	121.0
140.80	667.0
142.90	1015.0
144.90	378.0
146.00	128.0
147.80	142.0
154.80	163.0
156.80	156.0
160.90	121.0
170.80	146.0
171.90	937.0
172.90	686.0
173.90	56688.0
174.90	4394.0
175.90	55848.0
176.90	3116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB025