

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061818\
 Data File : VU024689.D
 Acq On : 18 Jun 2018 14:11
 Operator : MD/SY
 Sample : J3463-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T2-MW-1-9.0-061218

Quant Time: Jun 18 18:25:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	202687	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	322454	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	300936	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.49	152	151099	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	142171	42.97	ug/l	0.00
Spiked Amount	50.000		Recovery	=	85.94%	
35) Dibromofluoromethane	4.89	113	128676	48.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.16%	
50) Toluene-d8	7.57	98	465572	47.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.40%	
62) 4-Bromofluorobenzene	10.31	95	164557	42.46	ug/l	0.00
Spiked Amount	50.000		Recovery	=	84.92%	
Target Compounds						
16) Acetone	2.32	43	186128	104.69	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061818\
 Data File : VU024689.D
 Acq On : 18 Jun 2018 14:11
 Operator : MD/SY
 Sample : J3463-04
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 T2-MW-1-9.0-061218

Quant Time: Jun 18 18:25:49 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 13 13:55:26 2018
 Response via : Initial Calibration




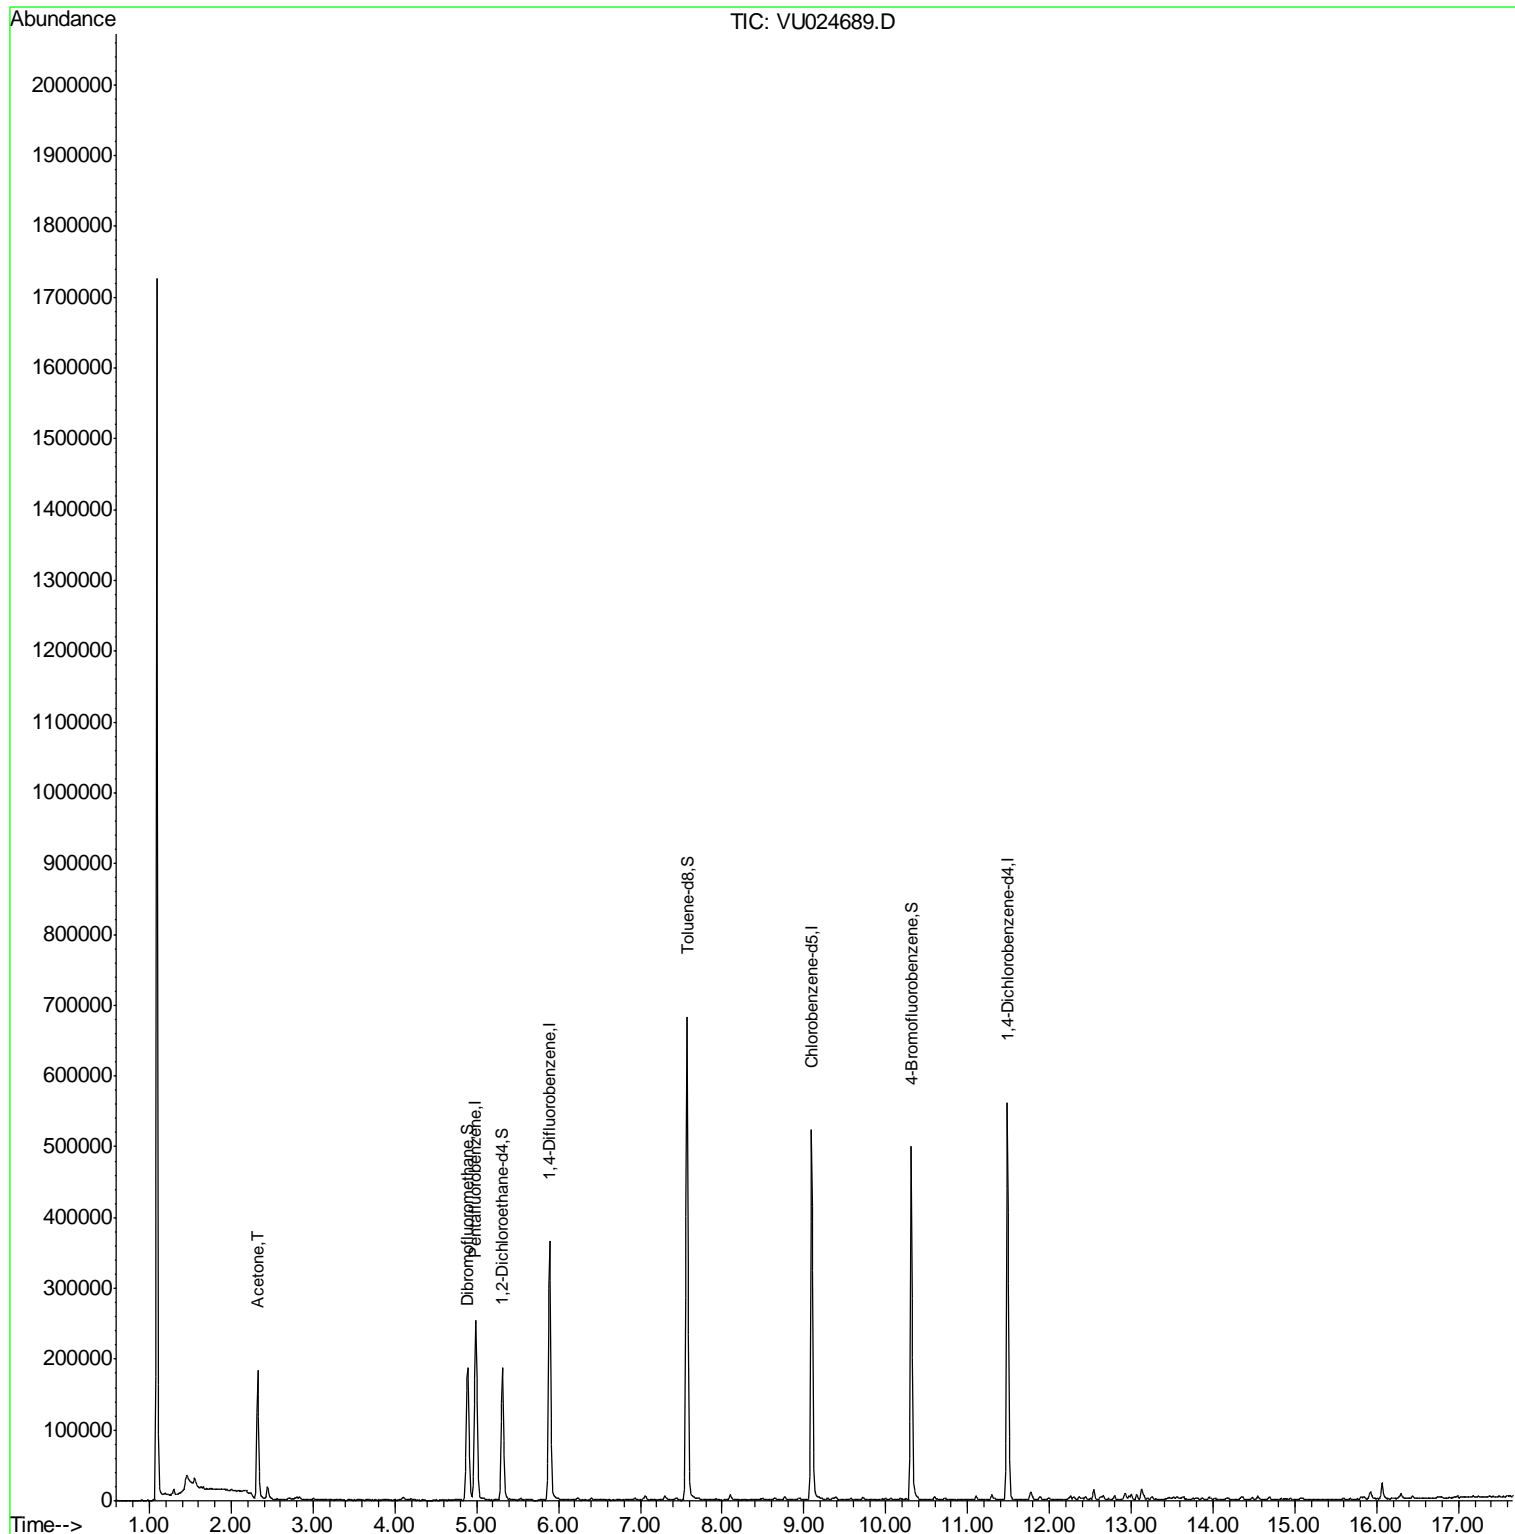


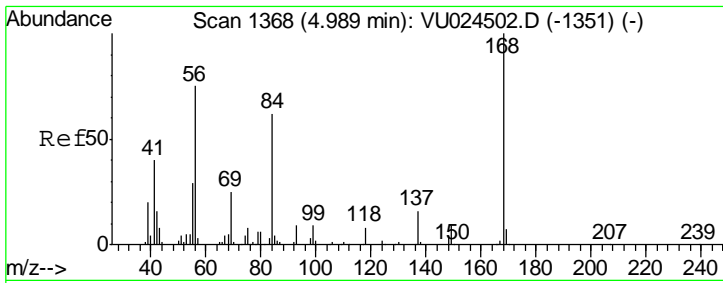

#1
 Pentafluorobenzene
 Concen: 50.00 ug/l
 RT: 4.99 min Scan# 1368
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11




Instrument :
 MSVOA_U
 ClientSampled :
 T2-MW-1-9.0-061218


Tgt Ion	Resp	Lower	Upper
168	100		
99	52.2	43.2	64.8

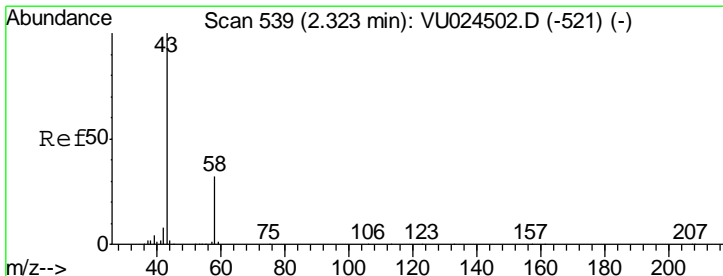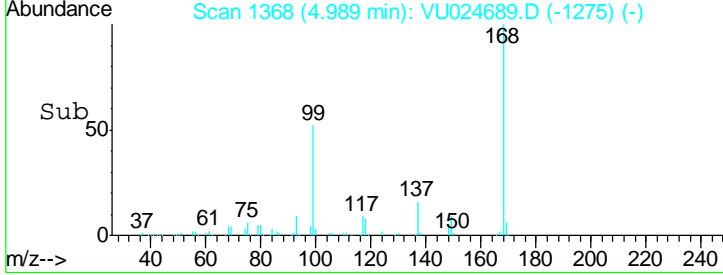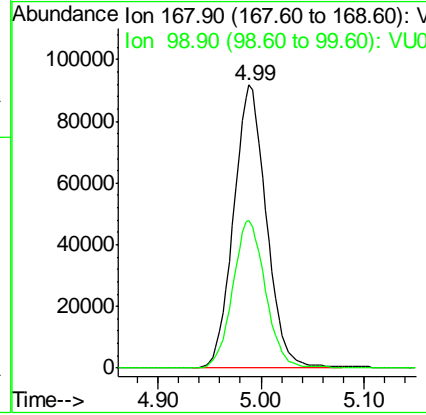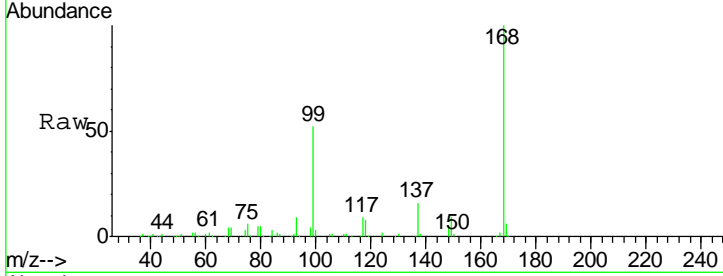

#16
 Acetone
 Concen: 104.69 ug/l
 RT: 2.32 min Scan# 539
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11

Tgt Ion	Resp	Lower	Upper
43	100		
58	33.0	24.4	36.6


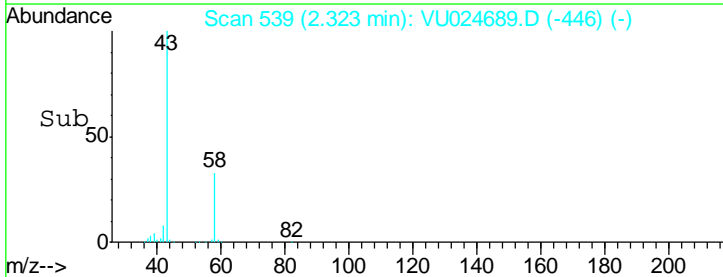
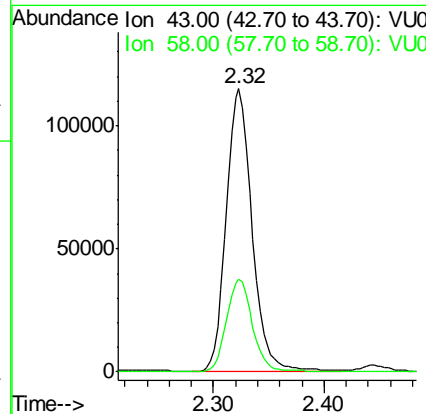
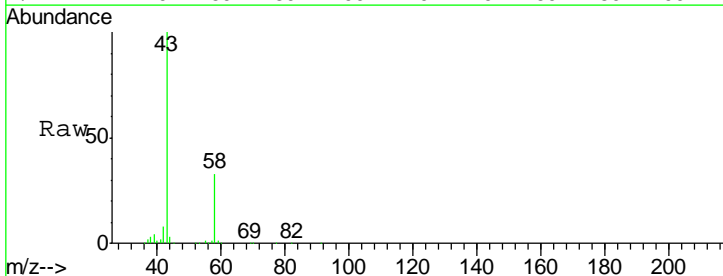


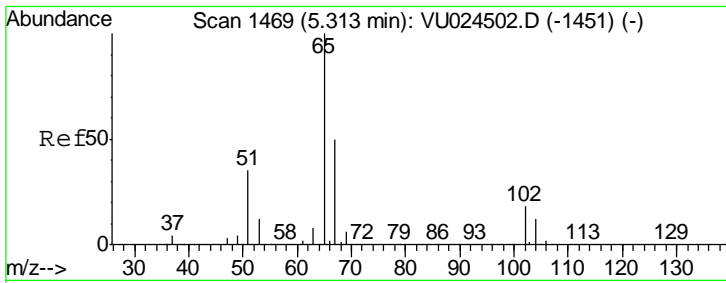

#33
 1,2-Dichloroethane-d4
 Concen: 42.97 ug/l
 RT: 5.31 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11




Instrument :
 MSVOA_U
ClientSampled :
 T2-MW-1-9.0-061218


Tgt Ion	Resp	Lower	Upper
65	142171		
67	54.3	0.0	107.0

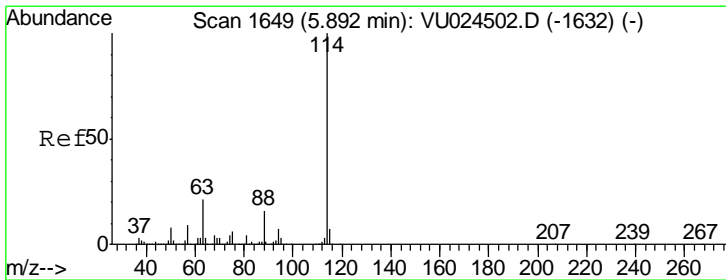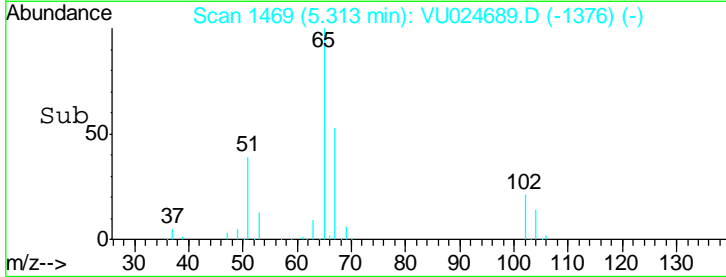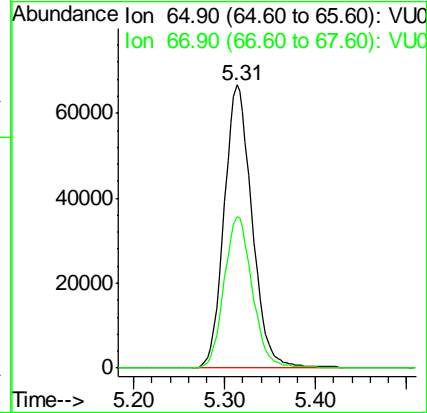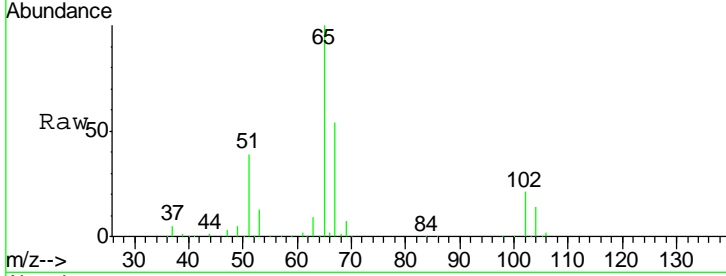

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 5.89 min Scan# 1649
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11

Tgt Ion	Resp	Lower	Upper
114	322454		
63	20.7	0.0	45.4
88	15.6	0.0	31.0


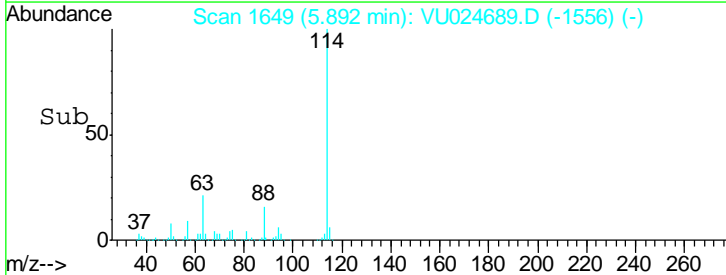
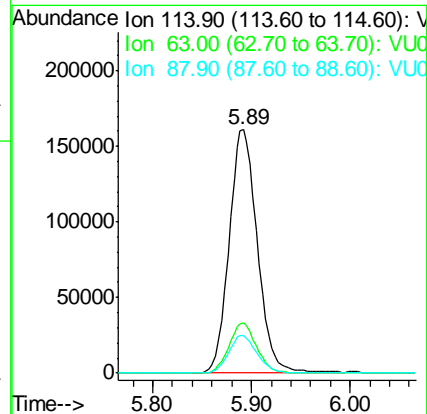
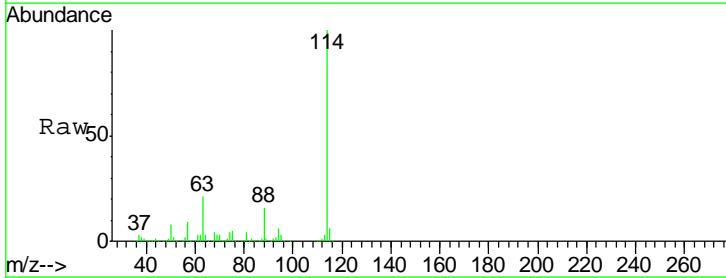


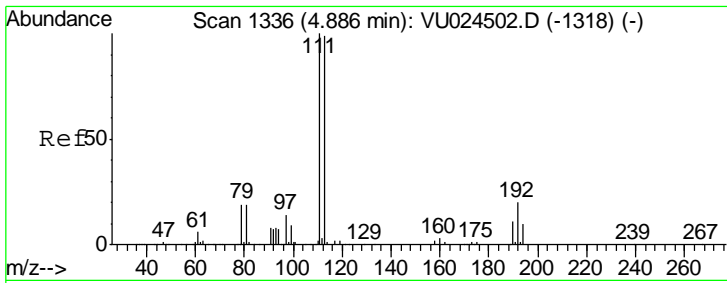

#35
 Dibromofluoromethane
 Concen: 48.08 ug/l
 RT: 4.89 min Scan# 1337
 Delta R.T. 0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11




Instrument :
 MSVOA_U
 ClientSampleId :
 T2-MW-1-9.0-061218


Tgt Ion	Resp	Lower	Upper
113	100		
111	102.6	82.2	123.4
192	21.8	16.2	24.4

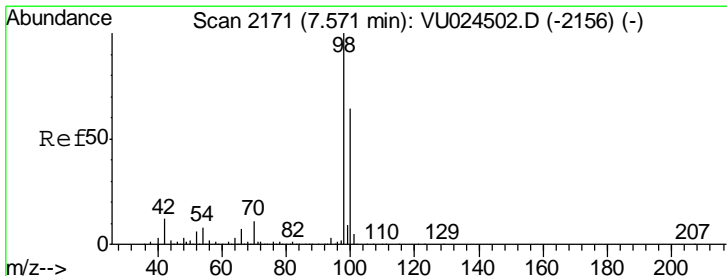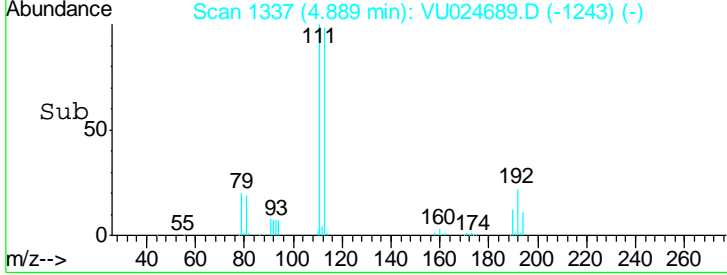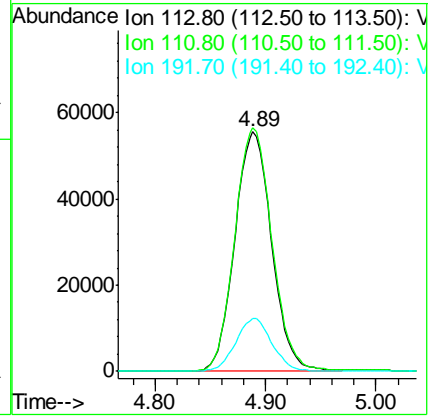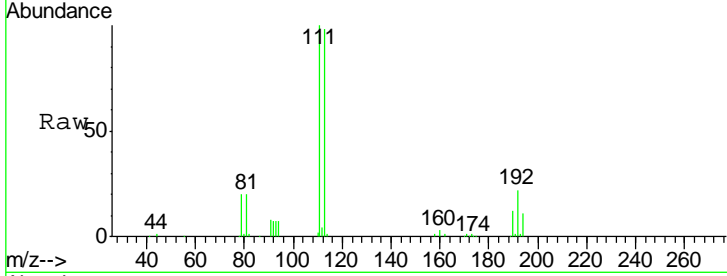

#50
 Toluene-d8
 Concen: 47.70 ug/l
 RT: 7.57 min Scan# 2171
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11

Tgt Ion	Resp	Lower	Upper
98	100		
100	63.9	51.1	76.7


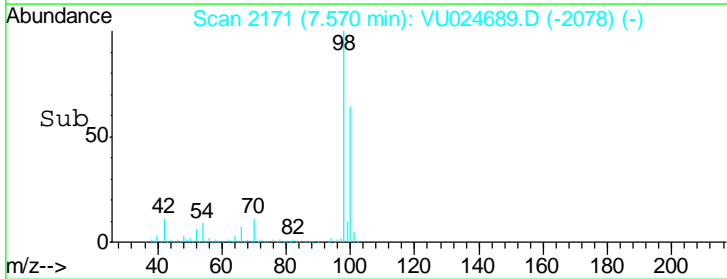
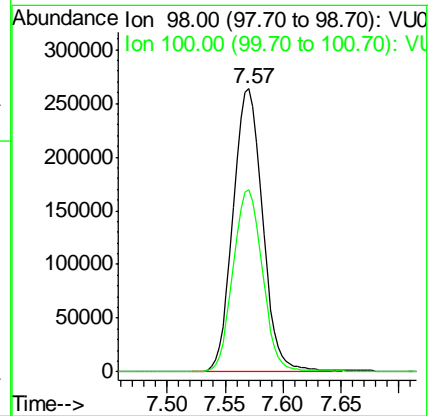
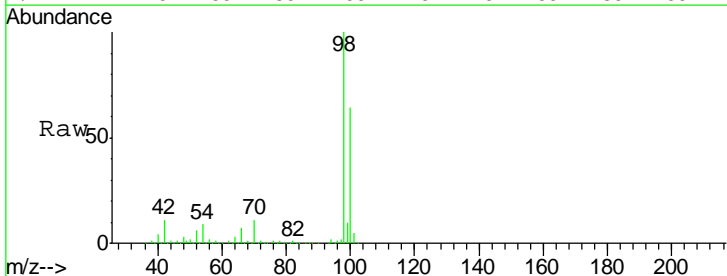


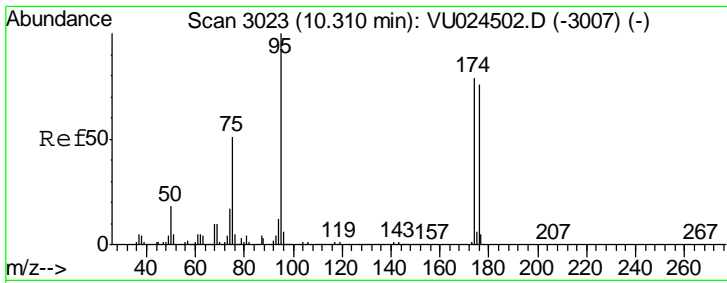

#62
 4-Bromofluorobenzene
 Concen: 42.46 ug/l
 RT: 10.31 min Scan# 3023
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11




Instrument :
 MSVOA_U
 ClientSampled :
 T2-MW-1-9.0-061218


Tgt Ion	Resp	Lower	Upper
95	164557		
174	86.8	0.0	165.8
176	83.5	0.0	159.4

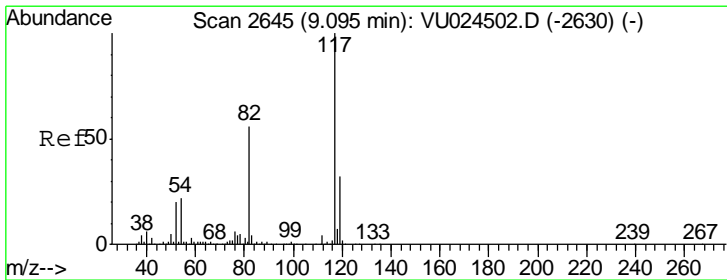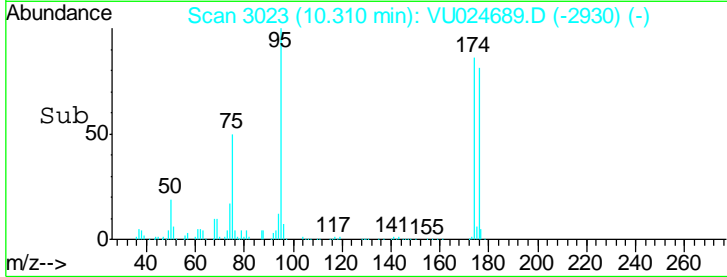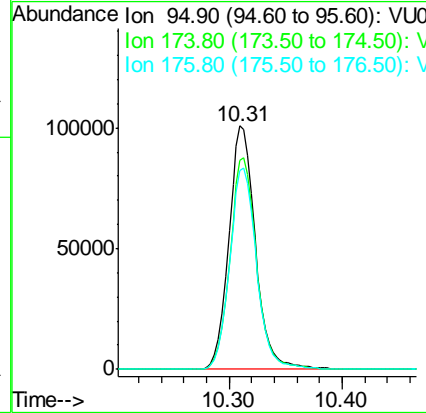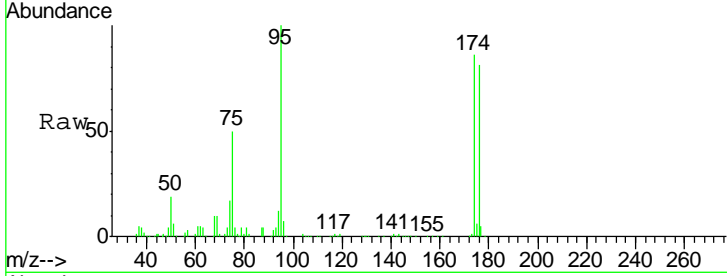

#63
 Chlorobenzene-d5
 Concen: 50.00 ug/l
 RT: 9.09 min Scan# 2645
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11

Tgt Ion	Resp	Lower	Upper
117	300936		
82	53.4	44.3	66.5
119	32.6	25.4	38.2

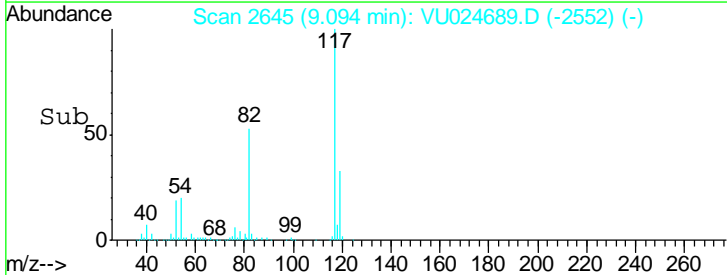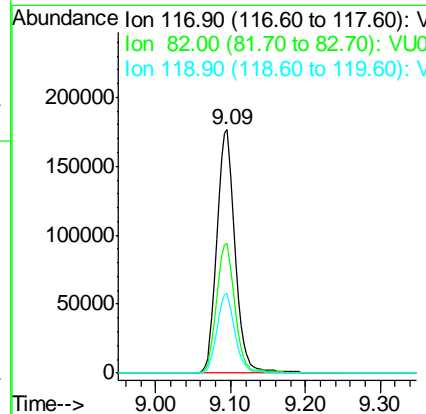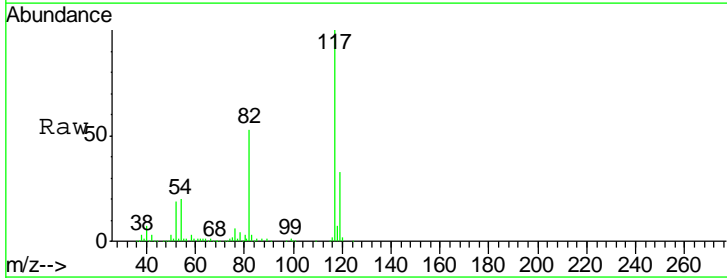

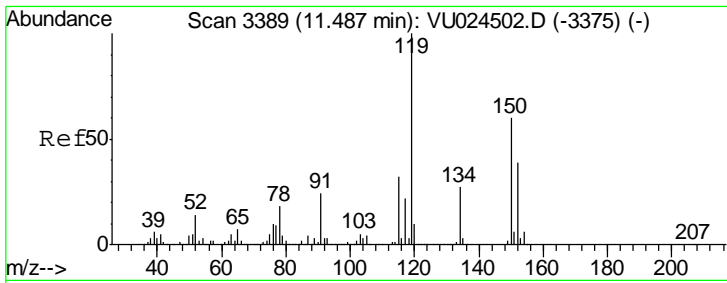

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.00 ug/l
 RT: 11.49 min Scan# 3389
 Delta R.T. -0.00 min
 Lab File: VU024689.D
 Acq: 18 Jun 2018 14:11

Instrument : MSVOA_U
 ClientSampled : T2-MW-1-9.0-061218

Tot Ion	Resp	Lower	Upper
152	151099		
152	100		
115	57.6	43.0	129.0
150	157.8	0.0	354.0

