


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061818\
Data File : VU024708.D
Acq On : 18 Jun 2018 22:16
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

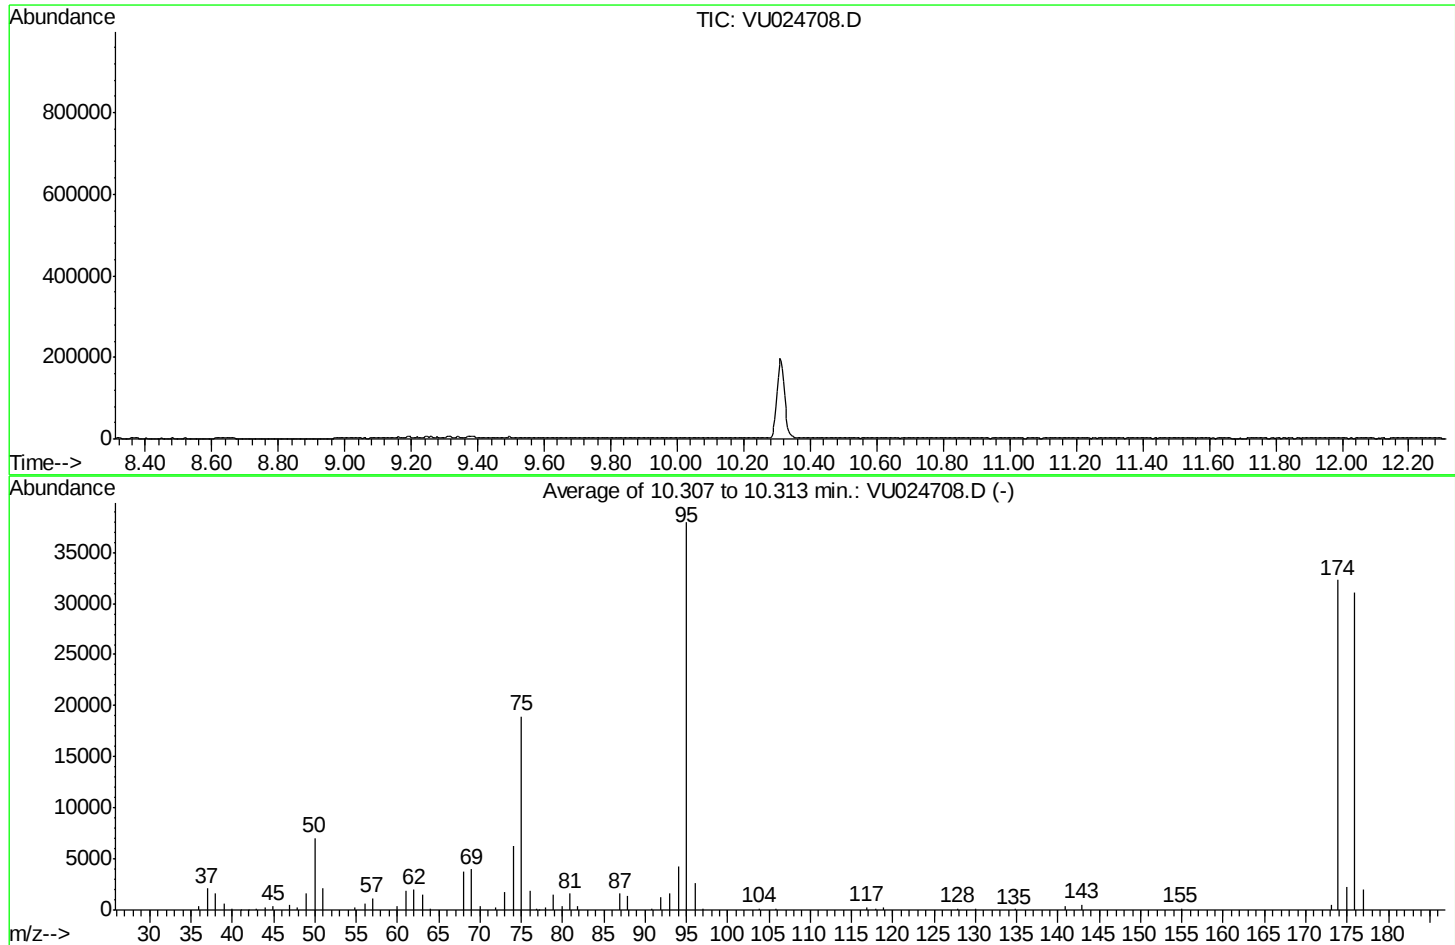

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7036	PASS
75	95	30	60	49.9	18946	PASS
95	95	100	100	100.0	37946	PASS
96	95	5	9	6.9	2628	PASS
173	174	0.00	2	1.5	470	PASS
174	95	50	100	85.0	32269	PASS
175	174	5	9	6.8	2202	PASS
176	174	95	101	96.4	31093	PASS
177	176	5	9	6.5	2016	PASS