

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\

Data File : VU038973.D

Acq On : 18 Jun 2020 16:27

Operator : SY/MD

Sample : L3058-07

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:18:44 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Jun 19 01:17:22 2020

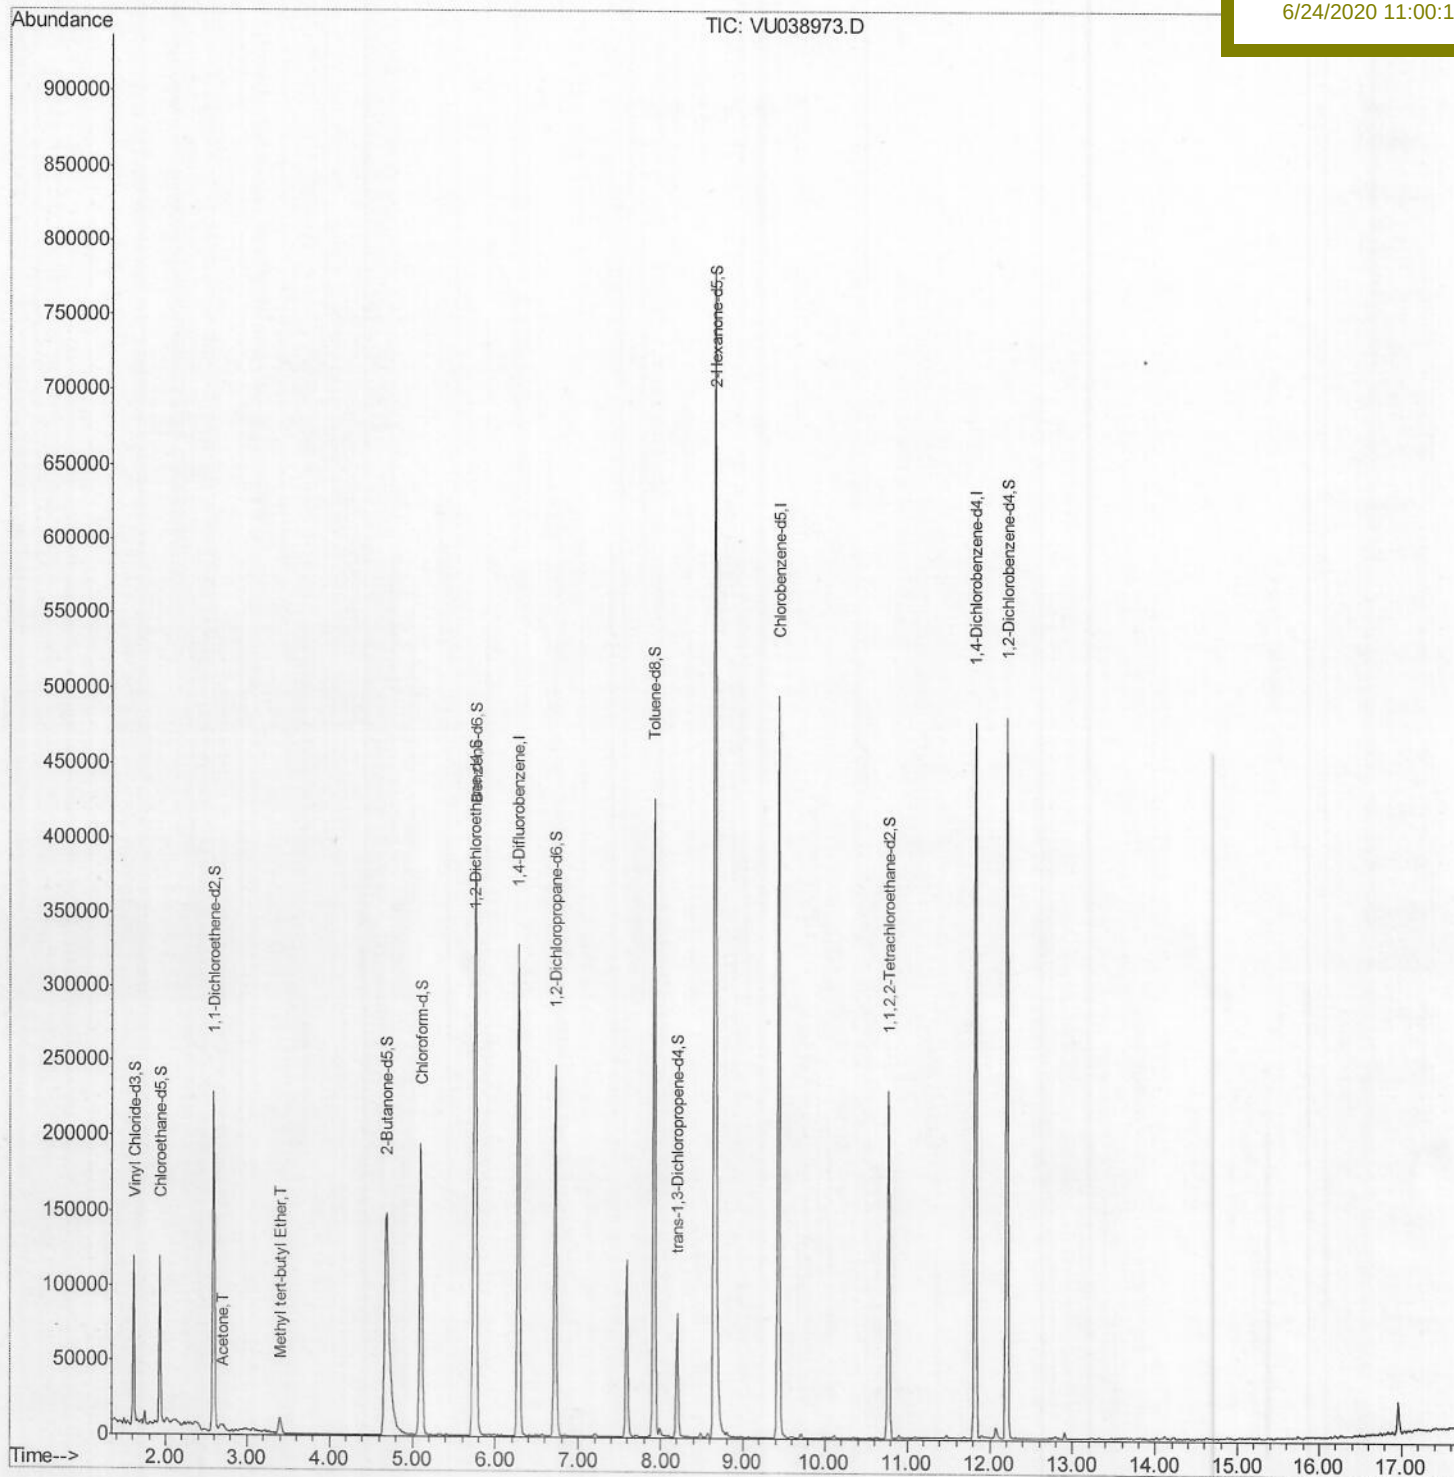
Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :

F9L38

Manual Integrations
APPROVEDMMDadoda
6/24/2020 11:00:14 AM

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\

Data File : VU038973.D

Acq On : 18 Jun 2020 16:27

Operator : SY/MD

Sample : L3058-07

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:20:41 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Jun 19 01:17:22 2020

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :

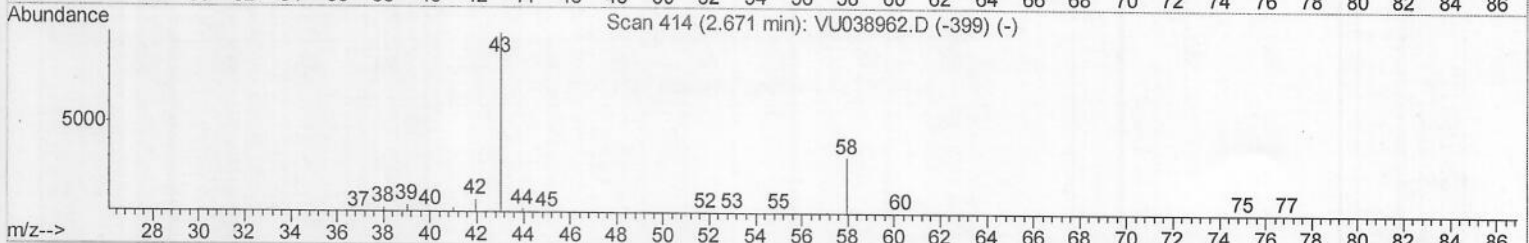
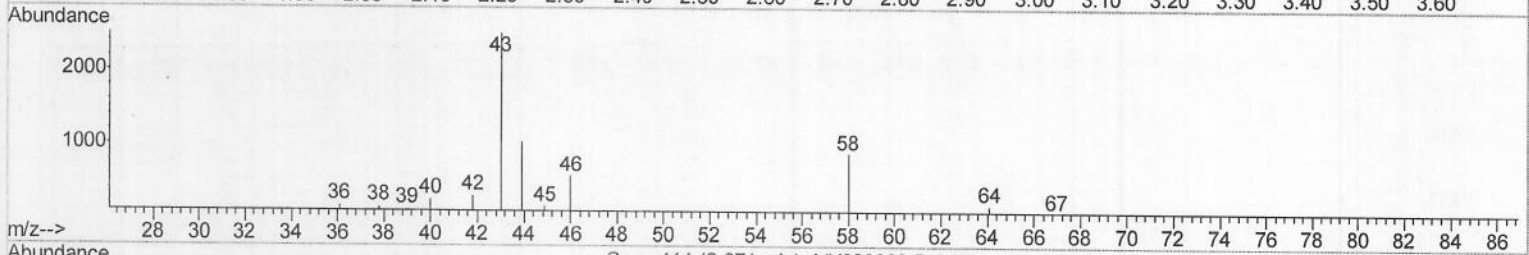
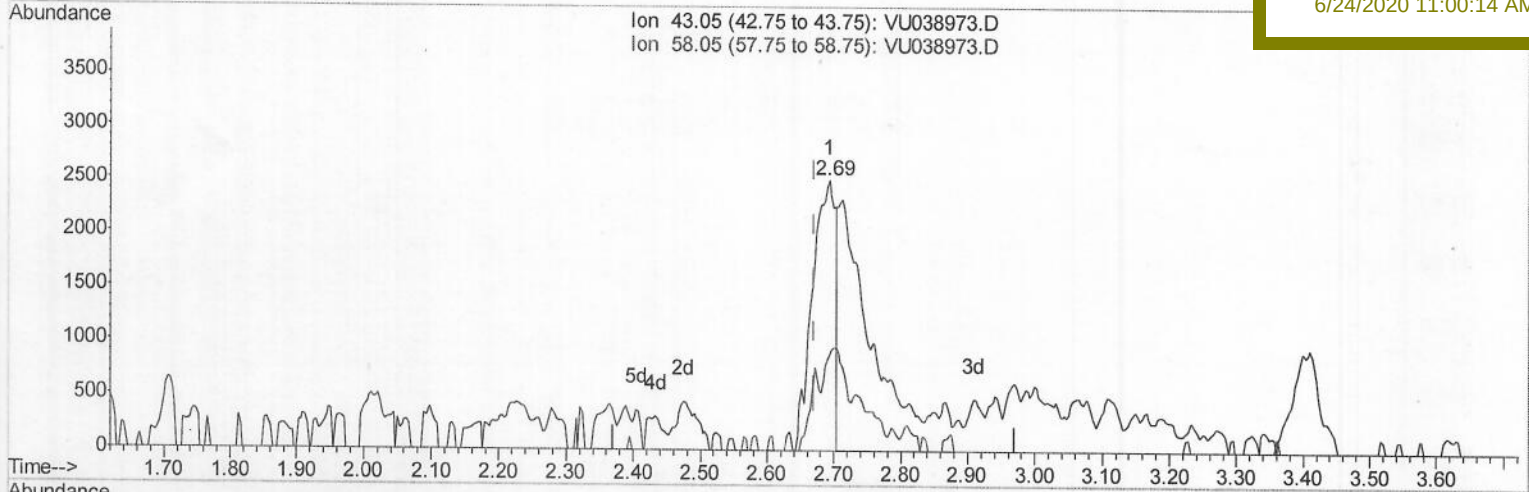
F9L38

Manual Integrations

APPROVED

MMDadoda

6/24/2020 11:00:14 AM



TIC: VU038973.D

(13) Acetone (T)

2.694min (+0.022) 1.51ug/L

response 5937

Ion	Exp%	Act%
43.05	100	100
58.05	32.50	34.61
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\

Data File : VU038973.D

Acq On : 18 Jun 2020 16:27

Operator : SY/MD

Sample : L3058-07

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 01:20:41 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Fri Jun 19 01:17:22 2020

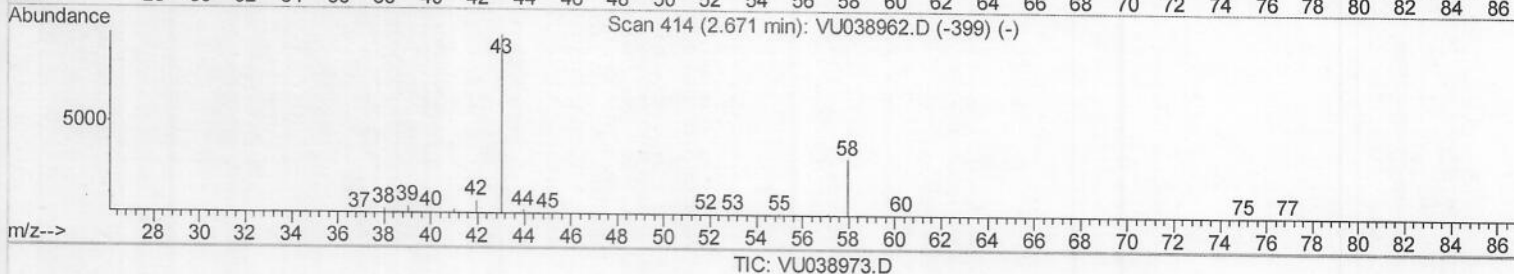
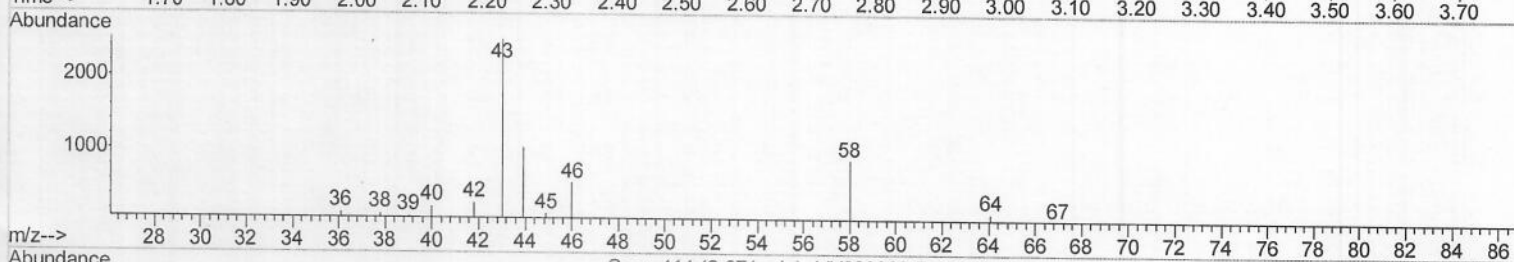
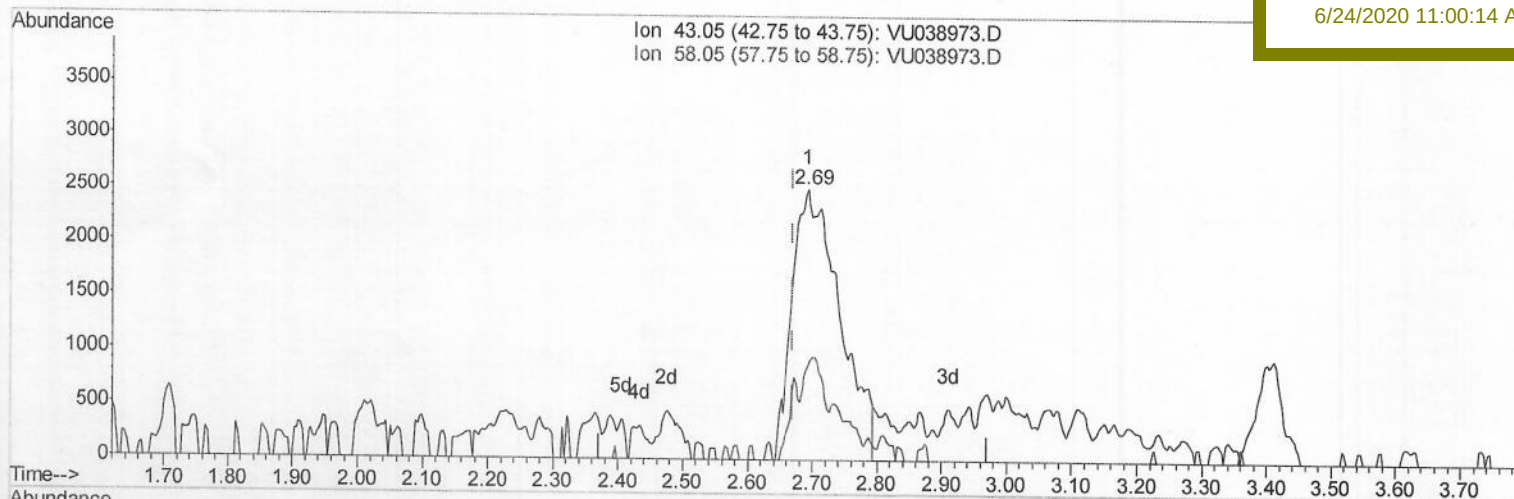
Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :

F9L38

Manual Integrations
APPROVEDMMDadoda
6/24/2020 11:00:14 AM

(13) Acetone (T)

2.694min (+0.022) 3.26ug/L m> Sy 06/24/20

response 12829

Ion	Exp%	Act%
43.05	100	100
58.05	32.50	16.02
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\
 Data File : VU038973.D
 Acq On : 18 Jun 2020 16:27
 Operator : SY/MD
 Sample : L3058-07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 02:18:44 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 19 01:17:22 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_U
 Client Sampled :
 F9L38

Manual Integrations
 APPROVED

MMDadoda
 6/24/2020 11:00:14 AM

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.28	114	259822	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	268477	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	125531	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	75045	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.93	69	76754	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.20%
11) 1,1-Dichloroethene-d2	2.59	63	133263	3.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.80%
20) 2-Butanone-d5	4.69	46	355853	61.65	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	123.30%
24) Chloroform-d	5.10	84	180676	5.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.80%
26) 1,2-Dichloroethane-d4	5.74	65	109673	5.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.00%
32) Benzene-d6	5.76	84	343891	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.72	67	109709	5.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.20%
41) Toluene-d8	7.92	98	270129	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.80%
43) trans-1,3-Dichloropropene-	8.20	79	44907	4.52	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.40%
46) 2-Hexanone-d5	8.66	63	283947	54.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	108.44%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	109250	5.35	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	118744	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%

Target Compounds

Target Compounds	R.T.	QI on	Response	Conc	Units	Ovalue
13) Acetone	2.69	43	12829mb	3.261	ug/L	
17) Methyl tert-butyl Ether	3.40	73	12098	0.252	ug/L #	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed