

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\
 Data File : VU038968.D
 Acq On : 18 Jun 2020 14:32
 Operator : SY/MD
 Sample : L3058-02
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9L29

Quant Time: Jun 19 01:54:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 19 01:17:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	263577	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	273988	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	130326	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	77560	4.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.80%
7) Chloroethane-d5	1.93	69	74150	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.40%
11) 1,1-Dichloroethene-d2	2.59	63	133585	3.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.00%
20) 2-Butanone-d5	4.67	46	247859	42.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	84.66%
24) Chloroform-d	5.10	84	188240	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.60%
26) 1,2-Dichloroethane-d4	5.74	65	108623	5.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.60%
32) Benzene-d6	5.76	84	353381	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
36) 1,2-Dichloropropane-d6	6.72	67	154442	6.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	139.40%
41) Toluene-d8	7.92	98	284617	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
43) trans-1,3-Dichloropropene-	8.20	79	44190	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.65	63	257023	48.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.18%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	100228	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	12.20	152	128982	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.67	43	13057	3.272 ug/L	95
14) Carbon disulfide	2.82	76	9767	0.156 ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\
Data File : VU038968.D
Acq On : 18 Jun 2020 14:32
Operator : SY/MD
Sample : L3058-02
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9L29

Quant Time: Jun 19 01:54:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 19 01:17:22 2020
Response via : Initial Calibration

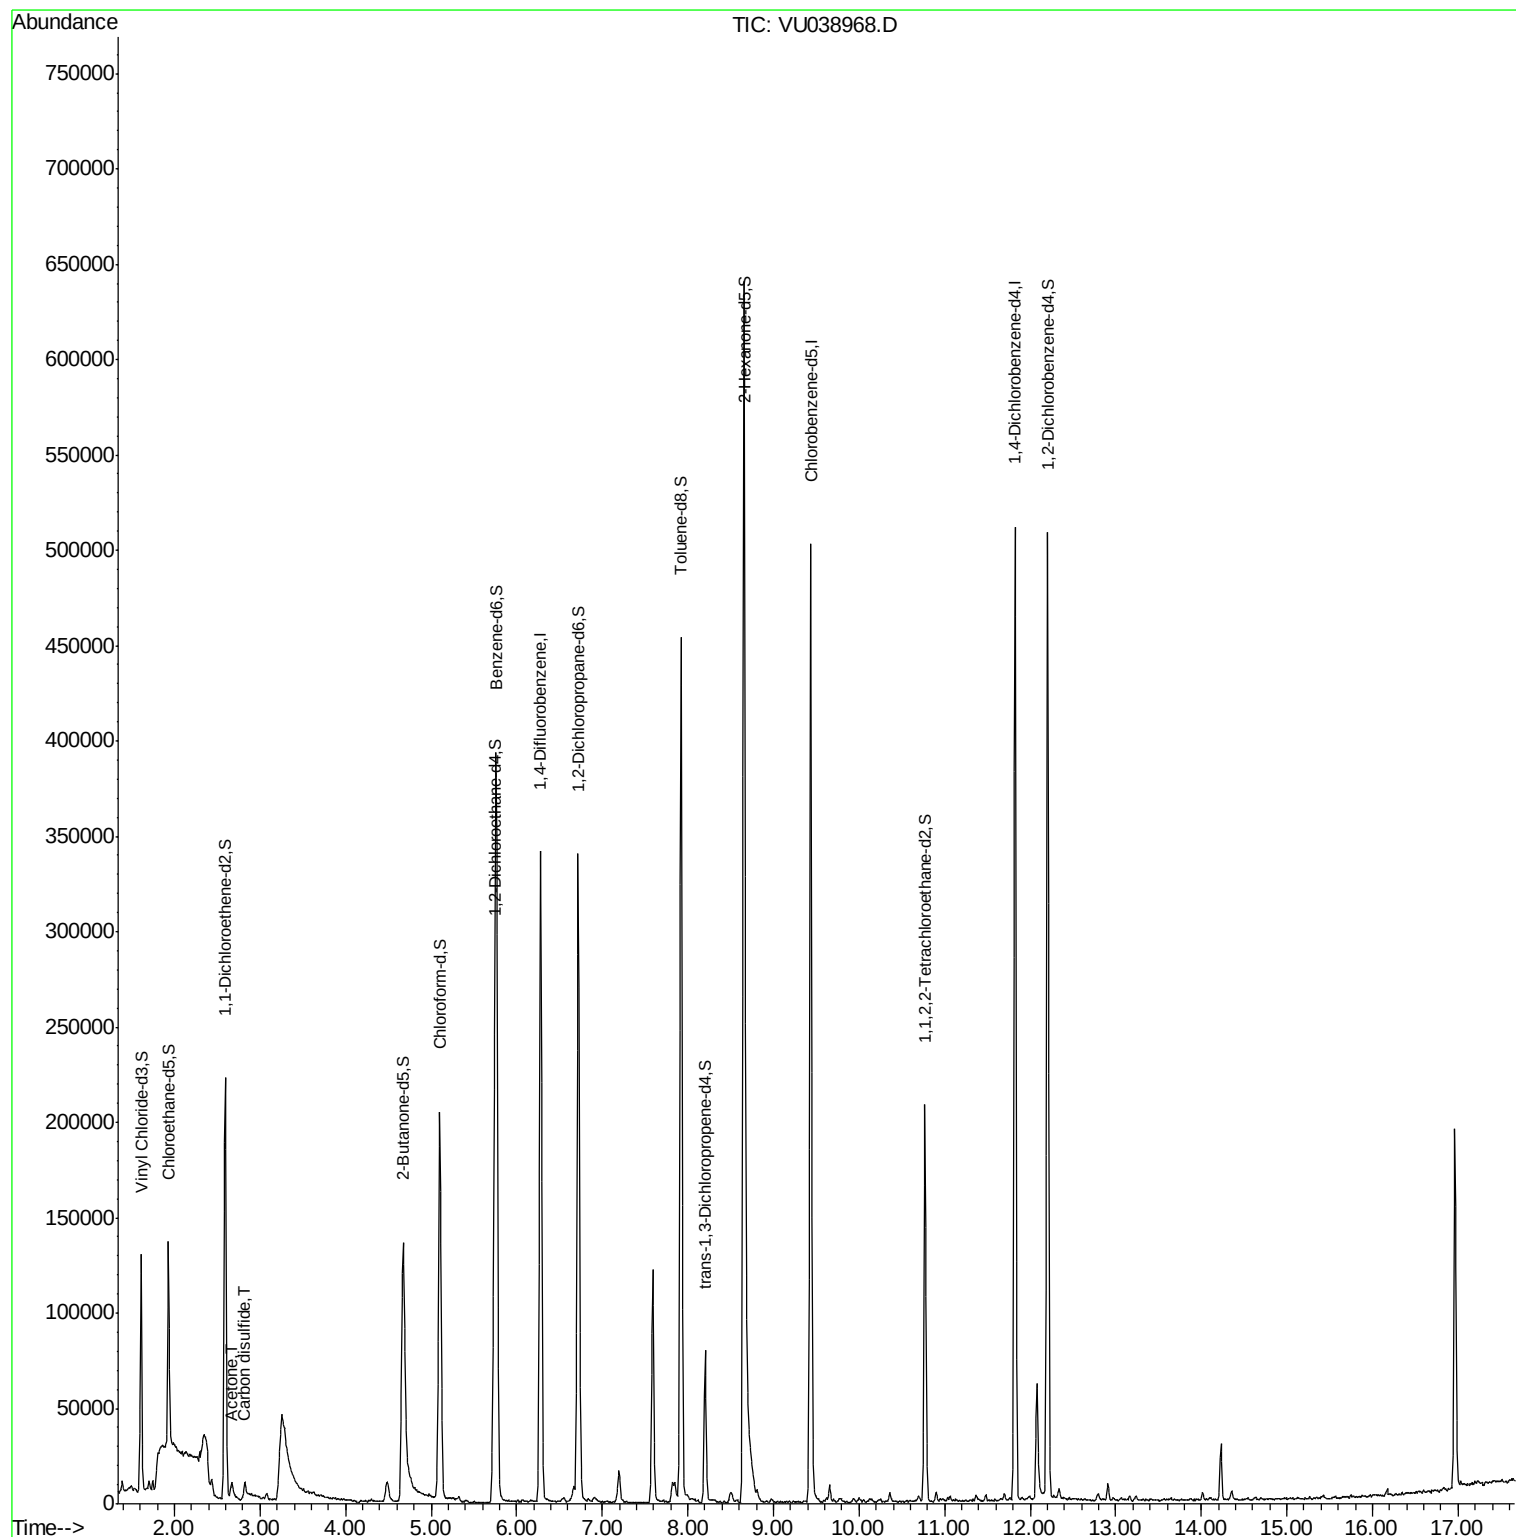

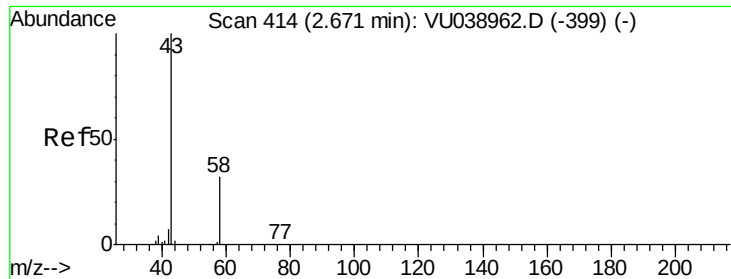

#13

Acetone

Concen: 3.272 ug/L

RT: 2.67 min Scan# 414

Delta R.T. -0.00 min

Lab File: VU038968.D

Acq: 18 Jun 2020 14:32

Instrument :

MSVOA_U

ClientSampleId :


F9L29

Tot Ion: 43 Resp: 13057




Ion Ratio Lower Upper

43 100

58 35.4 0.0 65.0

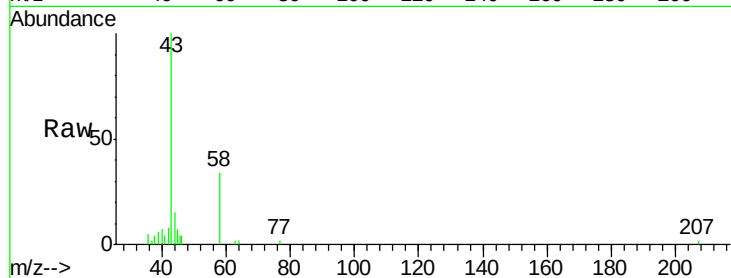

Abundance Ion 43.05 (42.75 to 43.75): VU038968.D (-321) (-)

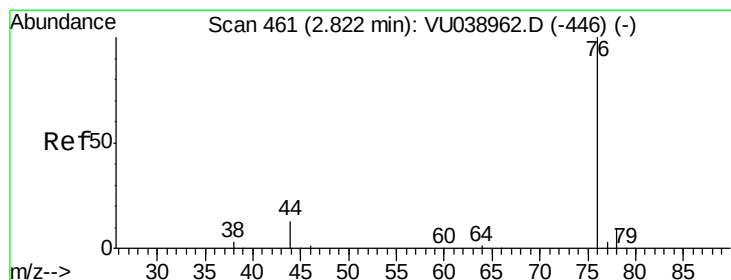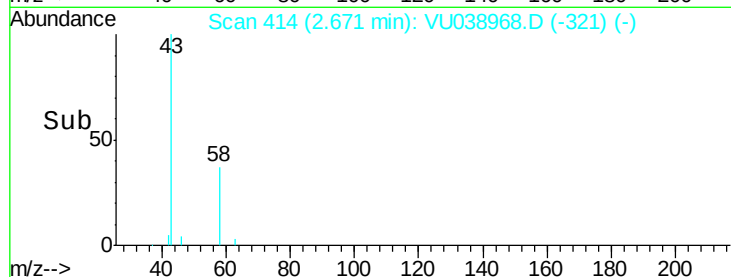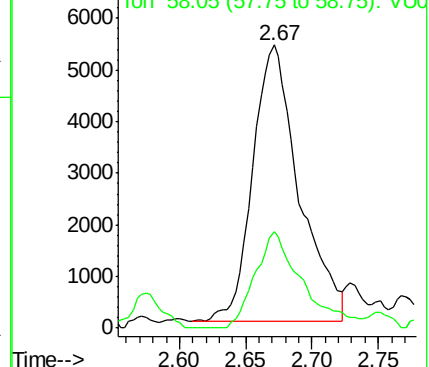

#14

Carbon disulfide

Concen: 0.156 ug/L

RT: 2.82 min Scan# 461

Delta R.T. -0.00 min

Lab File: VU038968.D


Acq: 18 Jun 2020 14:32

Tgt Ion: 76 Resp: 9767

Ion Ratio Lower Upper

76 100

78 12.3 7.4 11.0#

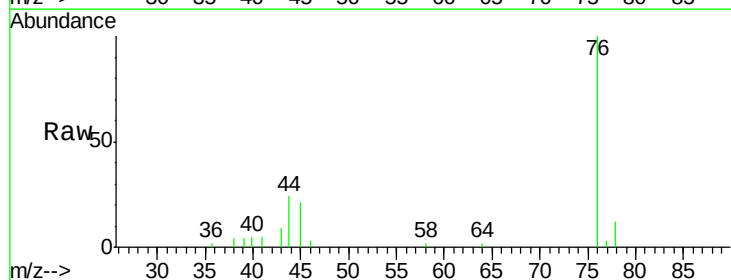

Abundance Ion 76.05 (75.75 to 76.75): VU038968.D (-368) (-)

