

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\
 Data File : VU038978.D
 Acq On : 18 Jun 2020 18:23
 Operator : SY/MD
 Sample : L3058-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9L44

Quant Time: Jun 19 02:38:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 19 01:17:22 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	255602	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	270694	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	122559	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	76655	4.32	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.40%
7) Chloroethane-d5	1.93	69	72825	4.88	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.60%
11) 1,1-Dichloroethene-d2	2.59	63	129091	3.59	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.80%
20) 2-Butanone-d5	4.67	46	435420	76.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	153.36%#
24) Chloroform-d	5.10	84	183727	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.20%
26) 1,2-Dichloroethane-d4	5.74	65	111380	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.60%
32) Benzene-d6	5.76	84	341617	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.72	67	110260	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.92	98	274342	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
43) trans-1,3-Dichloropropene-	8.20	79	45872	4.58	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.60%
46) 2-Hexanone-d5	8.66	63	281764	53.36	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.72%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	136916	6.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	133.00%#
64) 1,2-Dichlorobenzene-d4	12.20	152	120786	5.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.40%


Target Compounds					Ovalue
13) Acetone	2.68	43	7242	1.871 ug/L	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061820\
Data File : VU038978.D
Acq On : 18 Jun 2020 18:23
Operator : SY/MD
Sample : L3058-12
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9L44

Quant Time: Jun 19 02:38:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 19 01:17:22 2020
Response via : Initial Calibration

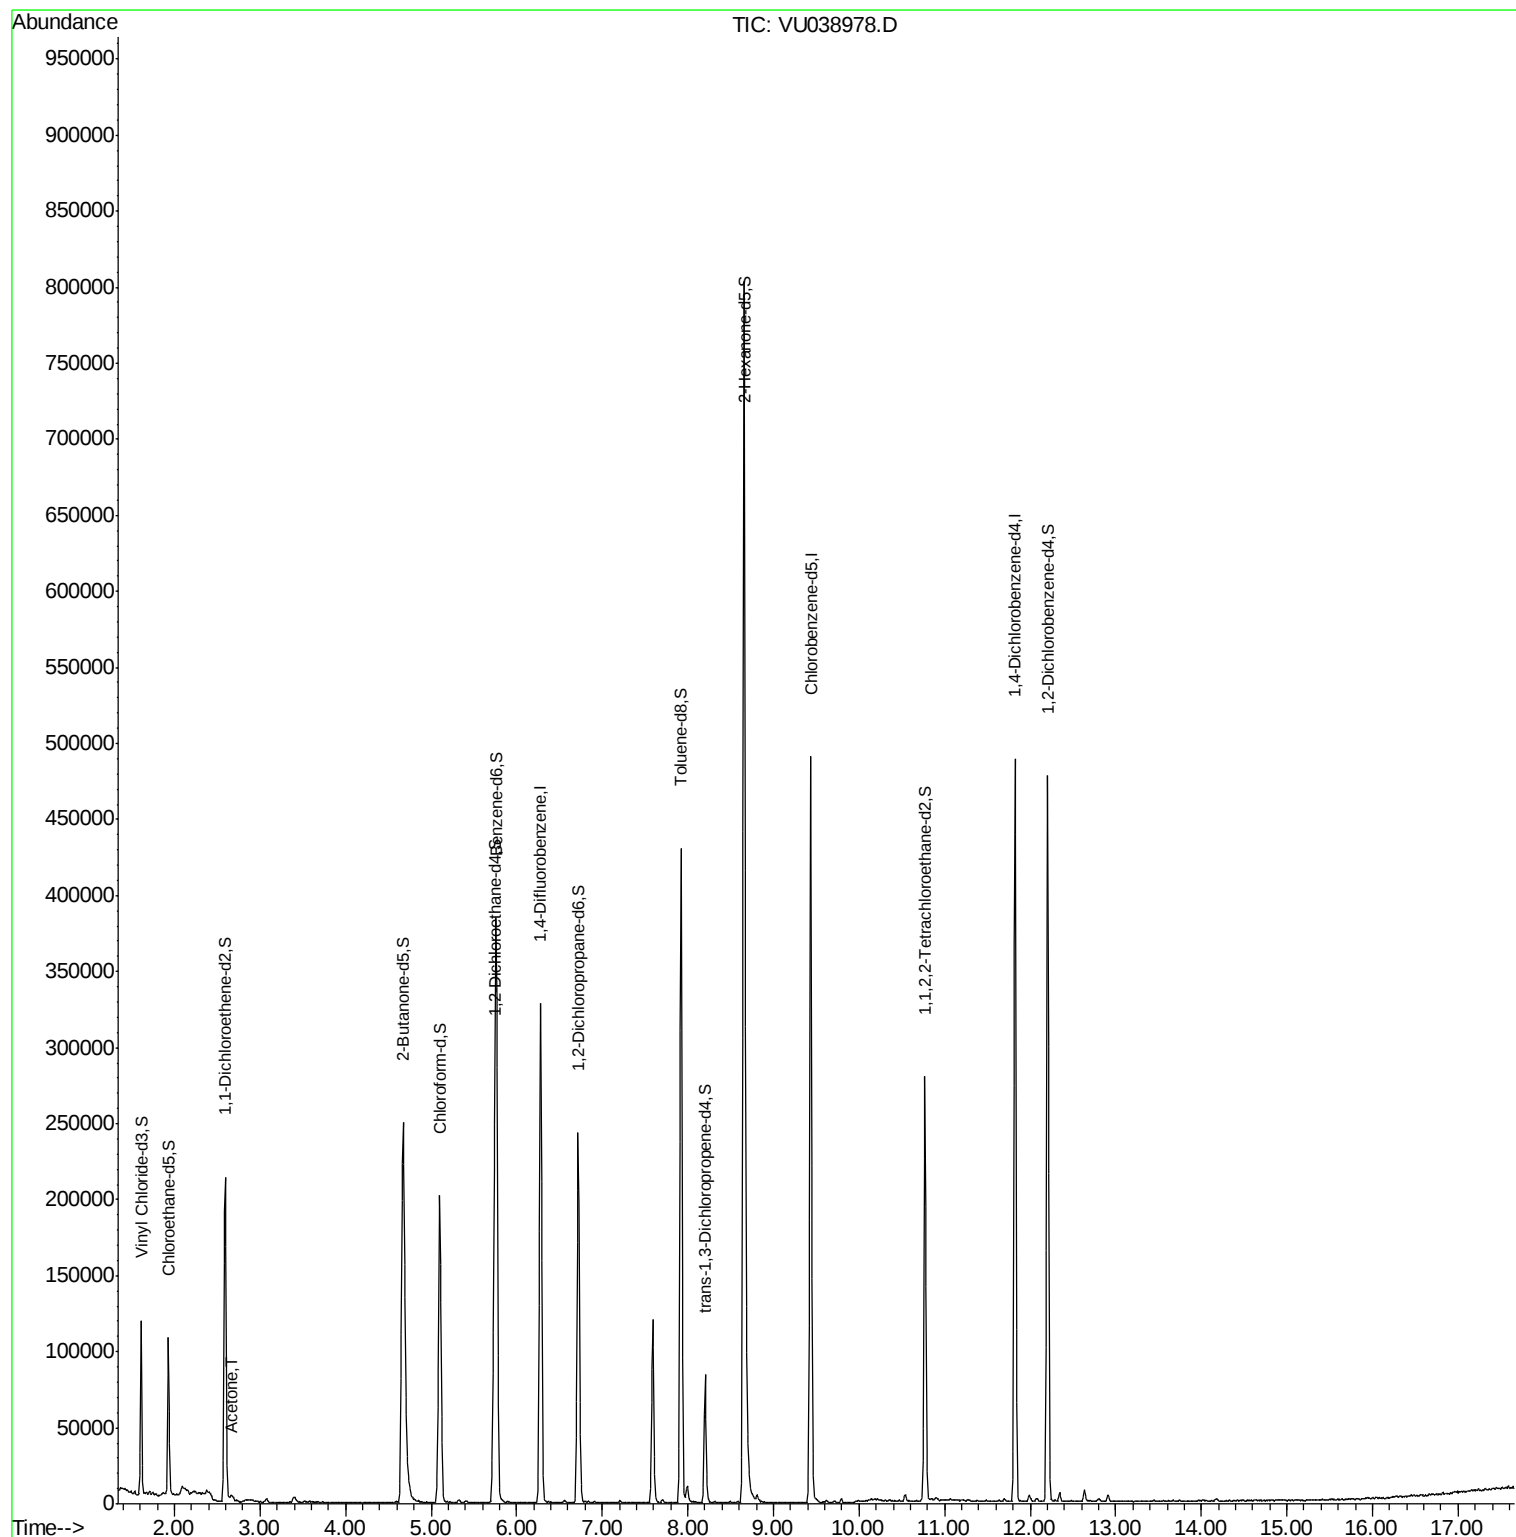

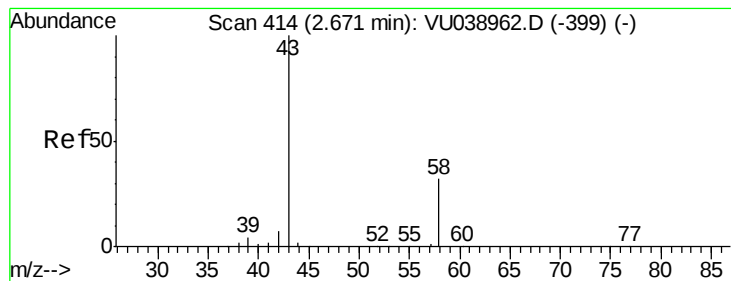

#13
 Acetone
 Concen: 1.871 ug/L
 RT: 2.68 min Scan# 416
 Delta R.T. 0.01 min
 Lab File: VU038978.D
 Acq: 18 Jun 2020 18:23

Instrument :
 MSVOA_U
 ClientSampleId :
 F9L44

Tot Ion: 43 Resp: 7242
 Ion Ratio Lower Upper
 43 100
 58 18.3 0.0 65.0

