


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061820\
 Data File : VU038961.D
 Acq On : 18 Jun 2020 09:29
 Operator : SY/MD
 Sample : BFB16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB16

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jun 19 01:17:22 2020

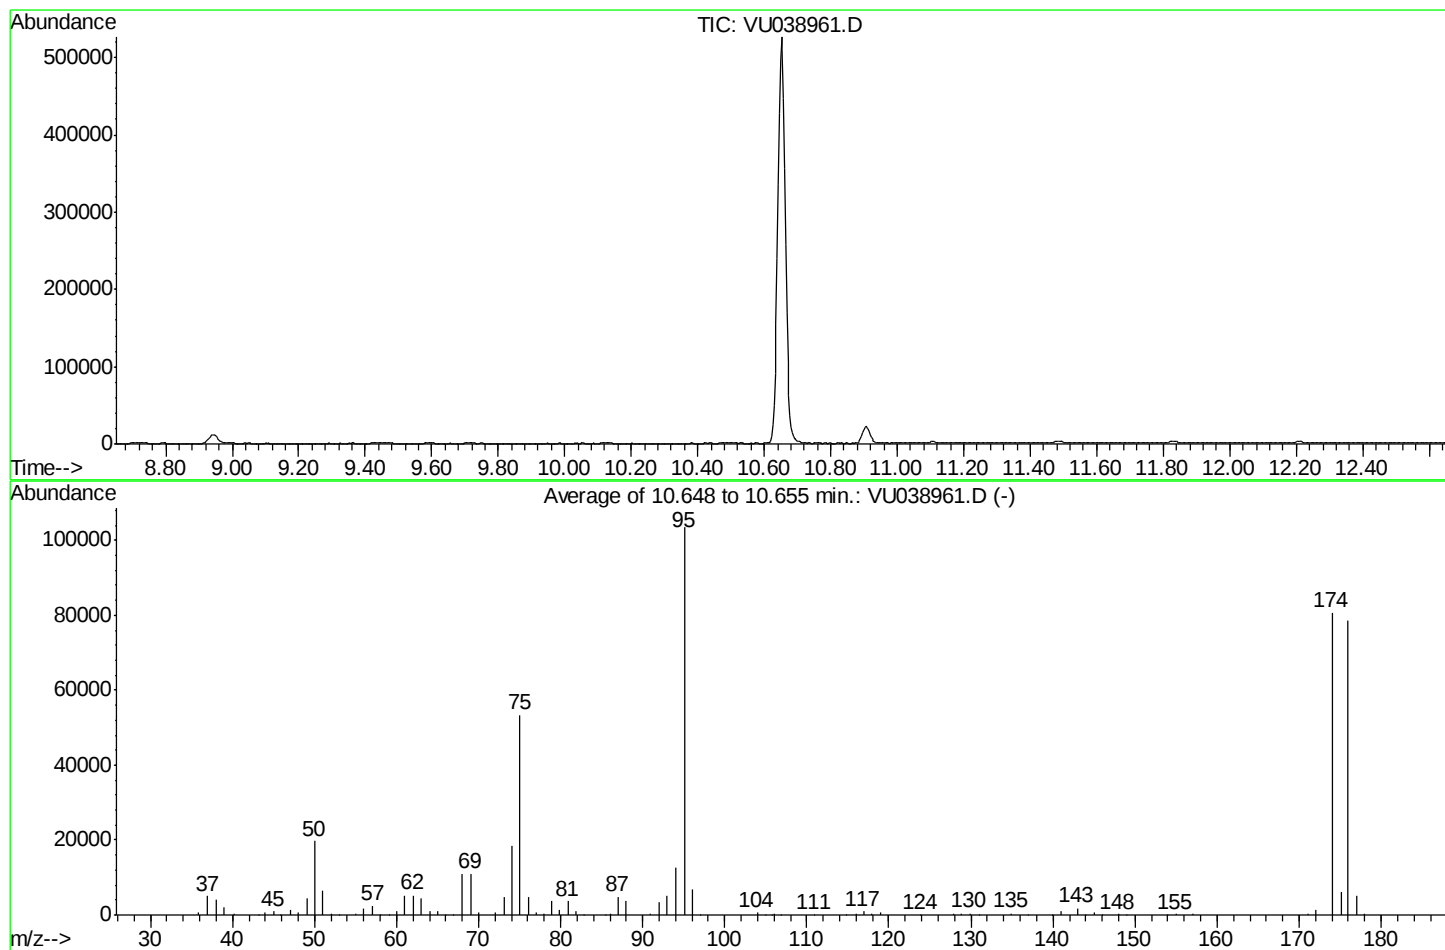

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	19696	PASS
75	95	30	80	51.5	53296	PASS
95	95	100	100	100.0	103453	PASS
96	95	5	9	6.7	6964	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.0	80645	PASS
175	174	5	9	7.7	6203	PASS
176	174	95	101	97.3	78496	PASS
177	176	5	9	6.6	5174	PASS

m/z	Abundance
35.90	694.0
37.00	4985.0
38.00	4300.0
39.00	2062.0
40.20	289.0
43.10	125.0
44.00	1597.0
45.00	929.0
45.80	113.0
47.00	1073.0
48.00	741.0
49.00	4470.0
50.00	19272.0
51.00	6946.0
52.10	433.0
53.10	152.0
55.00	278.0
56.00	1590.0
57.10	2628.0
58.00	126.0
60.00	994.0
61.00	5117.0
62.00	5457.0
63.00	4549.0
64.00	898.0
65.00	1188.0
66.00	138.0
68.00	11008.0
69.00	11129.0
70.00	797.0
72.00	733.0
73.10	4759.0
74.00	18104.0
75.00	52128.0
76.00	4734.0
76.90	581.0
78.00	499.0
78.90	3689.0
79.90	1531.0
80.90	3682.0
81.90	926.0
82.80	123.0
86.00	184.0
87.00	4769.0
88.00	3545.0
90.90	407.0
92.00	3265.0
93.00	4968.0
94.10	12158.0
95.10	99928.0
96.10	7056.0
104.00	507.0
105.00	128.0
105.80	373.0
106.70	163.0
110.90	112.0
114.90	121.0
116.00	461.0
116.90	877.0
117.90	425.0
118.90	556.0
128.00	304.0
128.90	269.0
129.90	351.0
131.00	191.0
135.00	325.0
141.00	1115.0
143.00	1816.0
144.00	174.0
145.00	568.0
148.00	193.0
148.90	144.0
155.00	300.0
157.00	174.0
171.10	309.0
172.10	1267.0
174.00	77744.0
175.10	6257.0
176.00	74648.0
177.00	5066.0
177.90	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
35.90	771.0
37.00	5359.0
38.00	4395.0
39.00	2031.0
40.20	299.0
43.10	183.0
44.00	1574.0
45.00	936.0
45.90	104.0
47.00	1296.0
48.10	830.0
49.00	4583.0
50.00	20184.0
51.00	6881.0
52.10	351.0
53.00	164.0
55.10	301.0
56.00	1868.0
57.10	2605.0
58.00	131.0
60.00	950.0
61.00	5172.0
62.00	5420.0
63.00	4509.0
64.00	921.0
65.10	1216.0
66.00	141.0
68.00	11196.0
69.00	11254.0
70.00	887.0
72.00	747.0
73.10	5098.0
74.00	19056.0
75.00	54784.0
76.00	5045.0
76.90	657.0
78.00	544.0
78.90	4048.0
79.90	1550.0
80.90	3865.0
81.90	918.0
82.80	167.0
85.40	109.0
86.00	189.0
87.00	5011.0
88.00	3962.0
90.90	453.0
92.00	3449.0
93.00	5206.0
94.10	13067.0
95.10	106960.0
96.10	7201.0
104.00	571.0
104.90	147.0
106.00	374.0
106.70	148.0
114.80	143.0
116.00	511.0
116.90	971.0
117.90	501.0
118.90	553.0
123.90	104.0
127.90	324.0
128.80	243.0
129.90	475.0
131.00	181.0
135.00	379.0
136.90	184.0
141.00	1178.0
143.00	1885.0
143.90	171.0
145.00	521.0
146.00	105.0
148.00	214.0
149.00	168.0
154.00	119.0
155.00	283.0
157.00	218.0
171.10	301.0
172.10	1546.0
174.00	82784.0
175.10	6287.0
176.00	80912.0
177.00	5305.0
178.00	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

m/z	Abundance
35.90	746.0
37.00	5023.0
38.00	4106.0
38.90	1904.0
39.90	317.0
43.10	196.0
43.90	1291.0
45.00	813.0
45.90	105.0
47.00	1368.0
48.10	697.0
49.10	4273.0
50.00	19632.0
51.00	6181.0
52.10	226.0
53.00	202.0
55.10	328.0
55.90	1882.0
57.10	2445.0
59.10	102.0
60.00	897.0
61.00	4999.0
62.00	4976.0
63.00	4033.0
64.00	798.0
65.10	1191.0
65.90	134.0
66.90	343.0
68.00	10300.0
69.00	10443.0
70.00	829.0
72.00	631.0
73.00	4886.0
74.00	18376.0
75.00	52976.0
76.10	4836.0
77.00	751.0
78.00	500.0
78.90	3934.0
79.90	1363.0
80.90	3664.0
81.90	965.0
82.80	162.0
86.00	218.0
87.00	4647.0
88.00	3948.0
91.00	466.0
92.00	3319.0
93.00	4962.0
94.10	12749.0
95.10	103472.0
96.10	6637.0
97.00	105.0
104.00	516.0
105.00	178.0
106.00	418.0
106.80	117.0
114.80	134.0
115.90	553.0
116.90	977.0
117.90	506.0
119.00	541.0
123.90	147.0
127.90	347.0
128.80	179.0
129.90	565.0
131.00	152.0
134.90	380.0
136.90	271.0
139.90	138.0
141.00	1158.0
143.00	1681.0
143.90	109.0
145.00	484.0
146.00	132.0
148.00	203.0
149.00	133.0
154.00	131.0
155.00	309.0
157.10	188.0
171.00	254.0
172.10	1575.0
174.00	81408.0
175.10	6067.0
176.00	79928.0
177.00	5152.0
178.00	192.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16

Scan 2882 (10.607 min): VU038961.D
BFB16

m/z	Abundance
40.00	205.0
43.90	833.0

Instrument :
MSVOA_U
ClientSampleId :
BFB16