

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU061919\
 Data File : VU032870.D
 Acq On : 19 Jun 2019 20:06
 Operator : JC/SP
 Sample : K3413-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALF2

Quant Time: Jun 20 07:28:43 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 07:24:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	105641	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	102840	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	54179	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	30694	4.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.40%
7) Chloroethane-d5	1.68	69	26120	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	89.00%
11) 1,1-Dichloroethene-d2	2.27	63	50647	3.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.60%
20) 2-Butanone-d5	4.18	46	115083	60.04	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.08%
24) Chloroform-d	4.64	84	67463	5.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	5.31	65	40568	6.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.20%
32) Benzene-d6	5.33	84	129913	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.60%
36) 1,2-Dichloropropane-d6	6.32	67	43289	5.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.00%
41) Toluene-d8	7.56	98	118603	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.40%
43) trans-1,3-Dichloropropene-	7.85	79	17228	5.12	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.40%
46) 2-Hexanone-d5	8.31	63	83628	49.56	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.12%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	36714	5.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.60%
64) 1,2-Dichlorobenzene-d4	11.85	152	52089	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%

Target Compounds


					Qvalue
8) Chloroethane	1.70	64	553	0.094 ug/L #	42
13) Acetone	2.32	43	3812	2.562 ug/L	96
14) Carbon disulfide	2.47	76	2982	0.139 ug/L #	77
17) Methyl tert-butyl Ether	3.00	73	69657	3.548 ug/L	97
35) Methylcyclohexane	6.32	83	10045	0.716 ug/L #	20
37) 1,2-Dichloropropane	6.32	63	5066	0.646 ug/L #	89
42) Toluene	7.63	91	25297	0.749 ug/L	93
47) Tetrachloroethene	8.22	164	9566	1.394 ug/L	96
48) 2-Hexanone	8.36	43	4929	1.235 ug/L #	93
49) Dibromochloromethane	8.22	129	8794	1.205 ug/L #	11
52) Ethylbenzene	9.25	91	5064	0.136 ug/L	100
53) m,p-Xylene	9.37	106	4357	0.309 ug/L	97
54) o-Xylene	9.77	106	1670	0.119 ug/L	76
59) 1,2,3-Trichloropropane	11.48	75	6706	1.302 ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU061919\
Data File : VU032870.D
Acq On : 19 Jun 2019 20:06
Operator : JC/SP
Sample : K3413-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALF2

Quant Time: Jun 20 07:28:43 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 07:24:34 2019
Response via : Initial Calibration




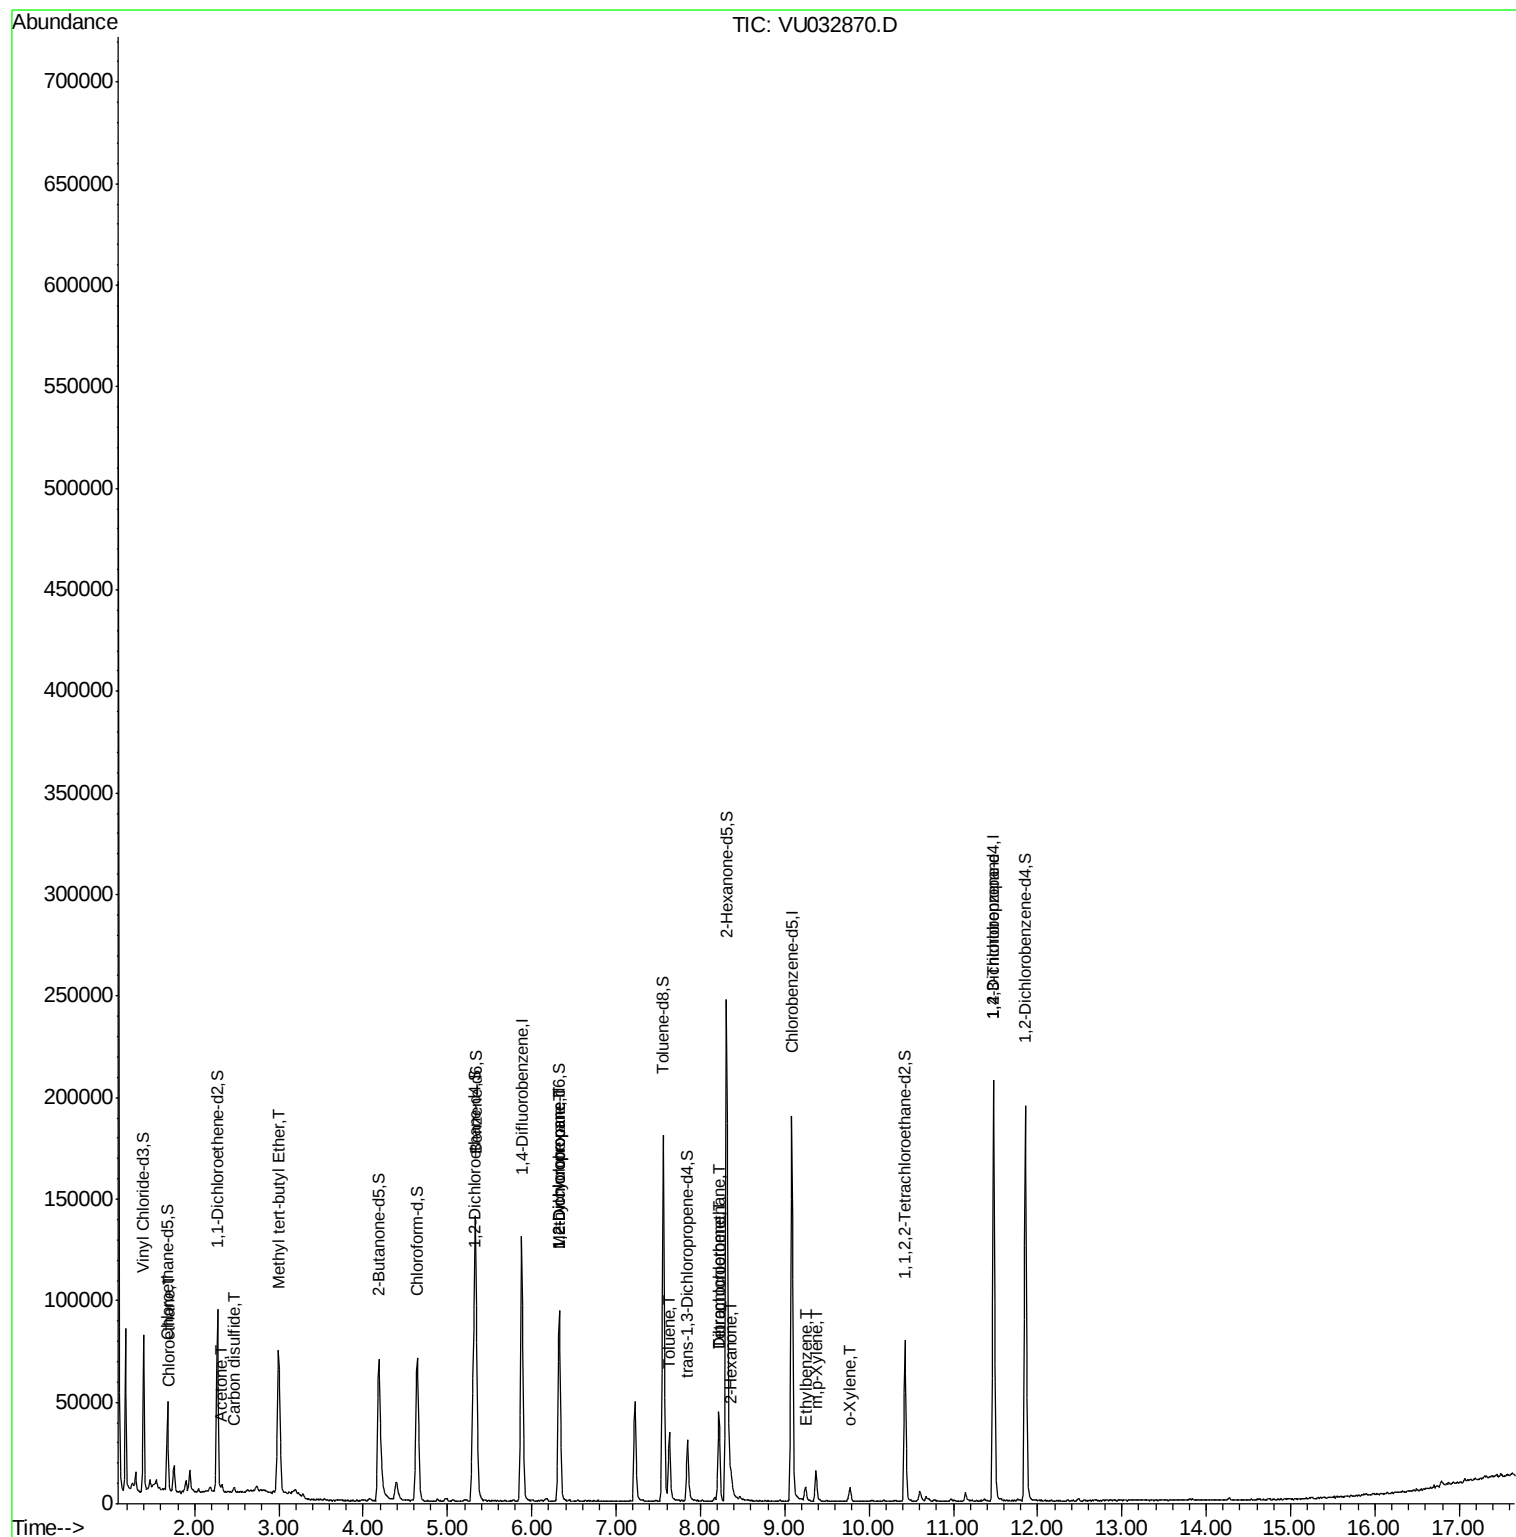


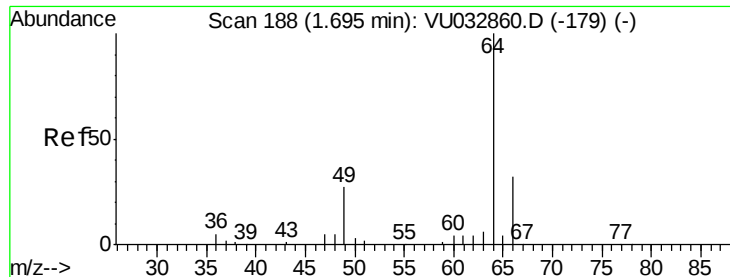

#8
Chloroethane
Concen: 0.094 ug/L
RT: 1.70 min Scan# 189
Delta R.T. 0.00 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06




Instrument :
MSVOA_U
ClientSampleId :
GALF2


Tgt Ion: 64 Resp: 553
Ion Ratio Lower Upper
64 100
66 0.0 22.8 42.4#

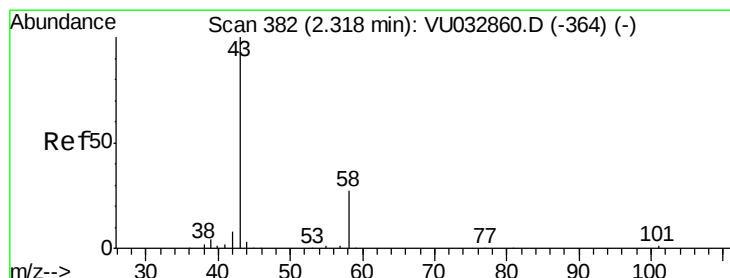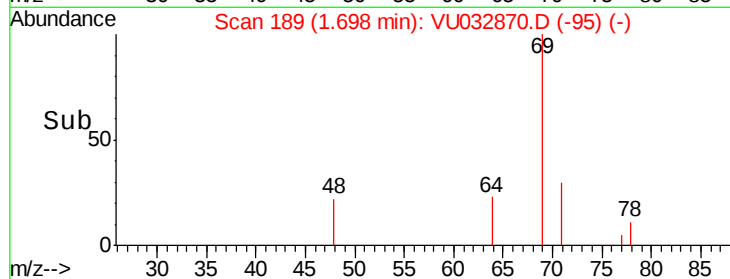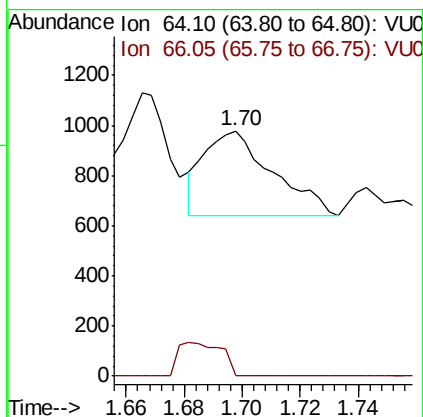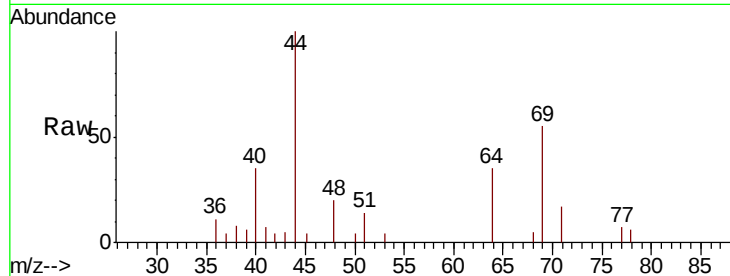

#13
Acetone
Concen: 2.562 ug/L
RT: 2.32 min Scan# 382
Delta R.T. -0.00 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06

Tgt Ion: 43 Resp: 3812
Ion Ratio Lower Upper
43 100
58 28.4 0.0 60.8

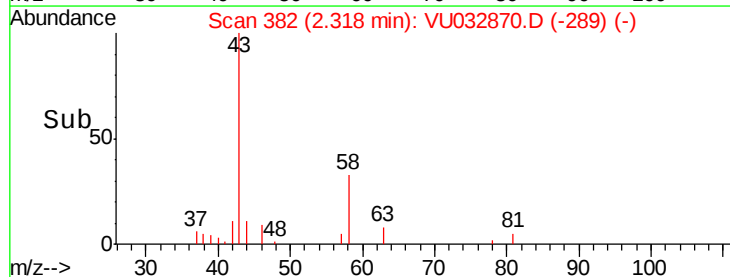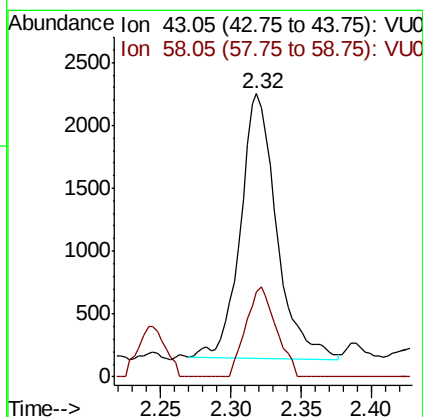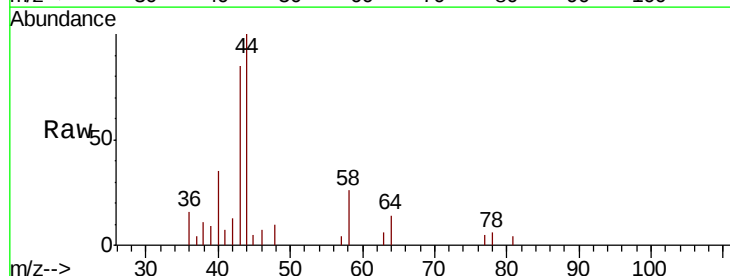

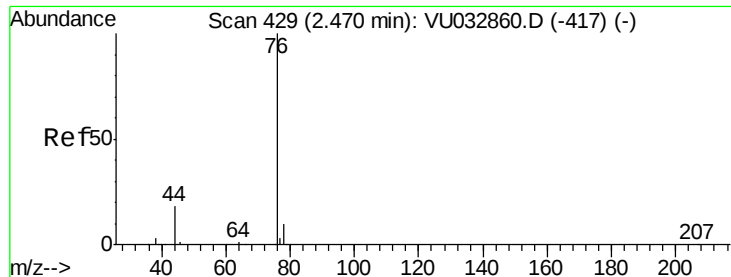

#14

Carbon disulfide

Concen: 0.139 ug/L

RT: 2.47 min Scan# 429

Delta R.T. -0.00 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06

Instrument :

MSVOA_U

ClientSampleId :


GALF2

Tgt Ion: 76 Resp: 2982

Ion Ratio Lower Upper




76 100

78 17.4 7.3 10.9#

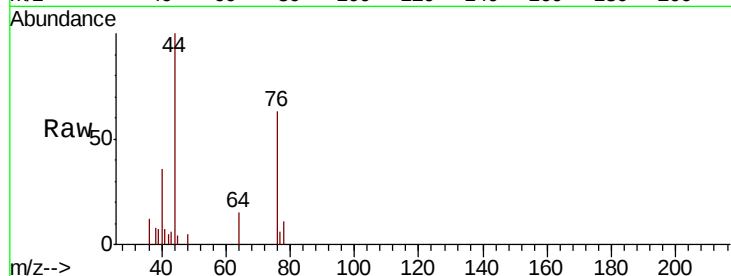

Abundance Ion 76.05 (75.75 to 76.75): VU032860.D (-417) (-)

Ion 78.00 (77.70 to 78.70): VU032860.D (-417) (-)

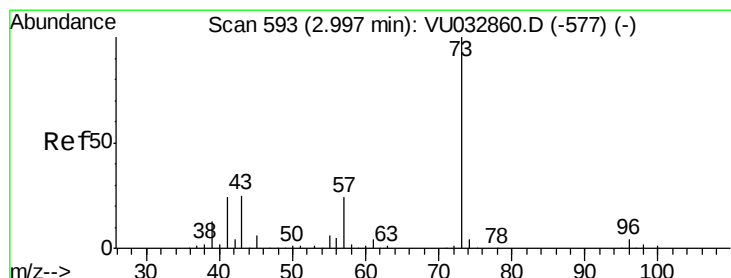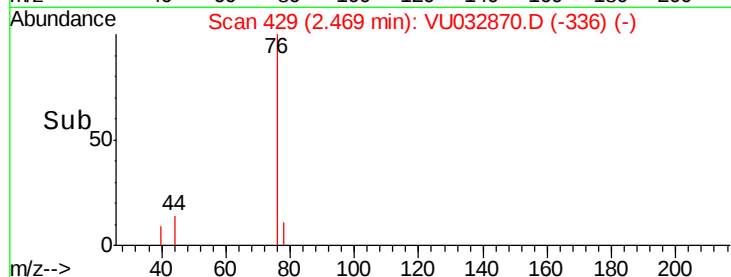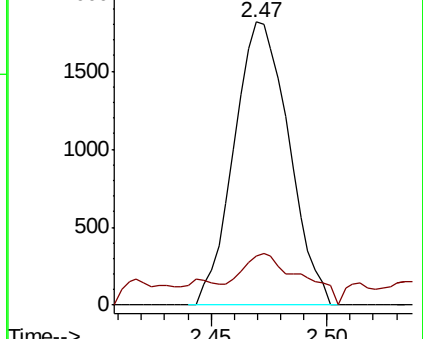

#17

Methyl tert-butyl Ether

Concen: 3.548 ug/L

RT: 3.00 min Scan# 594

Delta R.T. 0.00 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06


Tgt Ion: 73 Resp: 69657

Ion Ratio Lower Upper

73 100

43 24.8 18.6 27.8



57 24.3 18.3 27.5

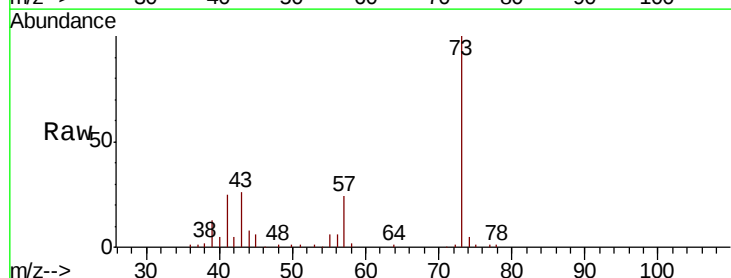


Abundance Ion 73.10 (72.80 to 73.80): VU032860.D (-577) (-)

Ion 43.05 (42.75 to 43.75): VU032860.D (-577) (-)

Ion 57.10 (56.80 to 57.80): VU032860.D (-577) (-)

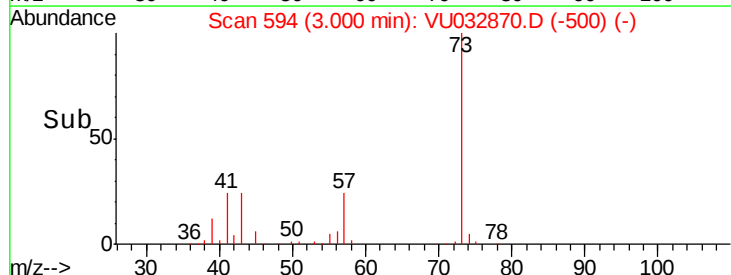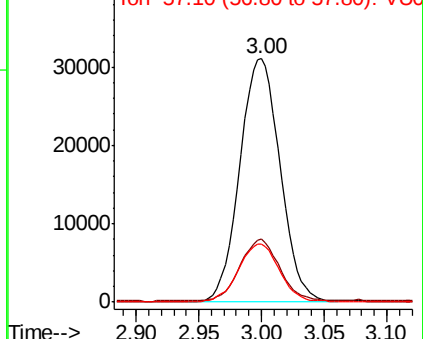

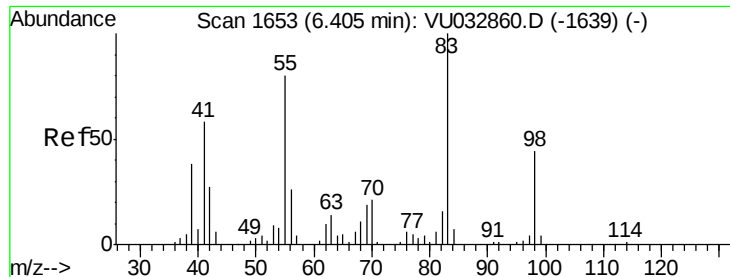

#35

Methylcyclohexane

Concen: 0.716 ug/L

RT: 6.32 min Scan# 1628

Delta R.T. -0.08 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06

Instrument :

MSVOA_U

ClientSampleId :

GALF2


Tgt Ion: 83 Resp: 10045

Ion Ratio Lower Upper

83 100

55 0.6 60.0 90.0#




98 0.8 37.8 56.8#

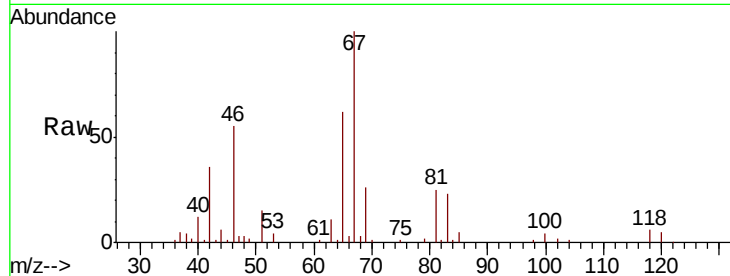

Abundance Ion 83.15 (82.85 to 83.85): VU0

Ion 55.10 (54.80 to 55.80): VU0

Ion 98.15 (97.85 to 98.85): VU0

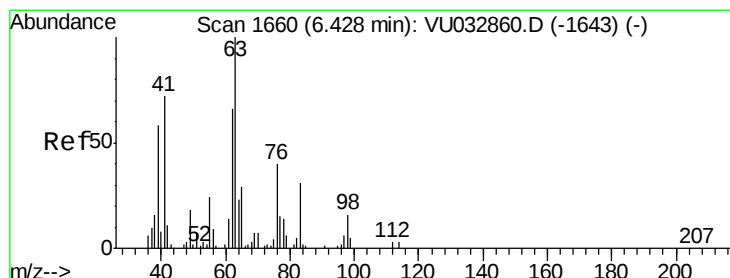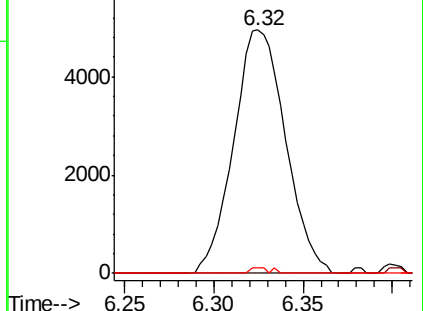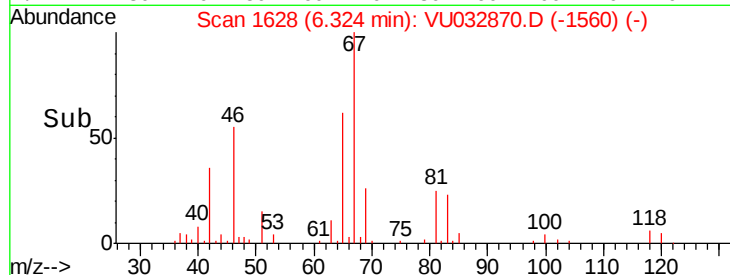

#37

1,2-Dichloropropane

Concen: 0.646 ug/L

RT: 6.32 min Scan# 1628

Delta R.T. -0.10 min

Lab File: VU032870.D


Acq: 19 Jun 2019 20:06

Tgt Ion: 63 Resp: 5066

Ion Ratio Lower Upper



63 100


112 0.0 2.9 4.3#

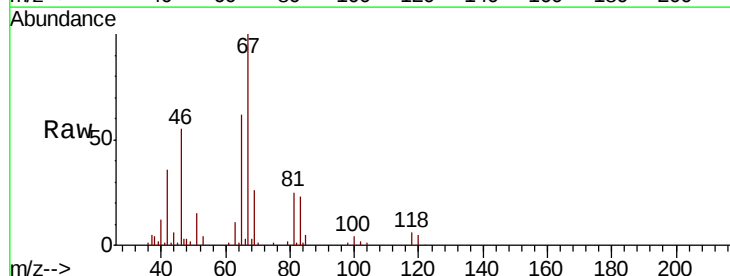

Abundance Ion 63.10 (62.80 to 63.80): VU0

Ion 112.10 (111.80 to 112.80): V

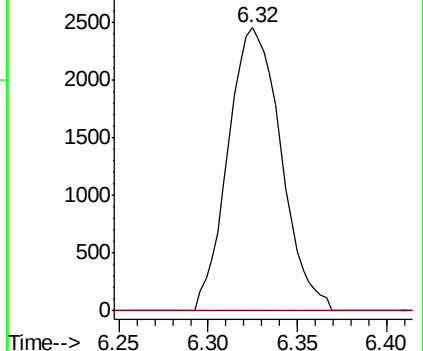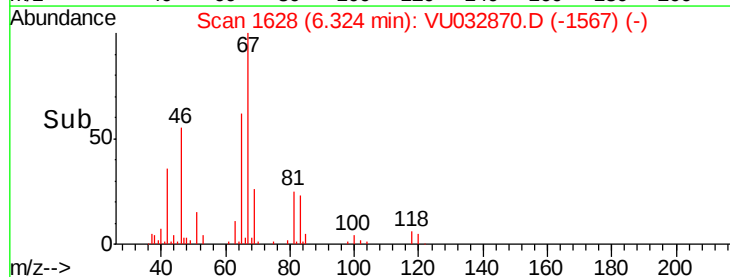

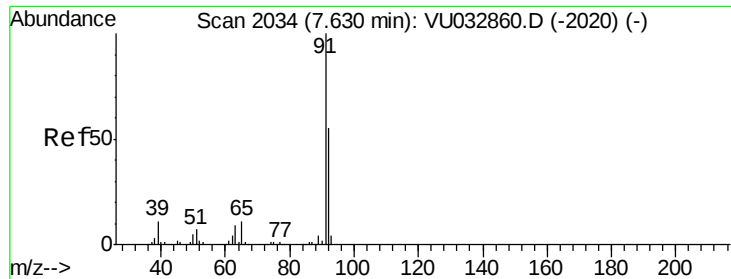

#42

Toluene

Concen: 0.749 ug/L

RT: 7.63 min Scan# 2034

Delta R.T. -0.00 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06

Instrument :

MSVOA_U

ClientSampleId :


GALF2

Tgt Ion: 91 Resp: 25297

Ion Ratio Lower Upper

91 100

92 53.5 40.9 75.9

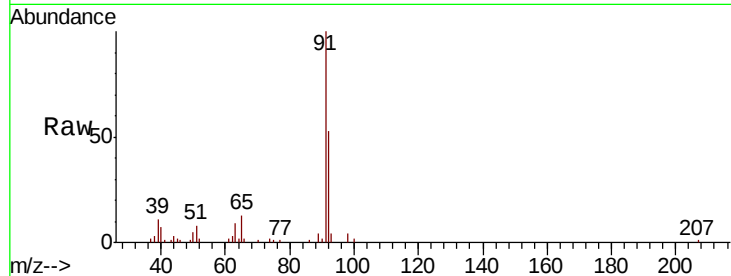

Abundance Ion 91.15 (90.85 to 91.85): VU032860.D (-2020) (-)

Ion 92.15 (91.85 to 92.85): VU032860.D (-2020) (-)

7.63

15000



10000

5000

0

Time-->

7.55 7.60 7.65 7.70

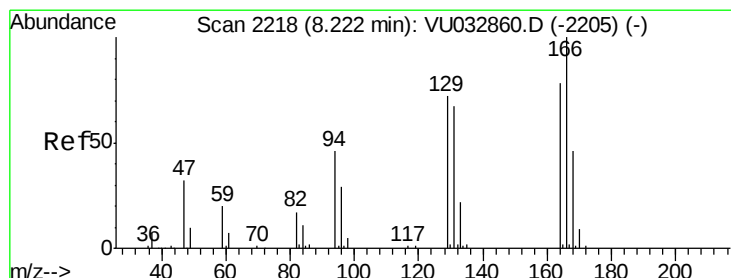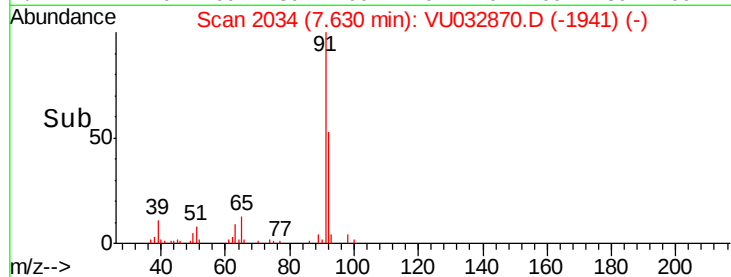

#47

Tetrachloroethene

Concen: 1.394 ug/L

RT: 8.22 min Scan# 2218

Delta R.T. -0.00 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06

Tgt Ion: 164 Resp: 9566


Ion Ratio Lower Upper

164 100

129 91.7 66.1 122.7

131 93.9 65.6 121.8

166 123.6 93.2 173.2

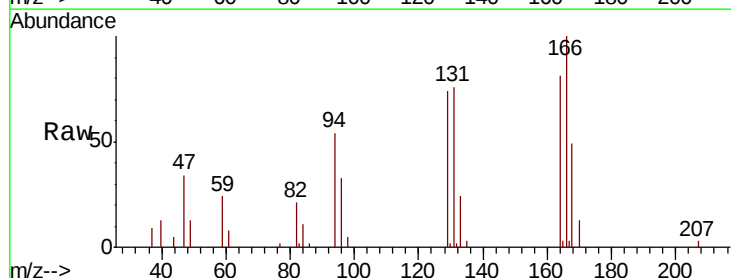

Abundance Ion 163.90 (163.60 to 164.60): VU032860.D (-2205) (-)

Ion 128.95 (128.65 to 129.65): VU032860.D (-2205) (-)

Ion 130.95 (130.65 to 131.65): VU032860.D (-2205) (-)

Ion 165.90 (165.60 to 166.60): VU032860.D (-2205) (-)

8.22

10000

8000

6000


4000


2000

0

Time-->

8.15 8.20 8.25




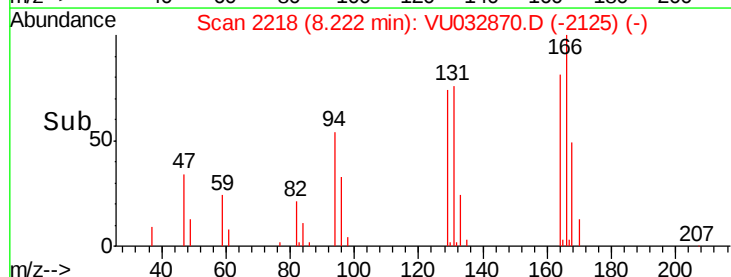


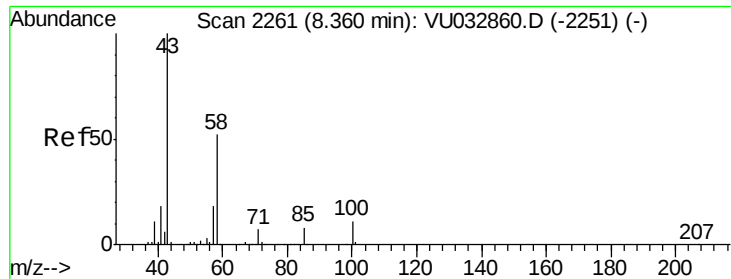

#48
2-Hexanone
Concen: 1.235 ug/L
RT: 8.36 min Scan# 2262
Delta R.T. 0.00 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06




Instrument :
MSVOA_U
ClientSampleId :
GALF2


Tgt Ion: 43 Resp: 4929
Ion Ratio Lower Upper
43 100
58 48.0 41.9 62.9
57 16.7 15.1 22.7
100 6.4 9.0 13.6#

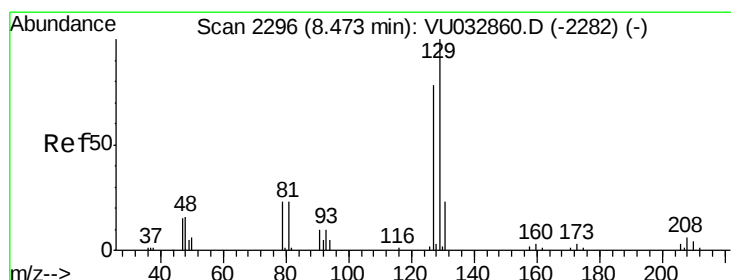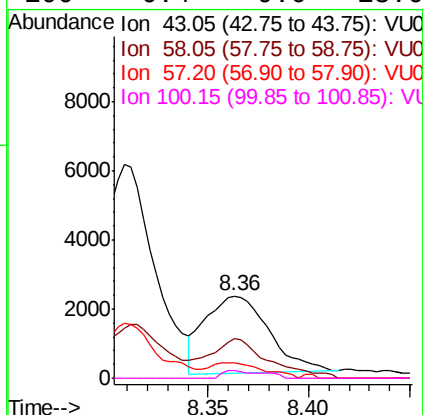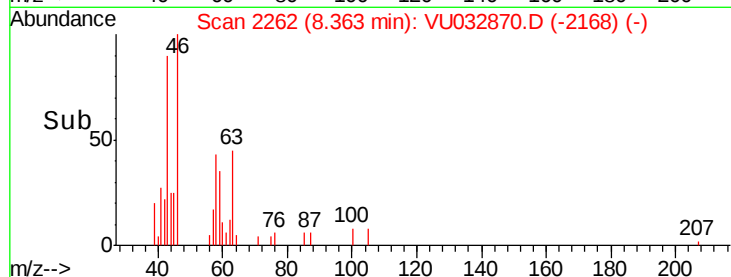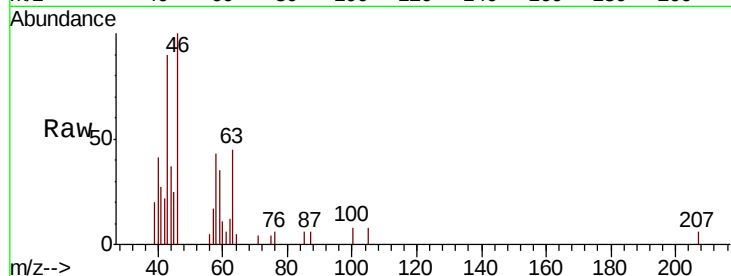

#49
Dibromochloromethane
Concen: 1.205 ug/L
RT: 8.22 min Scan# 2218
Delta R.T. -0.25 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06

Tgt Ion: 129 Resp: 8794
Ion Ratio Lower Upper
129 100
127 0.0 53.3 98.9#

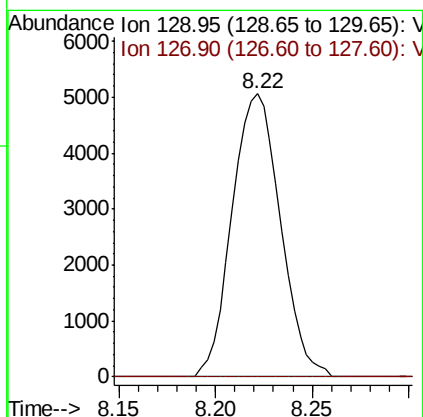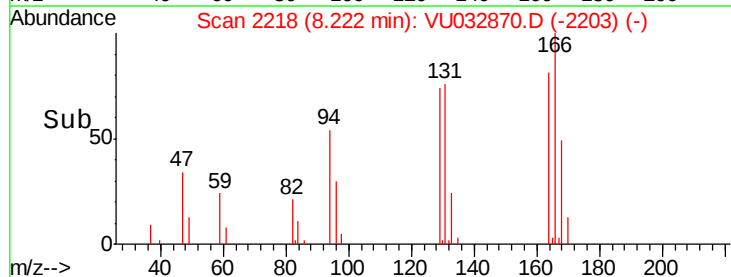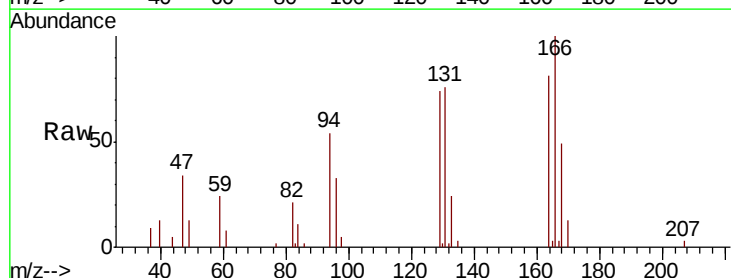

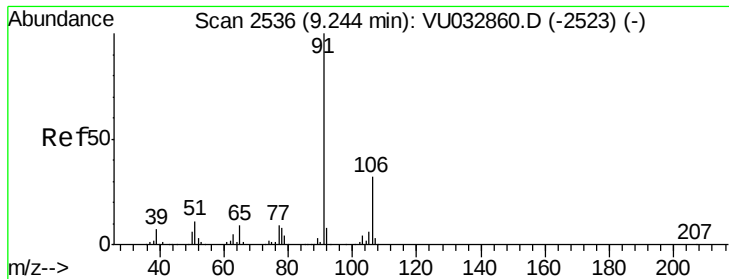

#52

Ethylbenzene

Concen: 0.136 ug/L

RT: 9.25 min Scan# 2537

Delta R.T. 0.00 min

Lab File: VU032870.D

Acq: 19 Jun 2019 20:06

Instrument :

MSVOA_U

ClientSampleId :


GALF2

Tgt Ion: 91 Resp: 5064




Ion Ratio Lower Upper

91 100

106 31.1 21.8 40.6

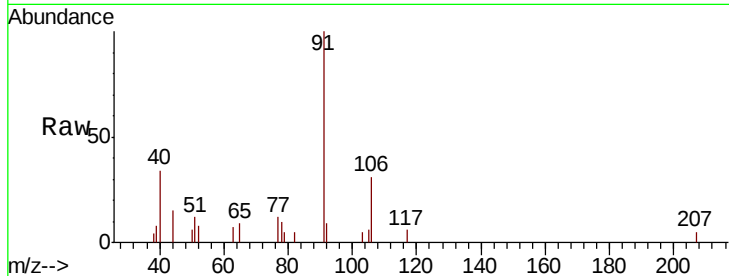

Abundance Ion 91.15 (90.85 to 91.85): VU032860.D (-2523) (-)

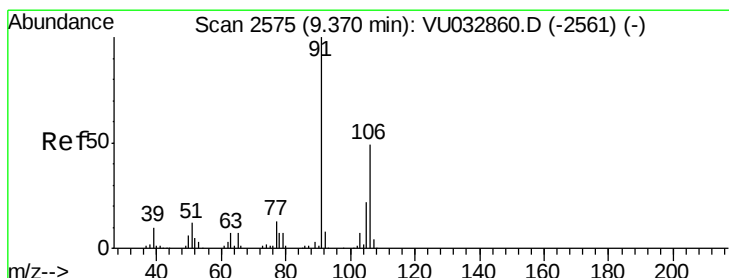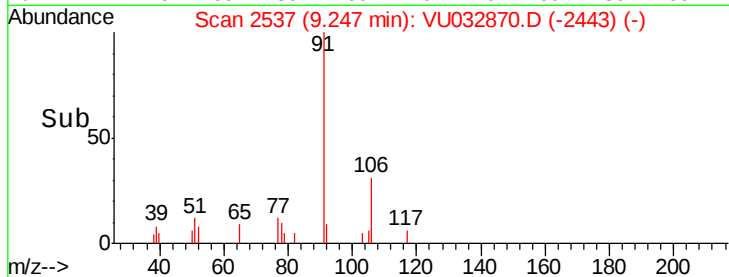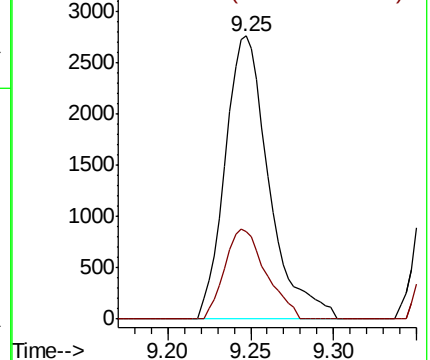

#53

m,p-Xylene

Concen: 0.309 ug/L

RT: 9.37 min Scan# 2576

Delta R.T. 0.00 min

Lab File: VU032870.D


Acq: 19 Jun 2019 20:06

Tgt Ion: 106 Resp: 4357



Ion Ratio Lower Upper


106 100

91 198.3 142.4 264.4

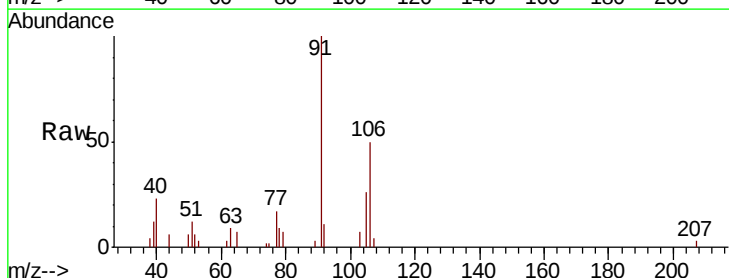

Abundance Ion 106.15 (105.85 to 106.85): VU032860.D (-2561) (-)

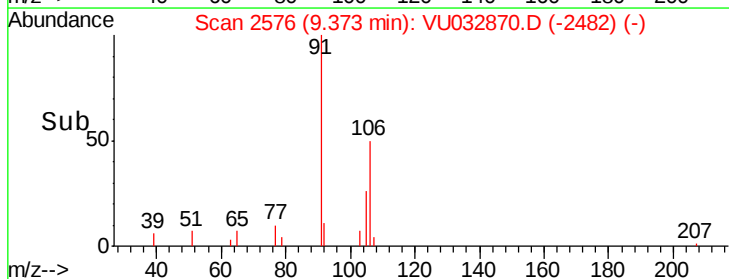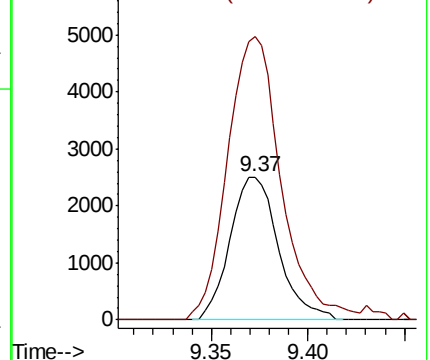


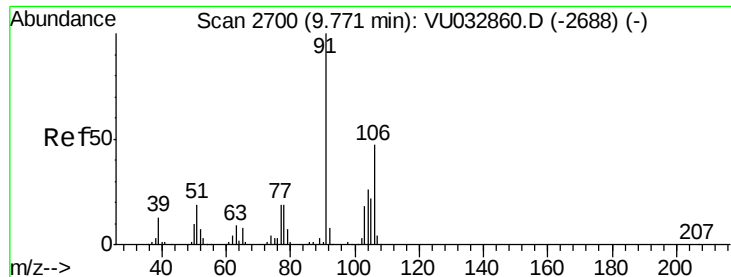




#54
o-Xylene
Concen: 0.119 ug/L
RT: 9.77 min Scan# 2701
Delta R.T. 0.00 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06

Instrument :
MSVOA_U
ClientSampled :
GALF2

Tgt Ion: 106 Resp: 1670
Ion Ratio Lower Upper
106 100
91 250.5 148.8 276.4

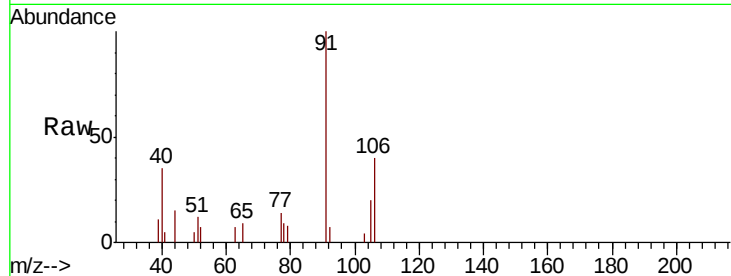


Abundance Ion 106.15 (105.85 to 106.85): VU032870.D (-2607) (-)
Ion 91.15 (90.85 to 91.85): VU032870.D (-2607) (-)

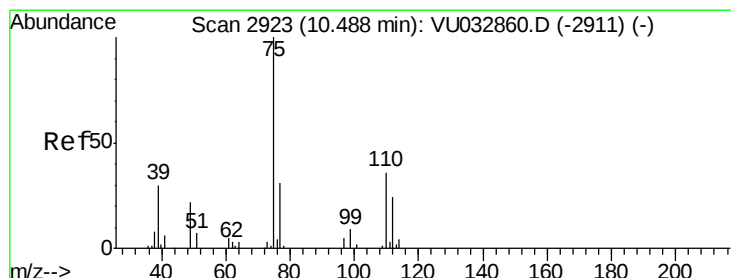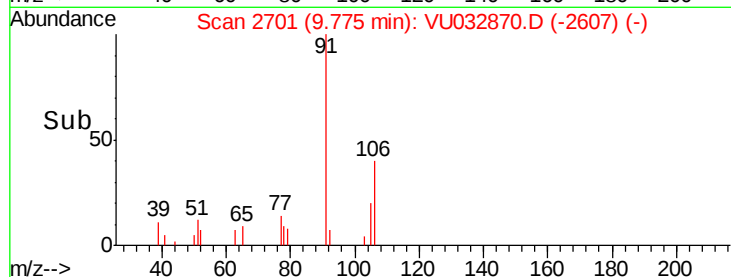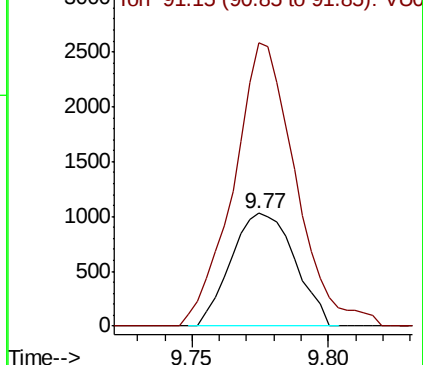

#59
1,2,3-Trichloropropane
Concen: 1.302 ug/L
RT: 11.48 min Scan# 3231
Delta R.T. 0.99 min
Lab File: VU032870.D
Acq: 19 Jun 2019 20:06

Tgt Ion: 75 Resp: 6706
Ion Ratio Lower Upper
75 100
77 38.1 25.3 37.9#

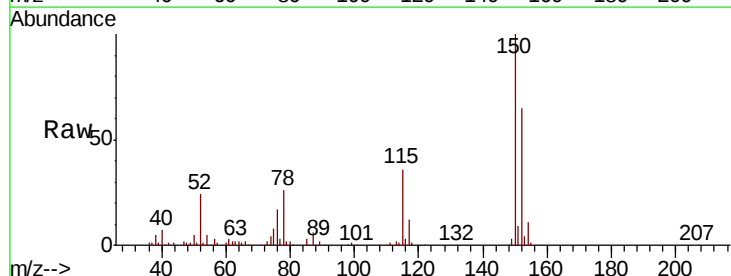

Abundance Ion 75.00 (74.70 to 75.70): VU032870.D (-2301) (-)
Ion 77.00 (76.70 to 77.70): VU032870.D (-2301) (-)

