

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061919\
 Data File : VU032846.D
 Acq On : 19 Jun 2019 10:22
 Operator : JC/SP
 Sample : K3413-25
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALH1

Quant Time: Jun 20 05:52:10 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 05:14:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	96815	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	94227	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	48786	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	29604	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.68	69	24682	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.27	63	47369	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	4.18	46	97870	55.71	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.42%
24) Chloroform-d	4.64	84	60420	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.20%
26) 1,2-Dichloroethane-d4	5.30	65	35883	6.09	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	121.80%
32) Benzene-d6	5.33	84	118466	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.32	67	38180	5.29	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.80%
41) Toluene-d8	7.56	98	108407	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
43) trans-1,3-Dichloropropene-	7.85	79	15534	5.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.60%
46) 2-Hexanone-d5	8.31	63	69511	44.96	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.92%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	31733	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.20%
64) 1,2-Dichlorobenzene-d4	11.85	152	46985	5.35	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	107.00%


Target Compounds				Ovalue
13) Acetone	2.32	43	19115	14.019 ug/L 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061919\
Data File : VU032846.D
Acq On : 19 Jun 2019 10:22
Operator : JC/SP
Sample : K3413-25
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALH1

Quant Time: Jun 20 05:52:10 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 05:14:15 2019
Response via : Initial Calibration

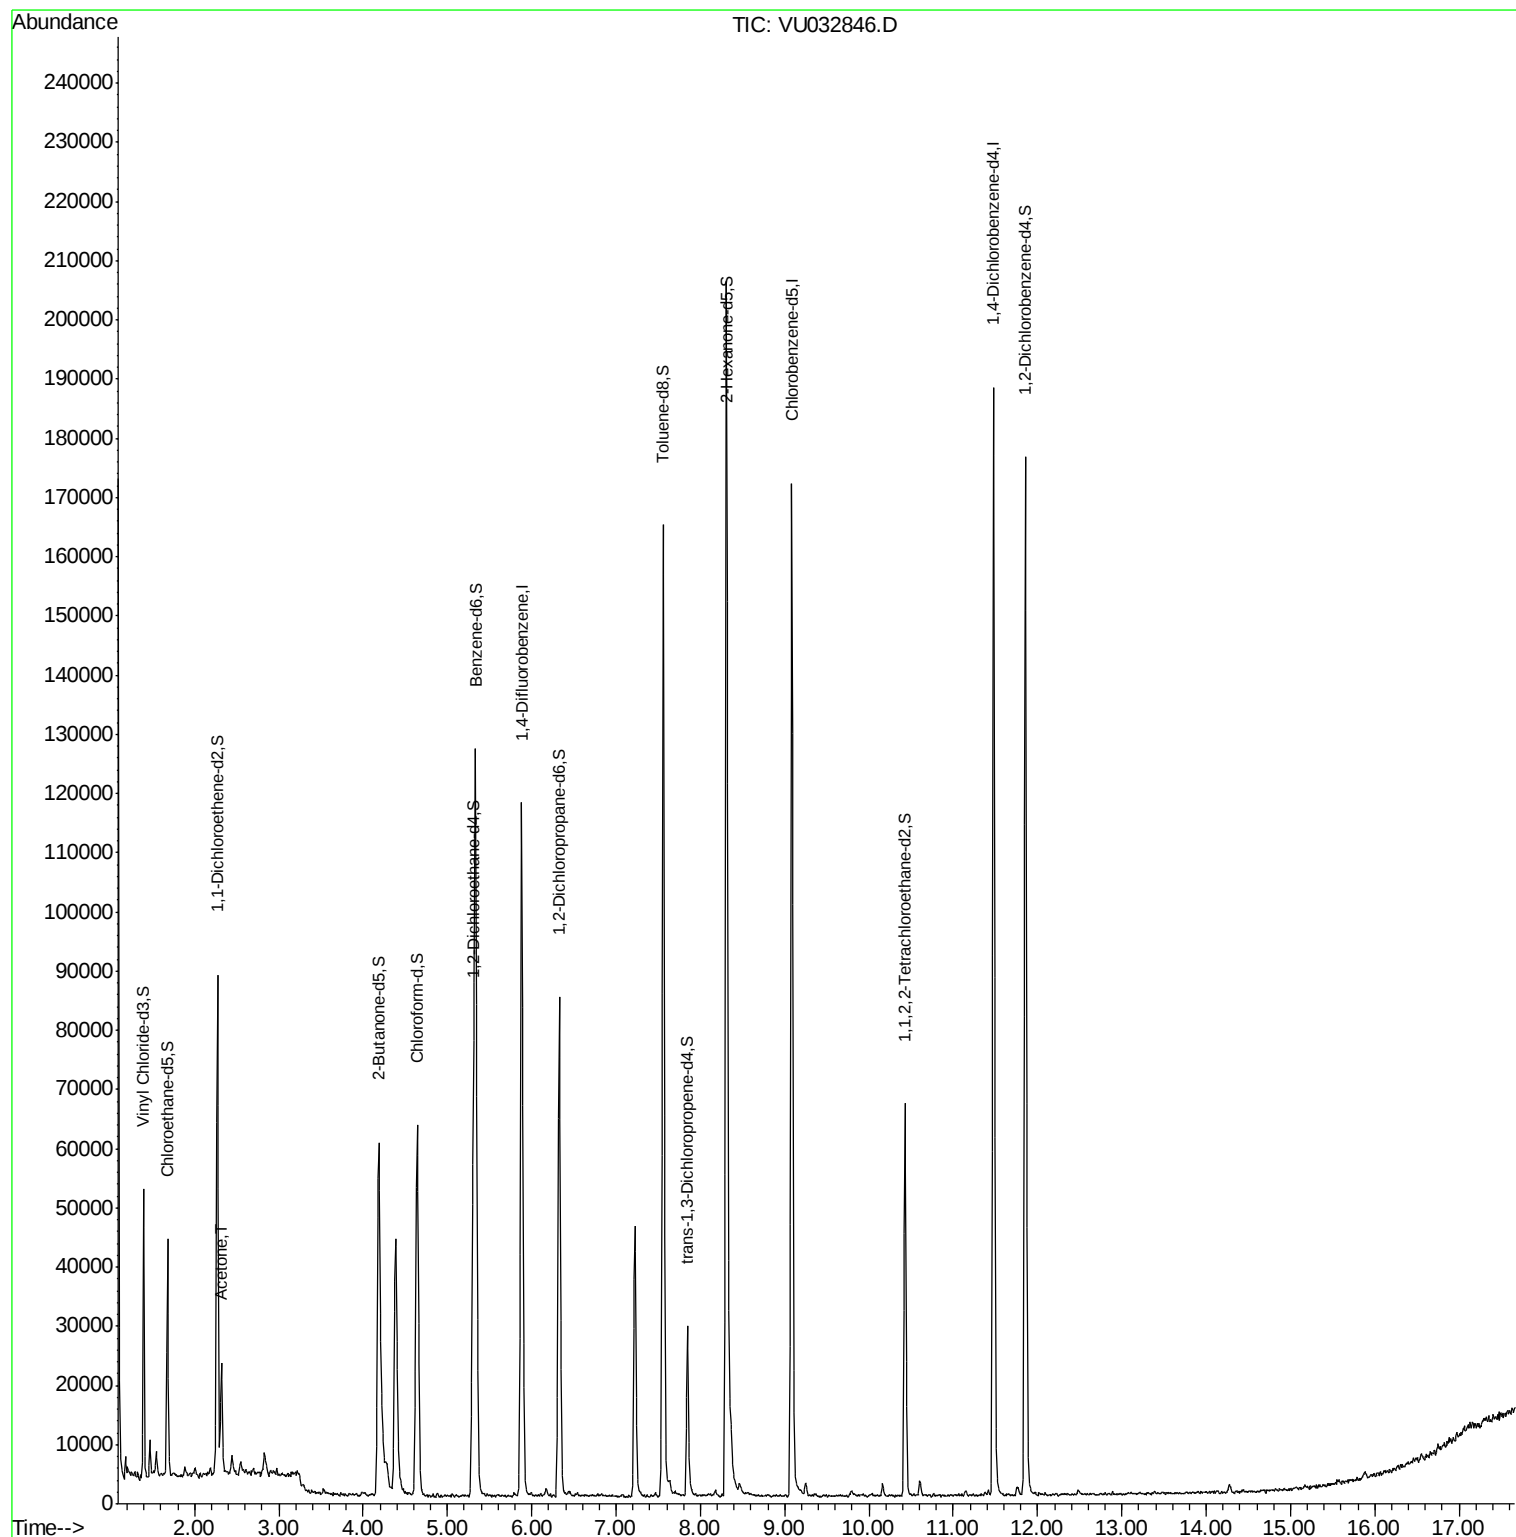

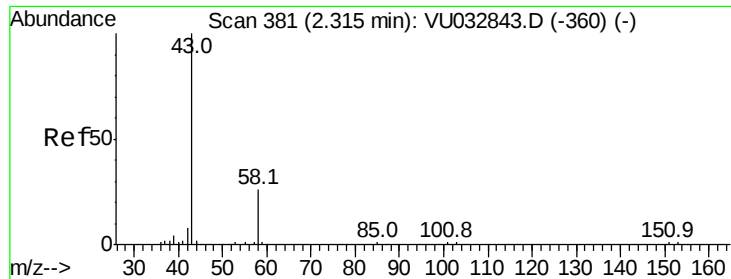

#13

Acetone

Concen: 14.019 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032846.D

Acq: 19 Jun 2019 10:22

Instrument :

MSVOA_U

ClientSampleId :

GALH1

Tot Ion: 43 Resp: 19115

Ion Ratio Lower Upper

43 100

58 29.0 0.0 60.8

