

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061919\
 Data File : VU032855.D
 Acq On : 19 Jun 2019 13:59
 Operator : JC/SP
 Sample : K3413-25
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALH1

Quant Time: Jun 20 07:05:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 05:14:15 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	92063	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	89904	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	47315	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	28106	4.70	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.00%
7) Chloroethane-d5	1.68	69	23575	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.20%
11) 1,1-Dichloroethene-d2	2.27	63	45053	3.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.20%
20) 2-Butanone-d5	4.18	46	97019	58.08	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.16%
24) Chloroform-d	4.64	84	57821	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
26) 1,2-Dichloroethane-d4	5.30	65	34245	6.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.20%
32) Benzene-d6	5.33	84	110760	4.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.20%
36) 1,2-Dichloropropane-d6	6.32	67	36515	5.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.00%
41) Toluene-d8	7.56	98	100466	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.20%
43) trans-1,3-Dichloropropene-	7.85	79	15110	5.13	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.60%
46) 2-Hexanone-d5	8.31	63	70363	47.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.40%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	31484	5.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	43532	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	8670	6.687 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061919\
Data File : VU032855.D
Acq On : 19 Jun 2019 13:59
Operator : JC/SP
Sample : K3413-25
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALH1

Quant Time: Jun 20 07:05:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 05:14:15 2019
Response via : Initial Calibration

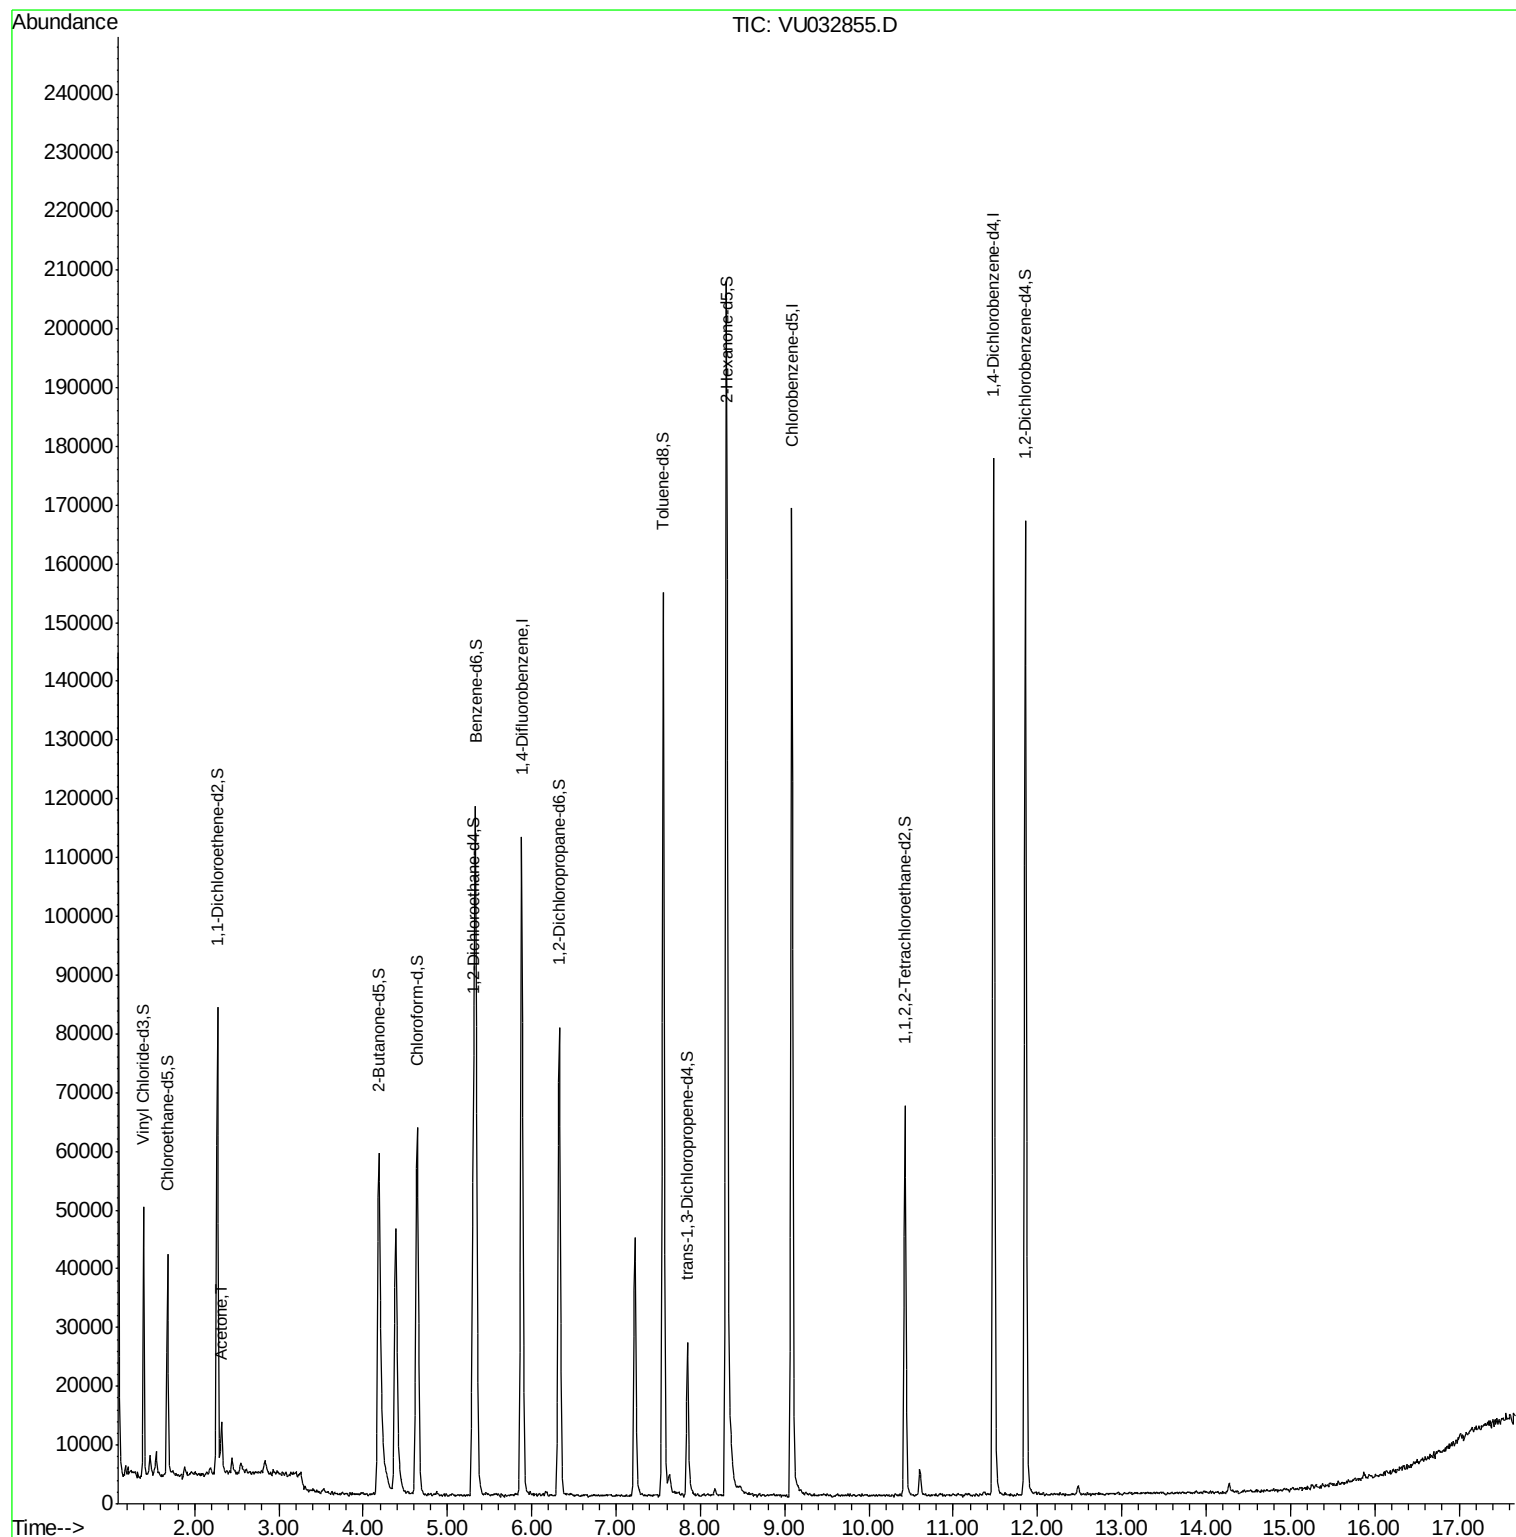

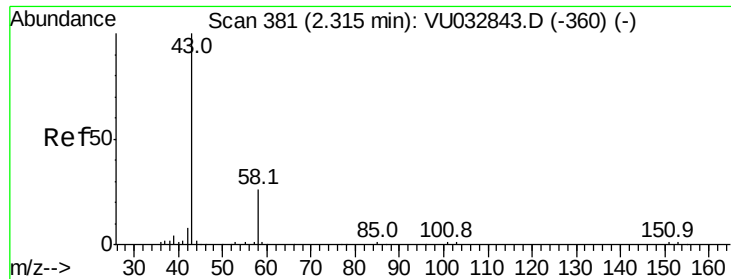

#13

Acetone

Concen: 6.687 ug/L

RT: 2.32 min Scan# 382

Delta R.T. 0.00 min

Lab File: VU032855.D

Acq: 19 Jun 2019 13:59

Instrument :

MSVOA_U

ClientSampleId :

GALH1

Tot Ion: 43 Resp: 8670

Ion Ratio Lower Upper

43 100

58 27.6 0.0 60.8

