

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061919\
 Data File : VU032880.D
 Acq On : 20 Jun 2019 00:07
 Operator : JC/SP
 Sample : K3414-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALM2

Quant Time: Jun 20 08:50:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Jun 20 07:24:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	94872	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	92867	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	47747	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	26199	4.25	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.00%
7) Chloroethane-d5	1.68	69	23881	4.53	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.60%
11) 1,1-Dichloroethene-d2	2.27	63	43638	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	4.19	46	99797	57.97	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.94%
24) Chloroform-d	4.64	84	60022	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.60%
26) 1,2-Dichloroethane-d4	5.30	65	35781	6.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	124.00%
32) Benzene-d6	5.33	84	112987	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
36) 1,2-Dichloropropane-d6	6.32	67	38088	5.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.00%
41) Toluene-d8	7.56	98	101768	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
43) trans-1,3-Dichloropropene-	7.85	79	14506	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.31	63	76528	50.22	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.44%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	33400	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.40%
64) 1,2-Dichlorobenzene-d4	11.85	152	44679	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
25) Chloroform	4.67	83	8379	0.705 ug/L	96
31) Carbon tetrachloride	5.13	117	546996	53.163 ug/L	98
42) Toluene	7.64	91	7396	0.242 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061919\
Data File : VU032880.D
Acq On : 20 Jun 2019 00:07
Operator : JC/SP
Sample : K3414-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALM2

Quant Time: Jun 20 08:50:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Jun 20 07:24:34 2019
Response via : Initial Calibration




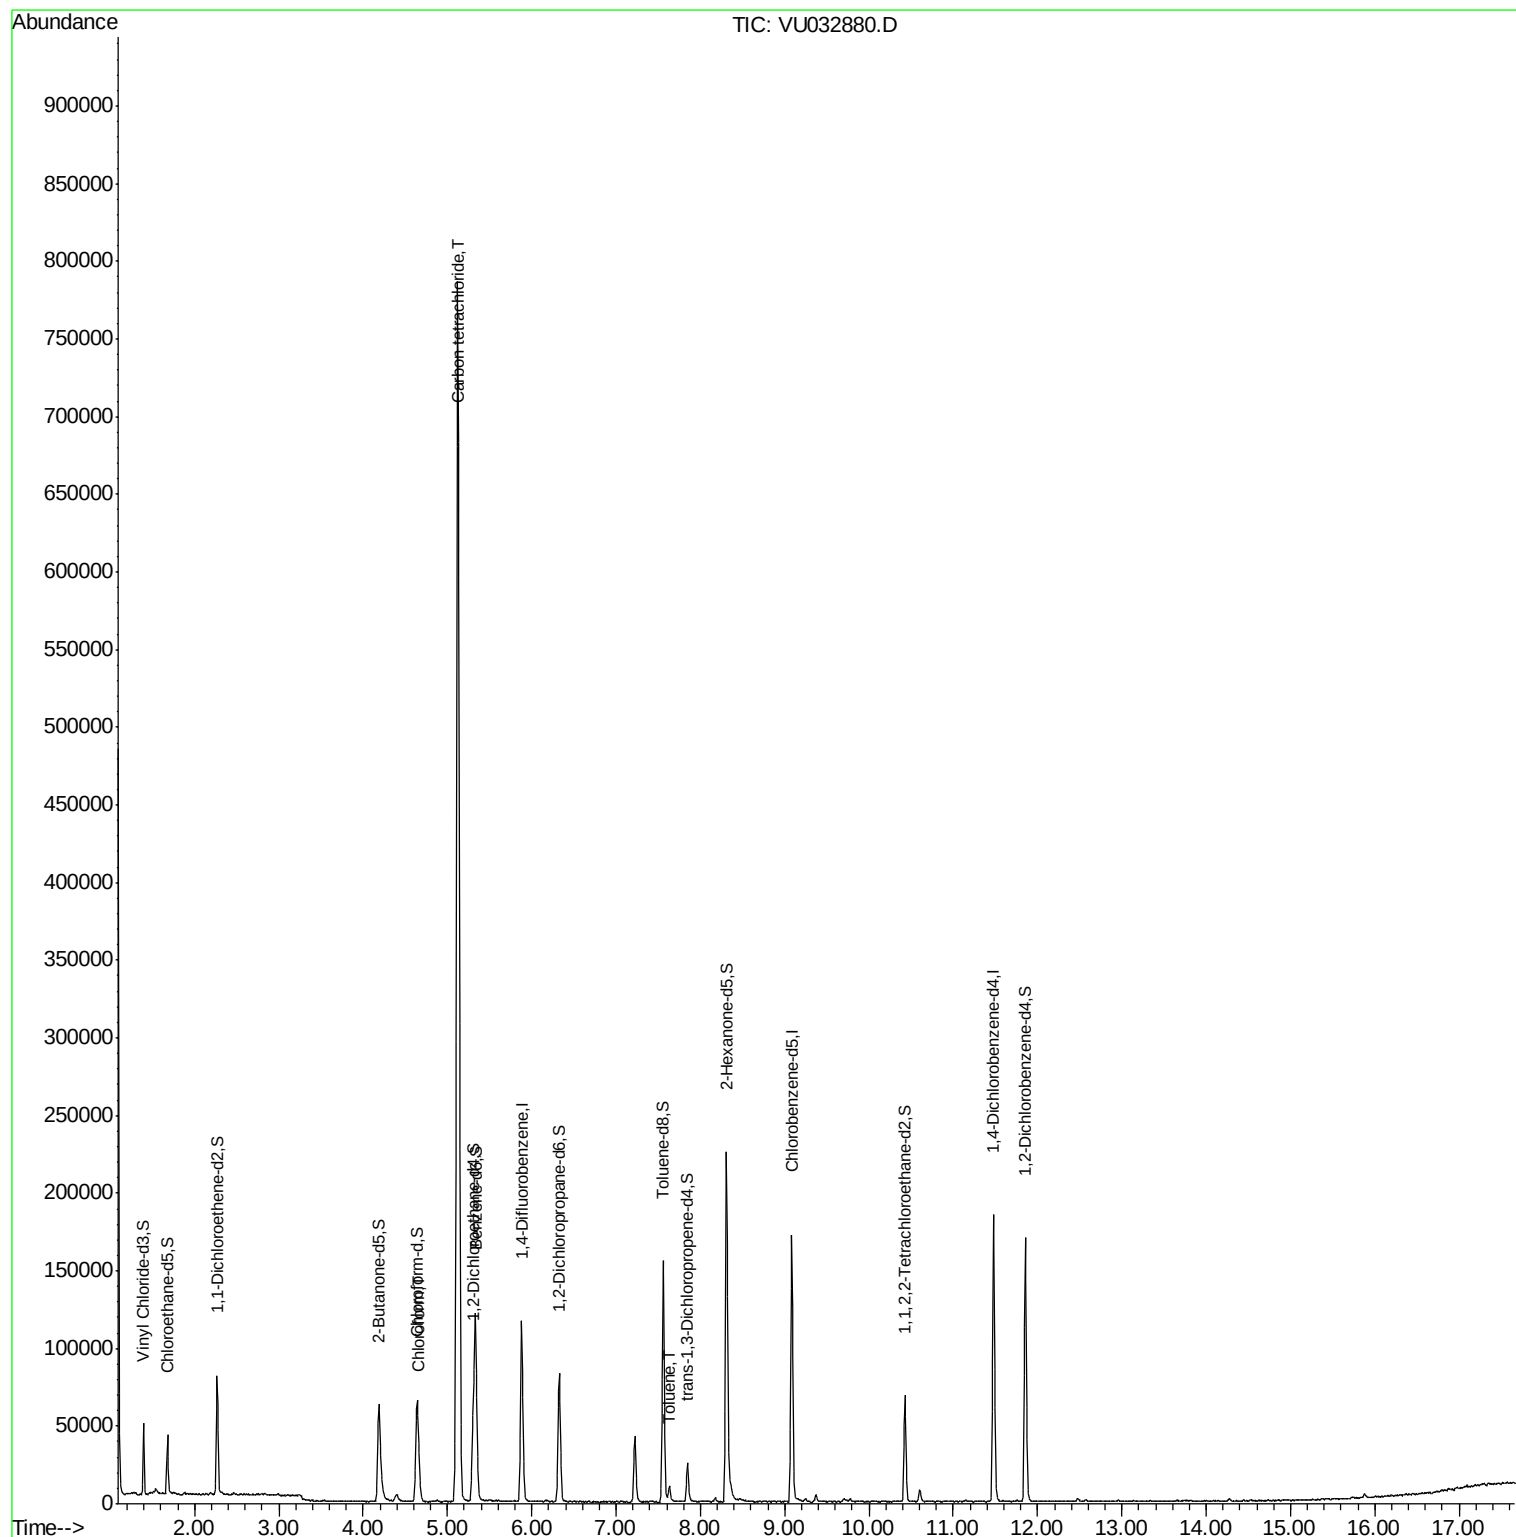


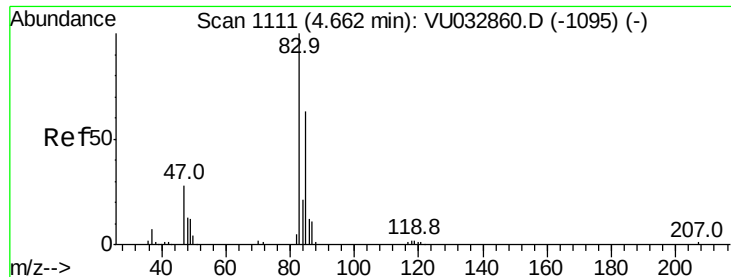

#25
Chloroform
Concen: 0.705 ug/L
RT: 4.67 min Scan# 1112
Delta R.T. 0.00 min
Lab File: VU032880.D
Acq: 20 Jun 2019 00:07




Instrument :
MSVOA_U
ClientSampleId :
GALM2


Tot Ion: 83 Resp: 8379
Ion Ratio Lower Upper
83 100
85 65.5 43.8 81.3

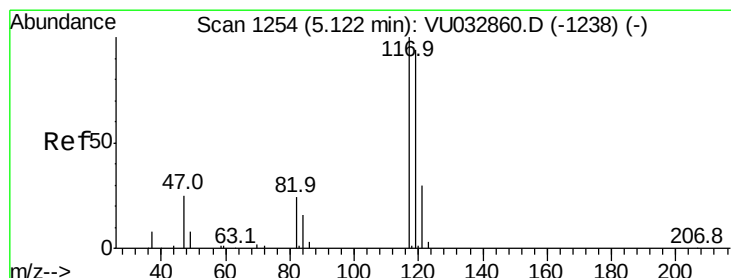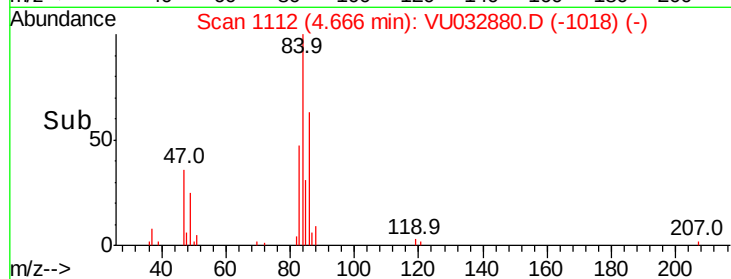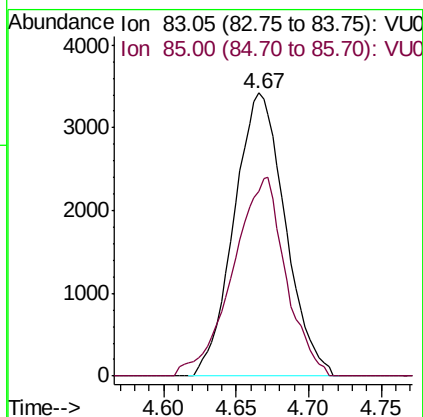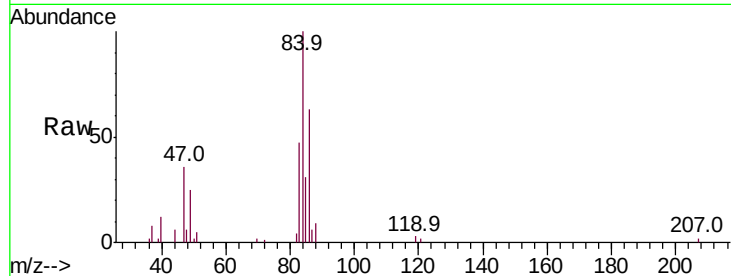

#31
Carbon tetrachloride
Concen: 53.163 ug/L
RT: 5.13 min Scan# 1255
Delta R.T. 0.00 min
Lab File: VU032880.D
Acq: 20 Jun 2019 00:07

Tgt Ion: 117 Resp: 546996
Ion Ratio Lower Upper
117 100
119 95.2 77.8 116.6

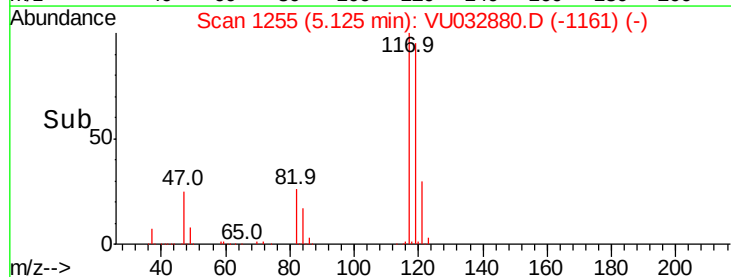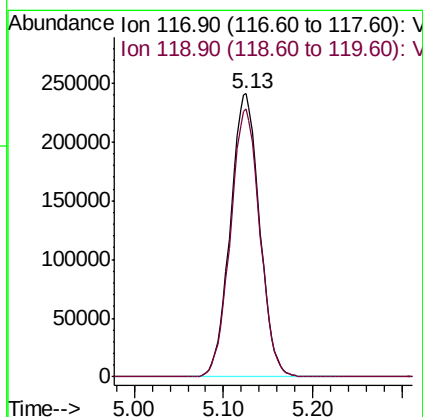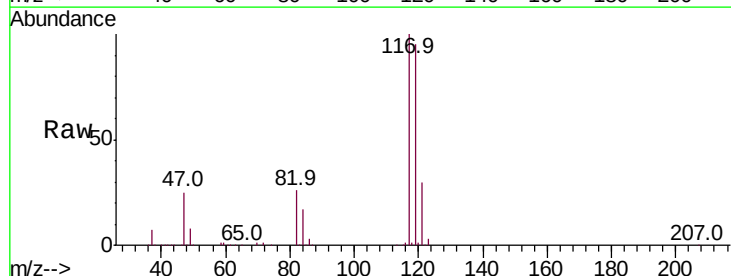

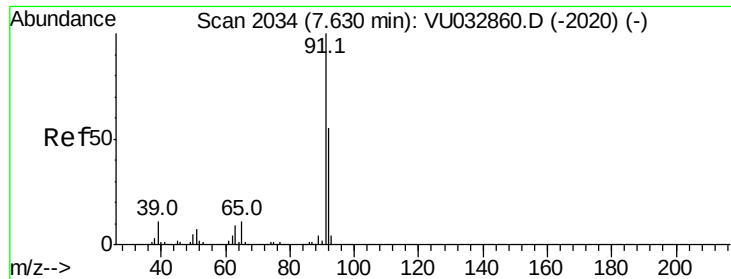

#42

Toluene

Concen: 0.242 ug/L

RT: 7.64 min Scan# 2036

Delta R.T. 0.01 min

Lab File: VU032880.D

Acq: 20 Jun 2019 00:07

Instrument :

MSVOA_U

ClientSampleId :

GALM2

Tot Ion: 91 Resp: 7396

Ion Ratio Lower Upper

91 100

92 53.5 40.9 75.9

