


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061919\
Data File : VU032842.D
Acq On : 19 Jun 2019 08:26
Operator : JC/SP
Sample : BFB41
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Jun 20 11:45:29 2019

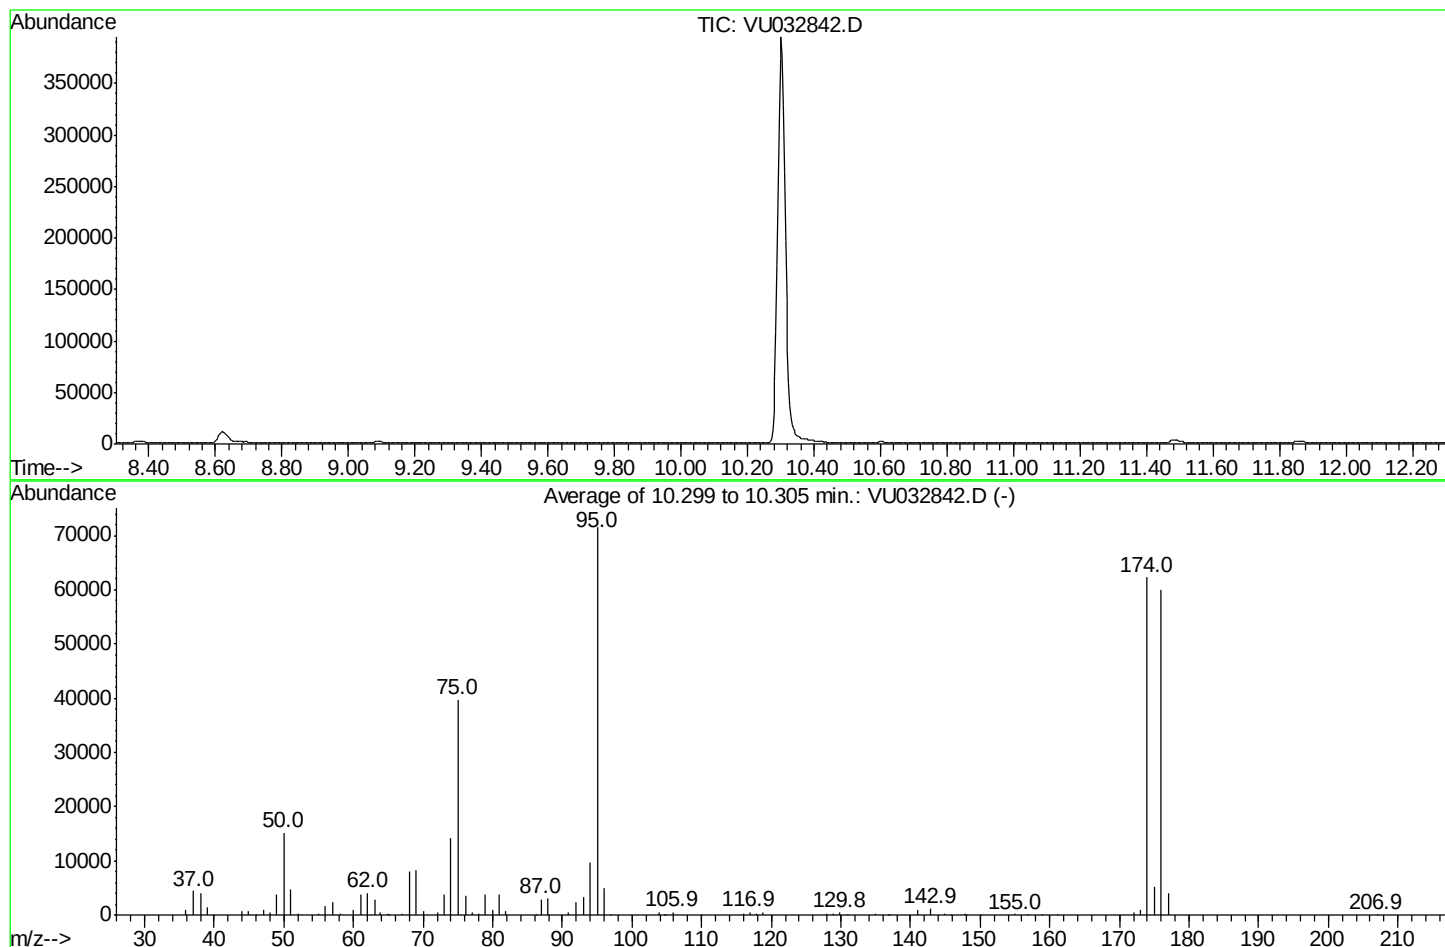

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	15172	PASS
75	95	30	80	55.5	39664	PASS
95	95	100	100	100.0	71498	PASS
96	95	5	9	6.8	4851	PASS
173	174	0.00	2	1.5	905	PASS
174	95	50	120	87.2	62314	PASS
175	174	5	9	8.2	5091	PASS
176	174	95	101	96.1	59912	PASS
177	176	5	9	6.8	4067	PASS

Scan 2851 (10.257 min): VU032842.D
BFB41

m/z	Abundance
40.00	783.0
44.00	326.0
207.00	148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	1010.0
37.00	4566.0
38.00	4091.0
39.00	1480.0
39.90	766.0
44.00	957.0
45.00	768.0
46.00	135.0
47.00	866.0
48.00	512.0
49.00	3618.0
50.00	15440.0
51.00	4755.0
52.00	241.0
54.90	251.0
56.00	1555.0
57.00	2430.0
58.10	105.0
59.90	976.0
61.00	3787.0
62.00	3957.0
63.00	2771.0
63.90	383.0
64.90	266.0
66.90	199.0
68.00	7815.0
69.00	8214.0
70.00	637.0
72.00	531.0
73.00	3736.0
74.00	13827.0
75.00	39736.0
76.00	3485.0
77.00	451.0
78.00	277.0
78.90	3725.0
80.00	984.0
80.90	3749.0
81.90	802.0
87.00	2715.0
88.00	2939.0
90.80	416.0
92.00	2359.0
93.00	3252.0
94.00	9535.0
95.00	70456.0
96.00	5030.0
97.00	122.0
103.90	447.0
104.90	118.0
105.90	488.0
115.90	271.0
116.90	493.0
117.80	308.0
118.80	415.0
127.90	242.0
128.80	176.0
129.80	373.0
131.00	100.0
134.90	175.0
136.80	101.0
141.00	879.0
142.90	1015.0
144.90	124.0
145.80	124.0
147.80	220.0
149.90	109.0
154.90	174.0
156.90	103.0
158.90	102.0
161.00	105.0
172.00	416.0
173.10	925.0
174.00	59224.0
175.00	4826.0
176.00	57680.0
177.00	4021.0
206.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	1114.0
37.00	4524.0
38.00	4025.0
39.00	1535.0
39.90	844.0
44.00	962.0
44.90	795.0
46.00	122.0
47.00	940.0
47.90	609.0
49.00	3896.0
50.00	15604.0
51.00	4940.0
52.00	259.0
54.90	242.0
56.00	1634.0
57.00	2531.0
58.10	134.0
59.90	898.0
61.00	3955.0
62.00	4165.0
63.00	3017.0
63.90	383.0
64.90	238.0
66.90	228.0
68.00	8210.0
69.00	8588.0
70.00	681.0
72.00	550.0
73.00	3863.0
74.00	14632.0
75.00	41104.0
76.10	3726.0
77.00	567.0
78.00	351.0
78.90	3835.0
79.90	997.0
80.90	3877.0
81.90	817.0
86.90	2916.0
87.90	3109.0
90.90	408.0
92.00	2491.0
93.00	3566.0
94.00	9906.0
95.00	73848.0
96.00	4953.0
96.90	131.0
103.90	489.0
104.80	115.0
105.90	498.0
116.00	331.0
116.90	561.0
117.80	322.0
118.90	496.0
127.90	253.0
128.90	192.0
129.90	382.0
130.90	103.0
134.90	216.0
137.00	106.0
140.90	857.0
142.90	1125.0
144.90	134.0
145.70	127.0
147.80	178.0
150.00	114.0
155.00	191.0
156.90	124.0
172.00	445.0
173.10	946.0
174.00	64472.0
175.00	5354.0
176.00	61904.0
177.00	4191.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	1034.0
37.00	4265.0
38.00	3612.0
39.00	1474.0
39.90	915.0
44.00	876.0
44.90	715.0
47.00	930.0
47.90	591.0
49.00	3643.0
50.00	14474.0
51.00	4558.0
52.00	250.0
54.90	233.0
56.00	1542.0
57.00	2344.0
58.00	151.0
59.90	778.0
61.00	3769.0
62.00	3980.0
63.00	2929.0
63.90	327.0
65.10	220.0
66.90	224.0
68.00	7777.0
69.00	8218.0
70.00	677.0
72.00	477.0
73.00	3625.0
74.00	14321.0
75.00	38152.0
76.10	3603.0
77.00	615.0
78.00	359.0
78.90	3594.0
79.90	902.0
80.90	3641.0
81.90	790.0
86.20	132.0
86.90	2893.0
87.90	2932.0
90.90	365.0
92.00	2365.0
93.00	3450.0
94.00	9303.0
95.00	70192.0
96.00	4572.0
97.00	101.0
103.90	439.0
104.60	101.0
105.90	475.0
109.90	118.0
116.00	348.0
116.90	583.0
117.80	304.0
118.90	537.0
127.90	253.0
128.90	192.0
129.90	350.0
130.80	105.0
134.90	202.0
137.00	121.0
140.90	814.0
142.90	1128.0
144.80	139.0
145.70	114.0
148.00	149.0
155.10	185.0
156.80	135.0
172.00	412.0
173.00	845.0
174.00	63248.0
175.00	5095.0
176.00	60152.0
177.00	3989.0
207.00	153.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41