

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU061920\
 Data File : VU038996.D
 Acq On : 19 Jun 2020 21:32
 Operator : SY/MD
 Sample : L3061-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFXK2

Quant Time: Jun 20 06:32:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061920WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Jun 20 05:43:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	254090	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	256642	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	120356	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	125754	5.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.00%
7) Chloroethane-d5	1.93	69	97591	5.62	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	112.40%
11) 1,1-Dichloroethene-d2	2.59	63	171665	4.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	81.20%
20) 2-Butanone-d5	4.68	46	380268	53.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.54%
24) Chloroform-d	5.10	84	206163	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.74	65	124226	5.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.20%
32) Benzene-d6	5.76	84	417084	5.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.60%
36) 1,2-Dichloropropane-d6	6.72	67	133189	5.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.40%
41) Toluene-d8	7.92	98	411551	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.20%
43) trans-1,3-Dichloropropene-	8.20	79	67593	5.65	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	113.00%
46) 2-Hexanone-d5	8.66	63	276614	52.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.98%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	115641	5.15	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.00%
64) 1,2-Dichlorobenzene-d4	12.20	152	140912	5.81	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.20%


Target Compounds					Ovalue
13) Acetone	2.68	43	6521	1.498 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU061920\
Data File : VU038996.D
Acq On : 19 Jun 2020 21:32
Operator : SY/MD
Sample : L3061-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFXK2

Quant Time: Jun 20 06:32:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061920WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Jun 20 05:43:50 2020
Response via : Initial Calibration

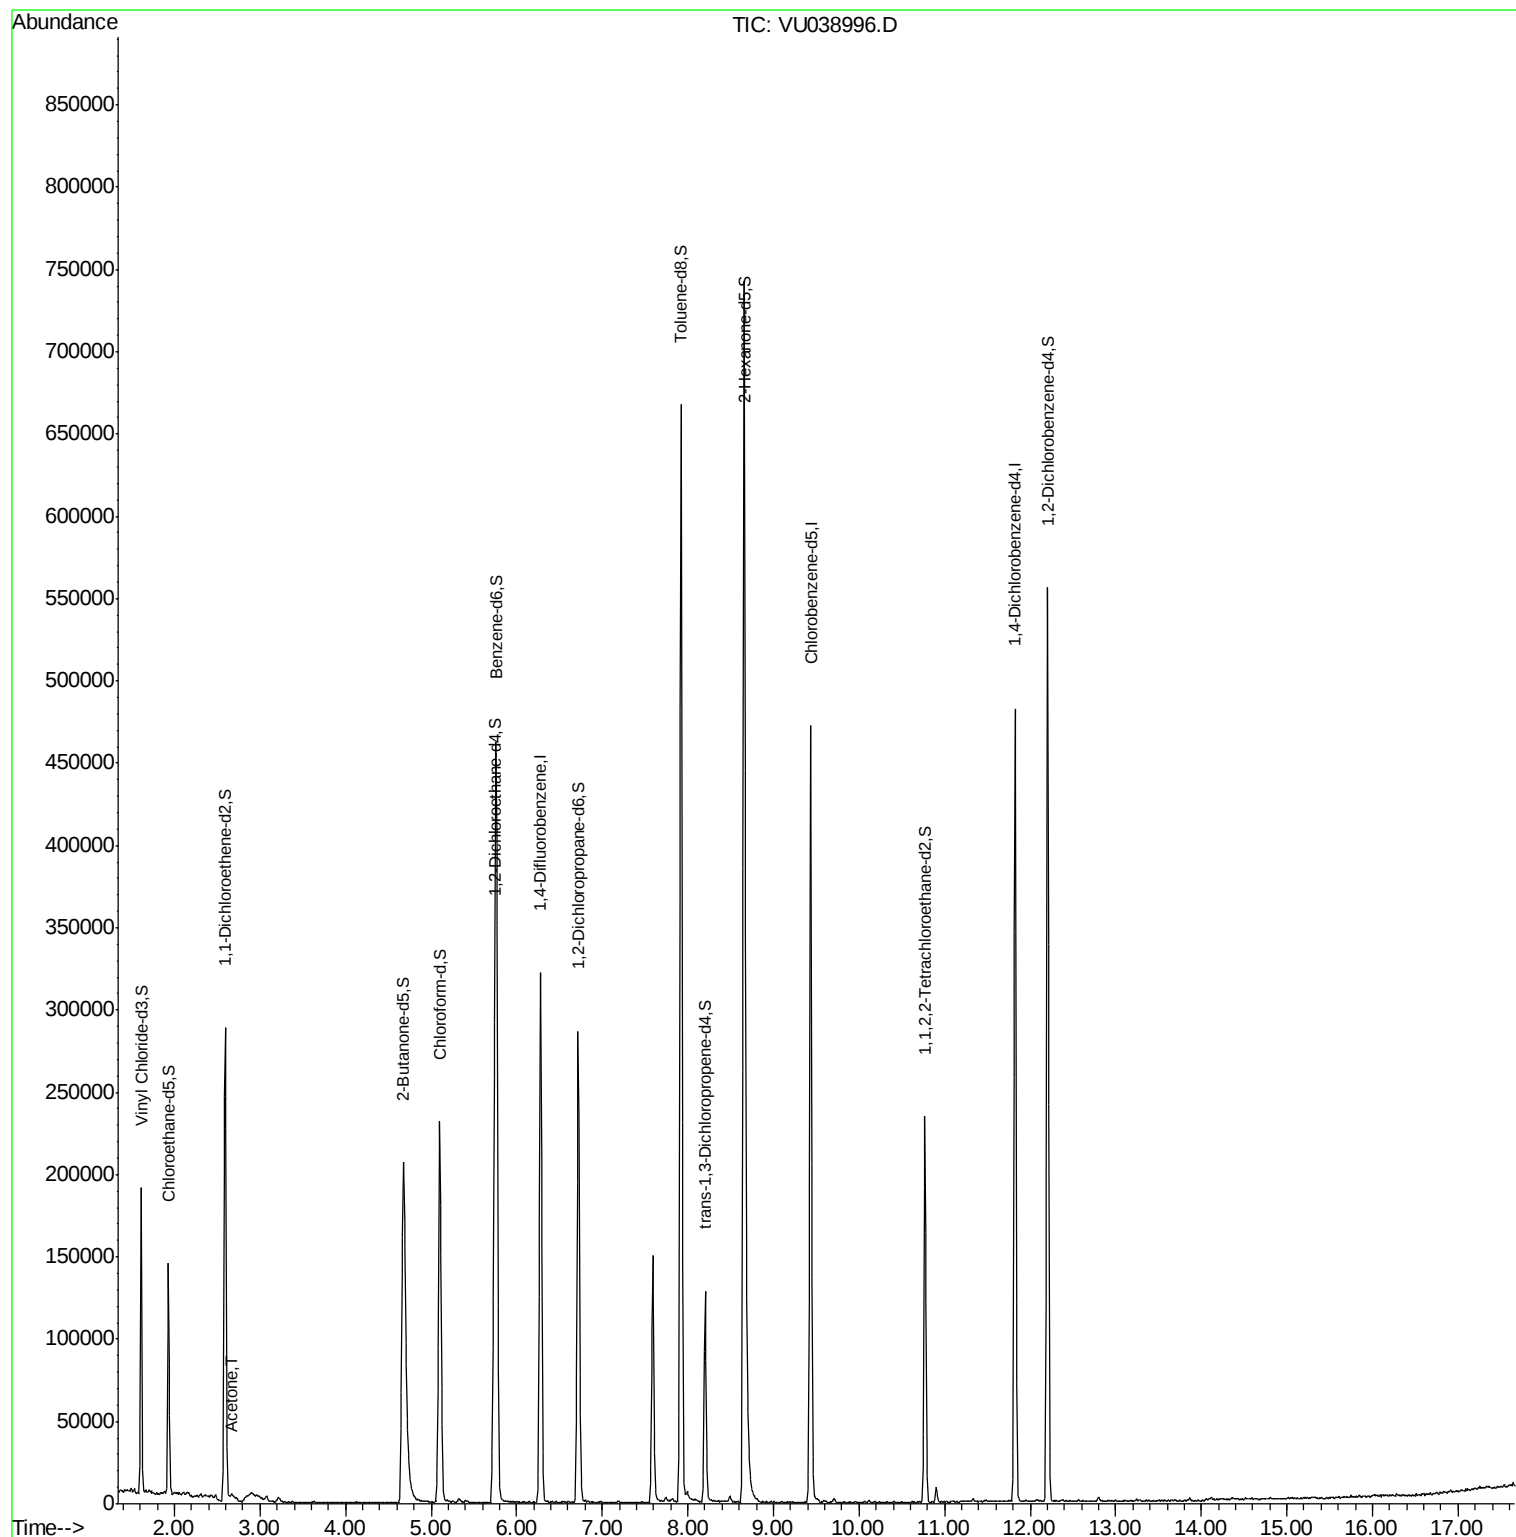

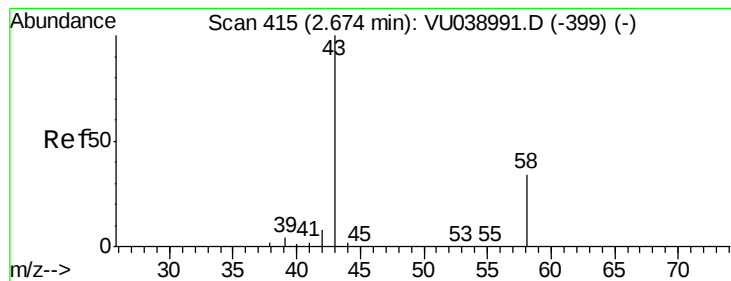

#13

Acetone

Concen: 1.498 ug/L

RT: 2.68 min Scan# 416

Delta R.T. 0.00 min

Lab File: VU038996.D

Acq: 19 Jun 2020 21:32

Instrument :
MSVOA_U
ClientSampleId :
BFXK2

Tot Ion: 43 Resp: 6521

Ion Ratio Lower Upper

43 100

58 32.9 0.0 64.4

