


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU061920\
 Data File : VU038983.D
 Acq On : 19 Jun 2020 12:50
 Operator : SY/MD
 Sample : BFB17
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB17

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR061920WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Jun 20 05:43:50 2020

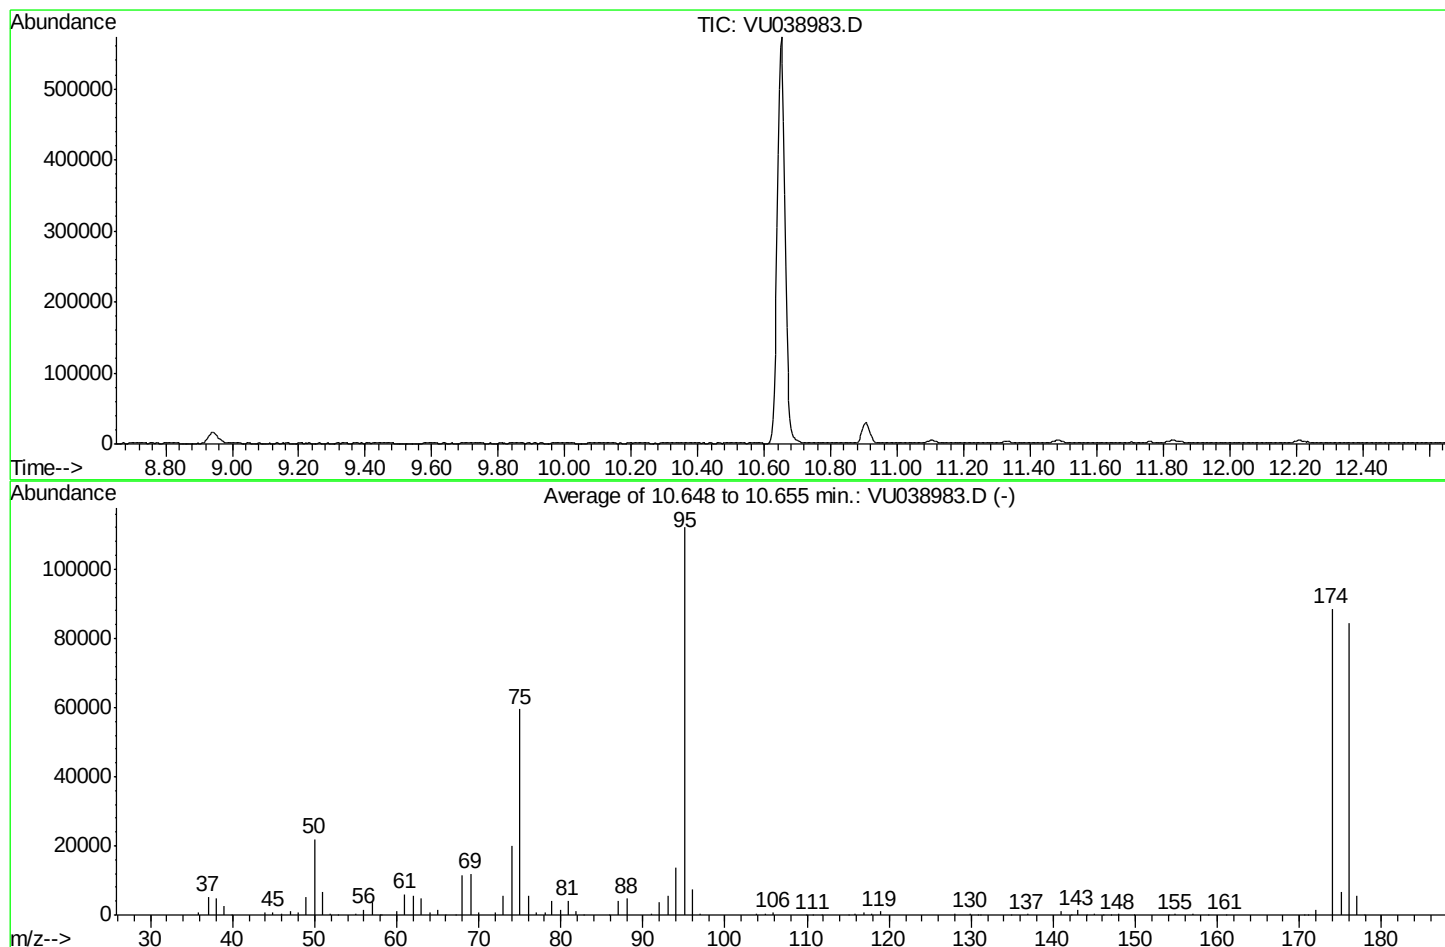

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	22016	PASS
75	95	30	80	53.1	59578	PASS
95	95	100	100	100.0	112112	PASS
96	95	5	9	6.8	7597	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.0	88613	PASS
175	174	5	9	7.5	6686	PASS
176	174	95	101	95.1	84304	PASS
177	176	5	9	6.6	5528	PASS

m/z	Abundance
35.80	923.0
37.00	5279.0
38.00	4904.0
39.00	2429.0
40.00	338.0
43.90	1432.0
44.90	941.0
46.00	246.0
47.10	1207.0
48.00	655.0
49.00	5327.0
50.00	22880.0
51.00	6939.0
52.00	397.0
53.00	178.0
55.00	404.0
56.00	1771.0
57.00	3591.0
57.90	197.0
59.90	1036.0
61.00	6397.0
62.00	5433.0
63.00	5014.0
64.00	777.0
65.10	1494.0
67.10	407.0
68.00	11595.0
69.00	12076.0
69.90	779.0
72.00	595.0
73.00	5686.0
74.00	20544.0
75.00	60376.0
76.00	5659.0
77.00	737.0
78.10	600.0
78.90	4268.0
80.00	1320.0
80.90	4251.0
81.90	1086.0
82.80	122.0
87.00	4391.0
88.00	4685.0
91.10	542.0
92.00	3709.0
93.00	5774.0
94.00	13610.0
95.10	113056.0
96.10	7268.0
96.90	224.0
103.90	589.0
104.90	225.0
105.90	528.0
109.90	111.0
110.70	137.0
115.00	134.0
115.90	432.0
117.00	1017.0
117.80	435.0
118.90	886.0
128.00	297.0
129.90	395.0
131.10	147.0
134.90	161.0
136.90	214.0
140.90	1221.0
142.20	118.0
143.00	1513.0
143.90	104.0
144.90	472.0
146.10	209.0
147.00	110.0
147.90	365.0
150.00	153.0
154.80	312.0
156.90	228.0
161.00	184.0
171.10	202.0
172.00	1354.0
174.00	88472.0
175.10	6634.0
176.00	83152.0
177.00	5433.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
35.90	928.0
37.00	5455.0
38.00	5014.0
39.00	2489.0
40.00	327.0
44.00	1469.0
44.90	859.0
46.00	231.0
47.00	1297.0
47.90	647.0
49.00	5387.0
50.00	22584.0
51.00	7091.0
51.90	370.0
52.90	177.0
55.00	388.0
56.00	1711.0
57.00	3692.0
58.10	201.0
59.90	1042.0
61.00	6250.0
62.00	5542.0
63.00	4789.0
64.00	809.0
65.00	1487.0
66.00	116.0
68.00	12085.0
69.00	12199.0
69.90	793.0
72.10	623.0
73.00	5711.0
74.00	20552.0
75.00	61416.0
76.00	5666.0
77.00	758.0
78.10	621.0
78.90	4288.0
80.00	1393.0
80.90	4187.0
81.90	1177.0
82.80	126.0
85.90	151.0
87.00	4285.0
88.00	4971.0
91.10	531.0
92.00	3769.0
93.10	5671.0
94.10	14113.0
95.10	115472.0
96.10	7874.0
96.90	201.0
103.90	575.0
104.90	238.0
105.90	577.0
109.90	144.0
110.70	174.0
111.80	162.0
115.10	150.0
115.90	508.0
117.00	966.0
117.90	474.0
118.90	1025.0
128.00	306.0
129.90	392.0
131.00	127.0
134.90	183.0
136.80	236.0
141.00	1255.0
142.10	104.0
142.90	1519.0
144.00	115.0
144.90	408.0
146.10	192.0
147.00	127.0
148.00	337.0
149.80	147.0
154.00	110.0
154.90	311.0
157.00	240.0
161.00	153.0
170.60	116.0
172.00	1440.0
174.00	91536.0
175.10	6964.0
176.00	86944.0
177.00	5729.0
177.90	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

m/z	Abundance
35.90	892.0
37.00	4948.0
38.00	4909.0
39.00	2376.0
39.90	331.0
43.90	1435.0
44.90	729.0
46.00	187.0
47.00	1261.0
47.90	563.0
49.00	4817.0
50.00	20584.0
51.00	6518.0
52.00	321.0
52.80	162.0
55.00	368.0
56.00	1490.0
57.00	3345.0
58.10	156.0
60.00	999.0
61.00	5712.0
62.00	5210.0
63.00	4140.0
64.00	823.0
65.00	1278.0
66.00	129.0
68.00	11331.0
69.00	11400.0
70.00	813.0
72.10	614.0
73.00	5289.0
74.10	18800.0
75.00	56944.0
76.00	5204.0
77.00	728.0
78.10	500.0
78.90	4086.0
80.00	1406.0
80.90	3818.0
81.90	1065.0
82.90	122.0
85.90	200.0
87.00	3903.0
88.00	4742.0
90.90	426.0
92.00	3489.0
93.00	4958.0
94.10	13340.0
95.10	107808.0
96.10	7649.0
97.00	183.0
103.90	497.0
104.90	179.0
105.90	655.0
110.00	142.0
110.70	153.0
111.80	199.0
115.10	164.0
115.90	520.0
117.00	778.0
117.90	483.0
118.90	1028.0
127.90	310.0
130.00	346.0
130.80	134.0
134.90	182.0
136.90	207.0
141.00	1097.0
142.90	1349.0
144.10	106.0
145.00	388.0
146.10	153.0
147.00	104.0
148.00	290.0
149.70	131.0
154.90	278.0
156.90	220.0
158.90	105.0
161.00	119.0
170.90	173.0
172.00	1347.0
174.00	85832.0
175.10	6462.0
176.00	82816.0
177.00	5422.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17

Scan 2882 (10.607 min): VU038983.D
BFB17

m/z	Abundance
40.00	216.0
43.90	682.0

Instrument :
MSVOA_U
ClientSampleId :
BFB17