

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
 Data File : VU054593.D
 Acq On : 19 Jun 2023 13:53
 Operator : MD/SY
 Sample : 03237-18
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YBW89

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	109	rVB	65022	78154	8.29%	1.064%
2	1.911	186	193	204	rBV	87459	116941	12.40%	1.591%
3	2.566	385	397	409	rBV	120798	196569	20.85%	2.675%
4	3.042	537	545	558	rVB3	5741	10361	1.10%	0.141%
5	4.624	1023	1037	1063	rBV2	146052	392995	41.69%	5.348%
6	5.058	1156	1172	1195	rBV	177644	399573	42.39%	5.438%
7	5.724	1356	1379	1407	rBV2	320896	864734	91.73%	11.768%
8	6.245	1525	1541	1563	rBV	303865	601082	63.76%	8.180%
9	6.689	1660	1679	1700	rBV	220318	441219	46.80%	6.004%
10	7.563	1936	1951	1979	rBV	86293	163313	17.32%	2.223%
11	7.894	2041	2054	2074	rBV	353859	638349	67.71%	8.687%
12	8.177	2129	2142	2157	rBV	53044	96143	10.20%	1.308%
13	8.470	2217	2233	2243	rBV2	10366	17767	1.88%	0.242%
14	8.631	2271	2283	2324	rBV2	466468	942718	100.00%	12.829%
15	9.415	2514	2527	2552	rBV	431041	744978	79.02%	10.138%
16	10.753	2928	2943	2957	rBV	166690	272793	28.94%	3.712%
17	10.888	2975	2985	2997	rVB	19411	32563	3.45%	0.443%
18	11.807	3259	3271	3297	rBV	451821	727321	77.15%	9.898%
19	12.190	3375	3390	3414	rBV	368398	610583	64.77%	8.309%




Sum of corrected areas: 7348156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054593.D
Acq On : 19 Jun 2023 13:53
Operator : MD/SY
Sample : 03237-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

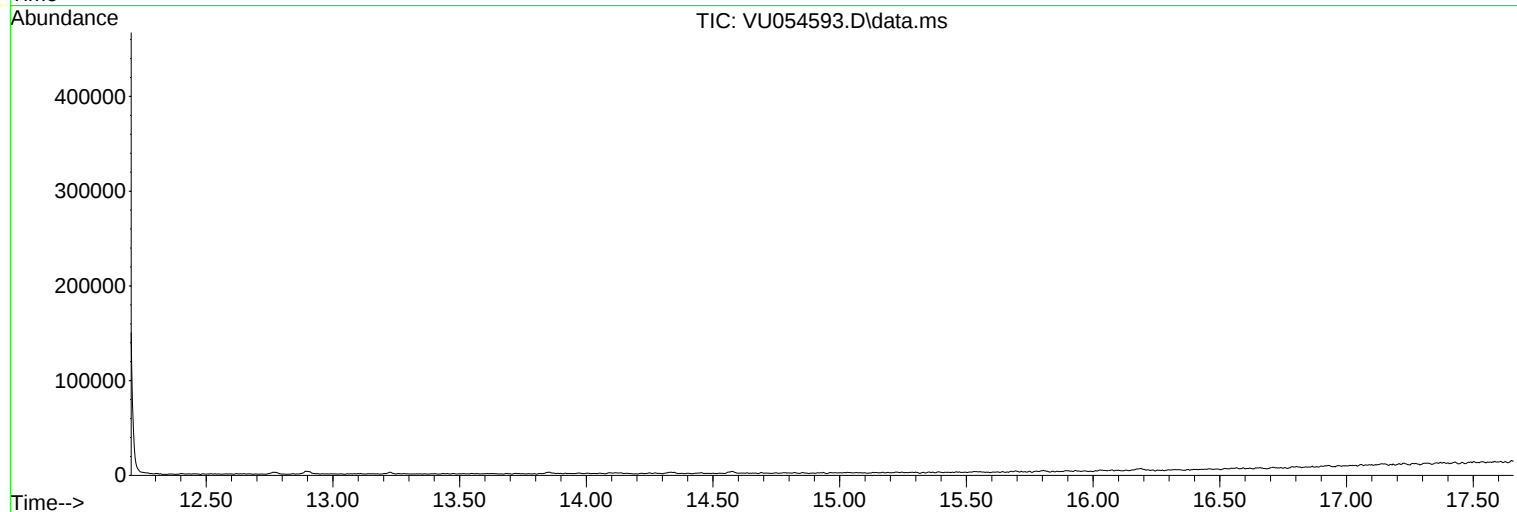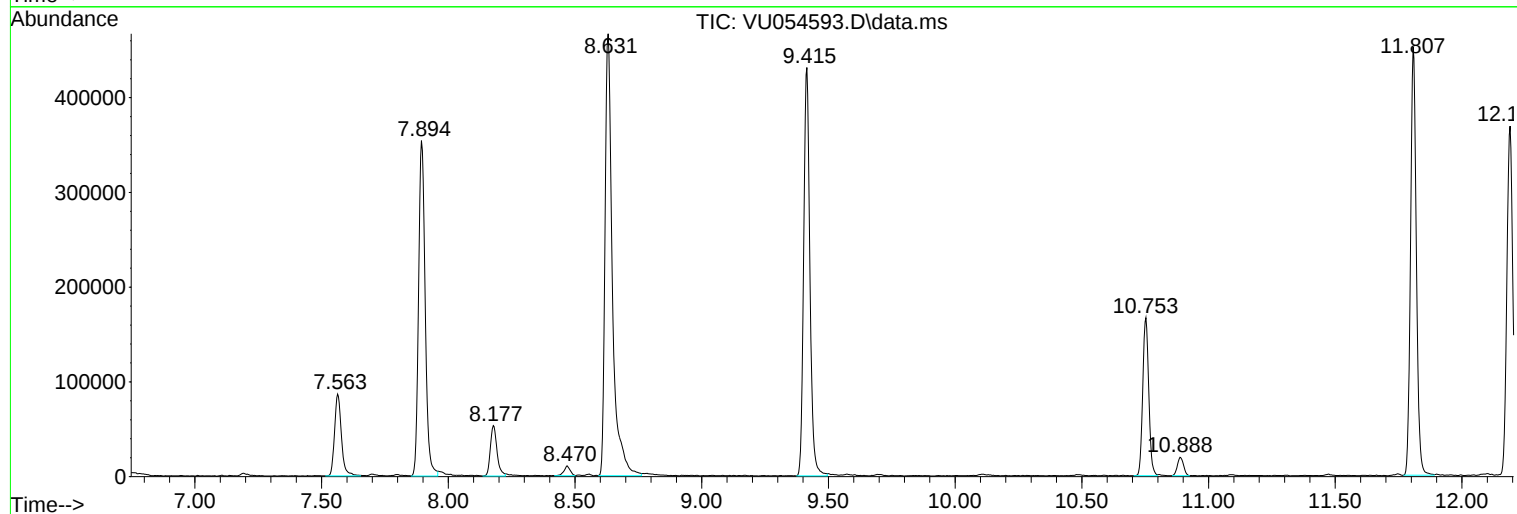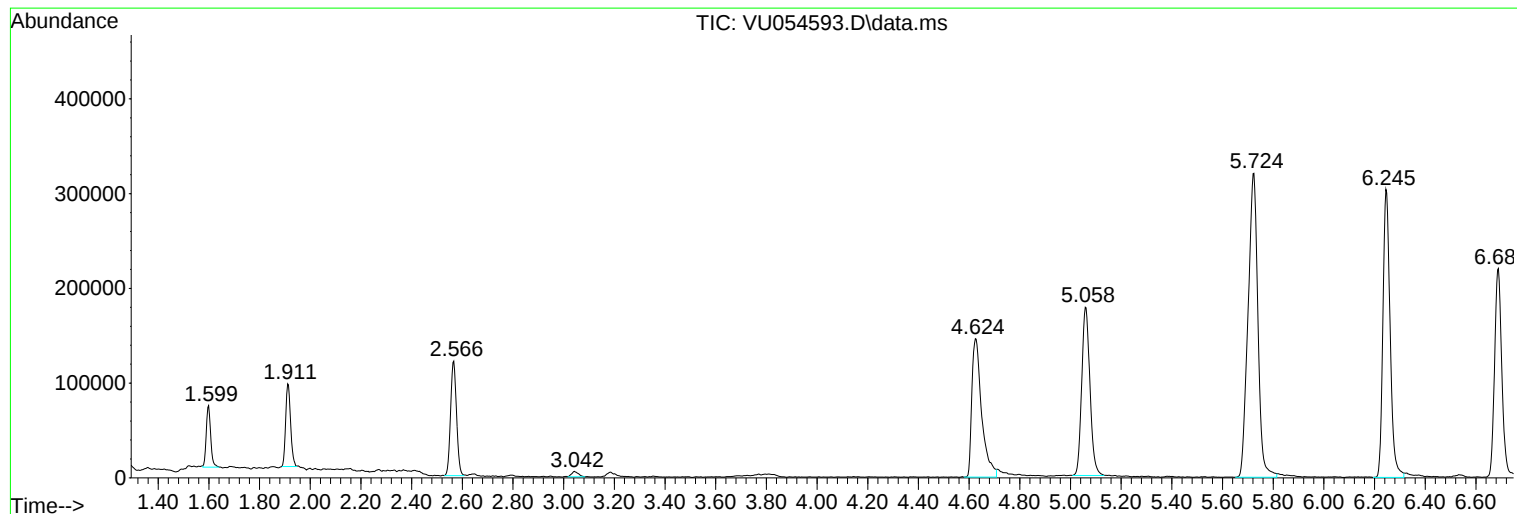

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054593.D
Acq On : 19 Jun 2023 13:53
Operator : MD/SY
Sample : 03237-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054593.D
Acq On : 19 Jun 2023 13:53
Operator : MD/SY
Sample : 03237-18
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc