

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
 Data File : VU054594.D
 Acq On : 19 Jun 2023 14:18
 Operator : MD/SY
 Sample : 03237-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 YBW73

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rBV	66526	80692	8.05%	1.044%
2	1.911	185	193	208	rBV	91696	128046	12.78%	1.657%
3	2.563	384	396	411	rBV	128147	211000	21.05%	2.730%
4	3.046	537	546	561	rVB3	6512	11989	1.20%	0.155%
5	4.624	1026	1037	1088	rBV	156382	444456	44.35%	5.751%
6	5.058	1156	1172	1197	rVB	185822	419229	41.83%	5.425%
7	5.721	1355	1378	1410	rBV2	344699	920660	91.87%	11.914%
8	6.245	1528	1541	1564	rBV	315456	612557	61.12%	7.927%
9	6.689	1659	1679	1698	rBV	234805	469692	46.87%	6.078%
10	7.563	1936	1951	1975	rBV	91808	170942	17.06%	2.212%
11	7.894	2039	2054	2074	rBV	374781	670053	66.86%	8.671%
12	8.177	2131	2142	2166	rBV	55468	102693	10.25%	1.329%
13	8.470	2219	2233	2244	rBV2	9414	16566	1.65%	0.214%
14	8.631	2271	2283	2323	rBV2	500644	1002150	100.00%	12.968%
15	9.415	2513	2527	2551	rBV	435266	759489	75.79%	9.828%
16	10.753	2930	2943	2958	rBV	176689	290343	28.97%	3.757%
17	10.888	2972	2985	2995	rBV	17331	30532	3.05%	0.395%
18	11.807	3260	3271	3295	rBV	453056	736355	73.48%	9.529%
19	12.190	3377	3390	3411	rBV	396541	650352	64.90%	8.416%




Sum of corrected areas: 7727796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054594.D
Acq On : 19 Jun 2023 14:18
Operator : MD/SY
Sample : 03237-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

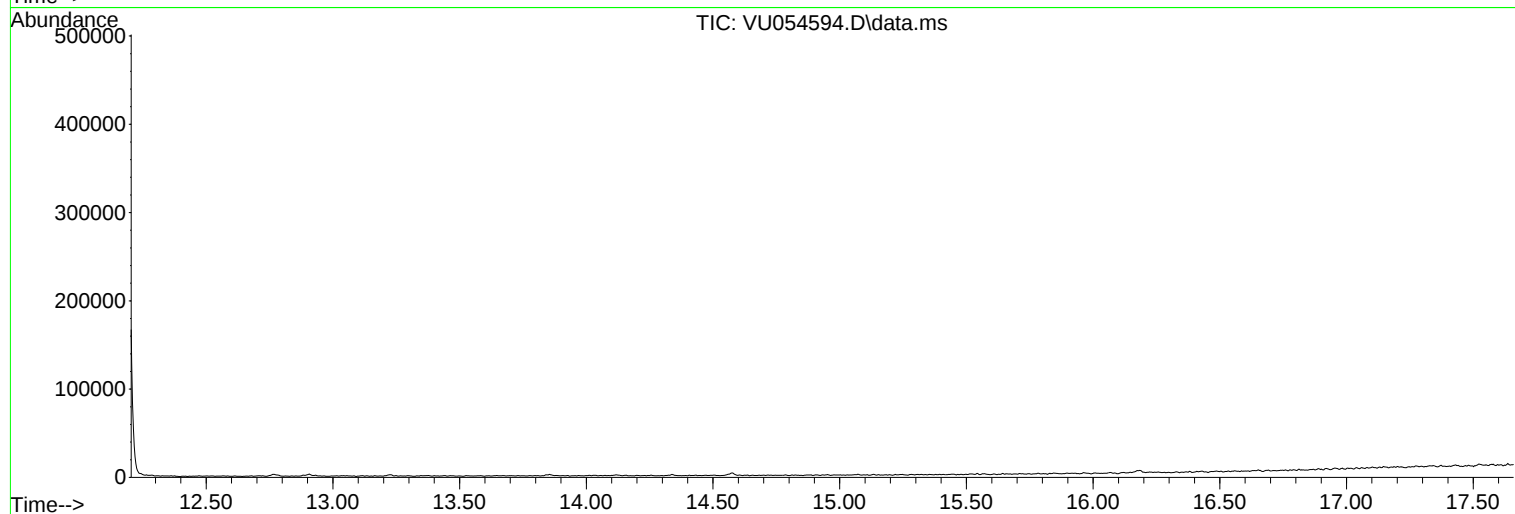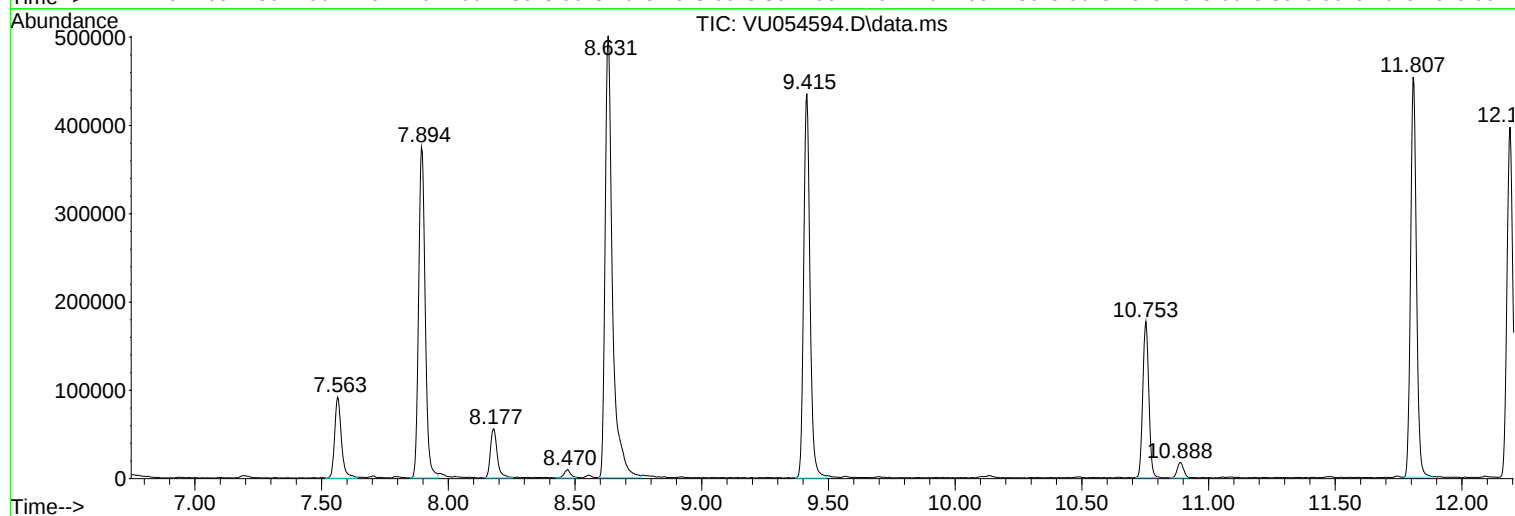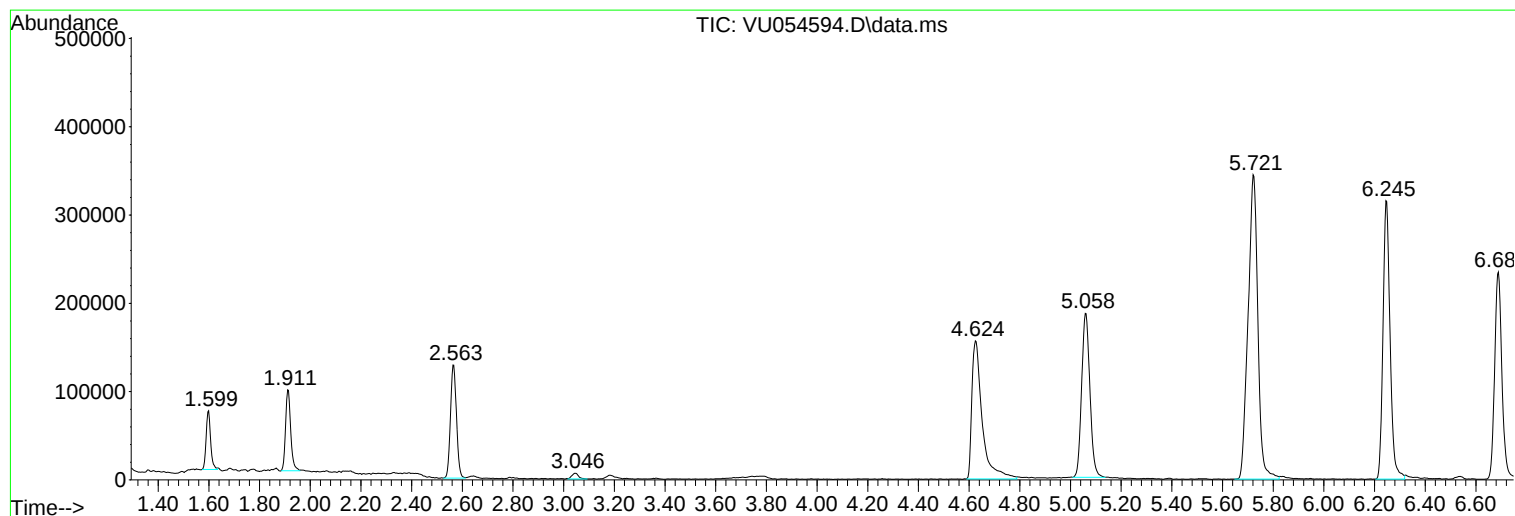

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054594.D
Acq On : 19 Jun 2023 14:18
Operator : MD/SY
Sample : 03237-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054594.D
Acq On : 19 Jun 2023 14:18
Operator : MD/SY
Sample : 03237-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
YBW73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc