

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
 Data File : VU054597.D
 Acq On : 19 Jun 2023 15:30
 Operator : MD/SY
 Sample : 03284-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	108	rVB	66123	81553	8.17%	1.079%
2	1.911	185	193	215	rVB	98433	140632	14.09%	1.861%
3	2.563	382	396	415	rBV	128417	215879	21.64%	2.857%
4	3.046	534	546	561	rVB3	17051	33841	3.39%	0.448%
5	4.624	1026	1037	1086	rBV	155315	428857	42.98%	5.676%
6	5.058	1156	1172	1193	rBV	184952	411225	41.21%	5.442%
7	5.721	1358	1378	1399	rBV2	341227	906775	90.88%	12.001%
8	6.245	1528	1541	1571	rBV	289118	576870	57.81%	7.635%
9	6.689	1663	1679	1696	rBV	232614	463688	46.47%	6.137%
10	7.563	1938	1951	1969	rBV	90545	165507	16.59%	2.190%
11	7.894	2040	2054	2074	rBV	380240	676492	67.80%	8.953%
12	8.177	2130	2142	2158	rBV	54357	99454	9.97%	1.316%
13	8.467	2223	2232	2245	rVB3	8427	15567	1.56%	0.206%
14	8.631	2271	2283	2319	rBV2	500210	997796	100.00%	13.206%
15	9.415	2512	2527	2553	rBV	405593	704294	70.58%	9.321%
16	10.753	2928	2943	2967	rBV	177320	290769	29.14%	3.848%
17	10.888	2974	2985	2999	rBV2	14642	26027	2.61%	0.344%
18	11.807	3260	3271	3294	rBV	405210	677848	67.93%	8.971%
19	12.190	3377	3390	3415	rBV	380415	642785	64.42%	8.507%




Sum of corrected areas: 7555859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054597.D
Acq On : 19 Jun 2023 15:30
Operator : MD/SY
Sample : 03284-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

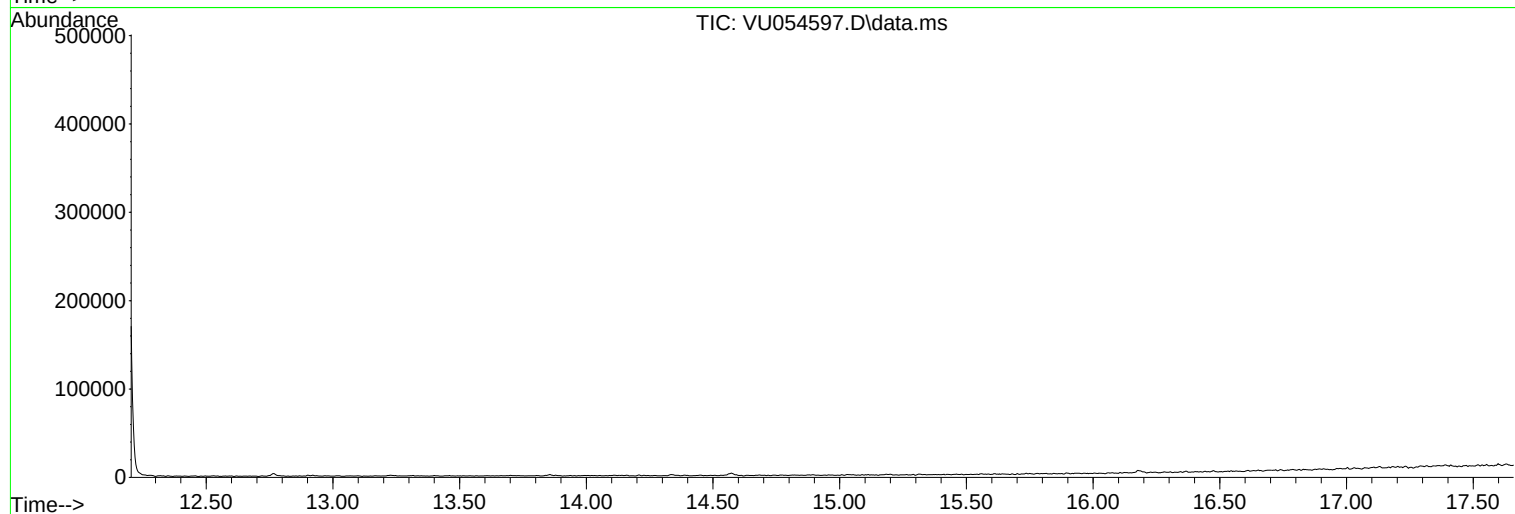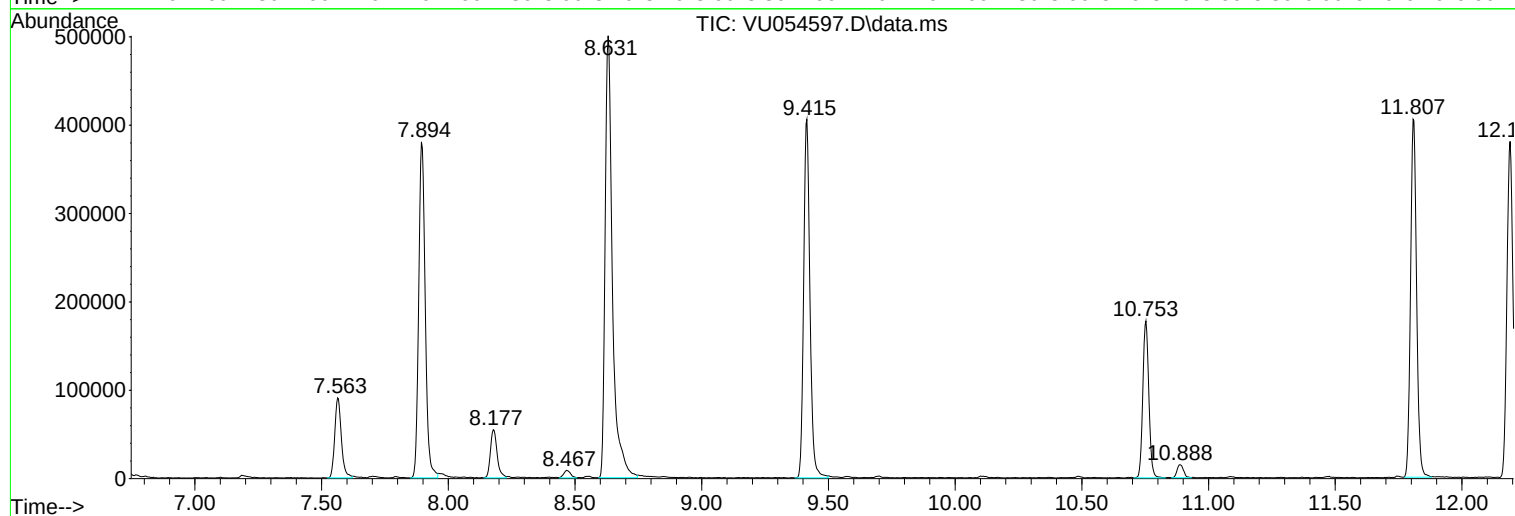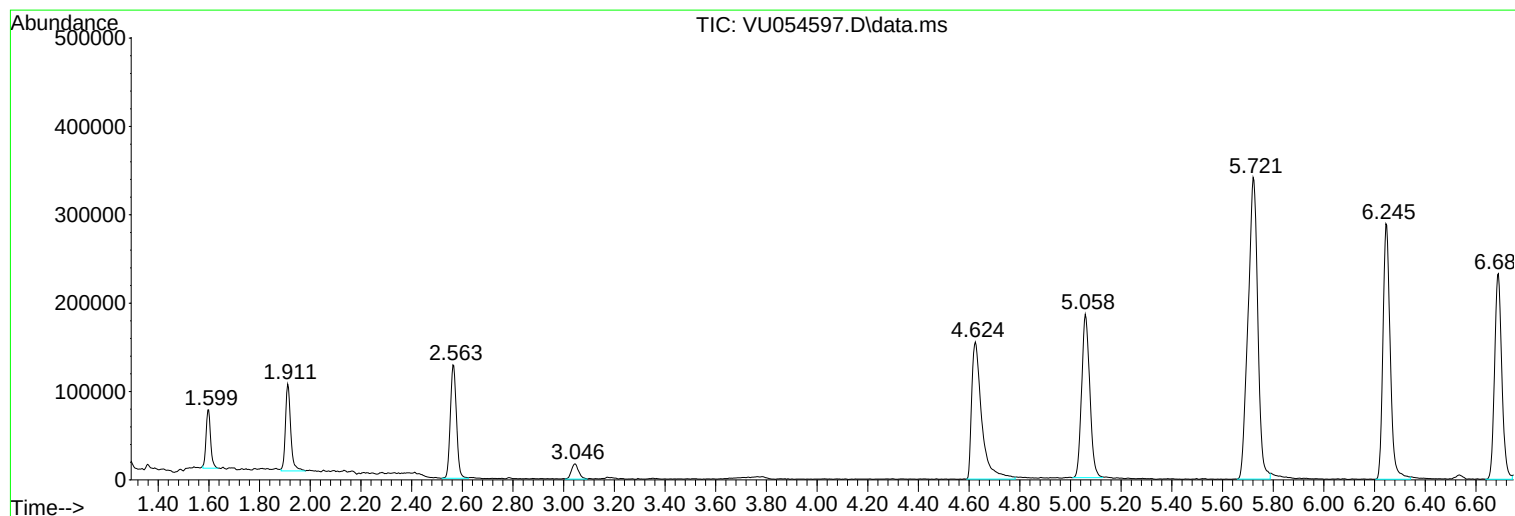

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054597.D
Acq On : 19 Jun 2023 15:30
Operator : MD/SY
Sample : 03284-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054597.D
Acq On : 19 Jun 2023 15:30
Operator : MD/SY
Sample : 03284-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
