

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
 Data File : VU054599.D
 Acq On : 19 Jun 2023 16:19
 Operator : MD/SY
 Sample : 03258-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCGX0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.872	482	492	507	rBV	109020	199092	29.10%	4.349%
2	5.354	1254	1264	1289	rVB	123958	308416	45.08%	6.736%
3	5.985	1440	1460	1483	rBV2	288505	684098	100.00%	14.942%
4	6.454	1594	1606	1636	rBV2	282494	558269	81.61%	12.194%
5	6.865	1716	1734	1750	rBV	162198	326712	47.76%	7.136%
6	8.001	2071	2087	2104	rBV	288557	542464	79.30%	11.849%
7	8.705	2291	2306	2336	rBV	187415	455201	66.54%	9.943%
8	9.467	2524	2543	2557	rBV	314230	554481	81.05%	12.111%
9	11.824	3263	3276	3293	rBV	307767	537249	78.53%	11.735%
10	12.200	3381	3393	3411	rVB2	242633	412310	60.27%	9.006%




Sum of corrected areas: 4578292

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054599.D
Acq On : 19 Jun 2023 16:19
Operator : MD/SY
Sample : 03258-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

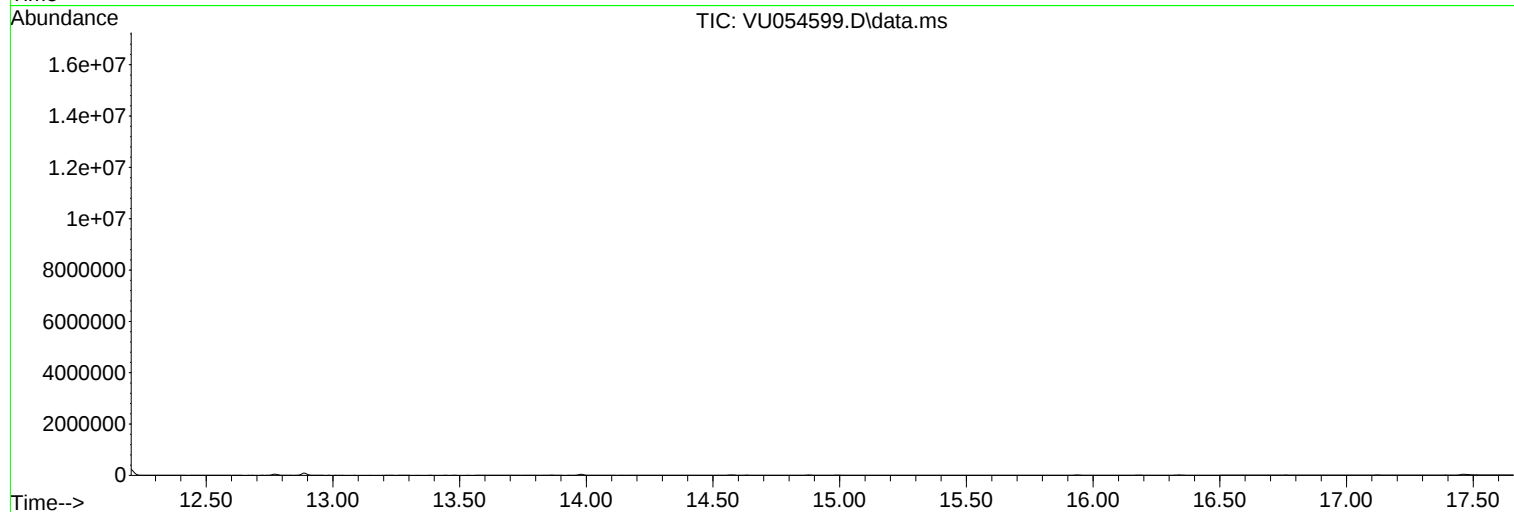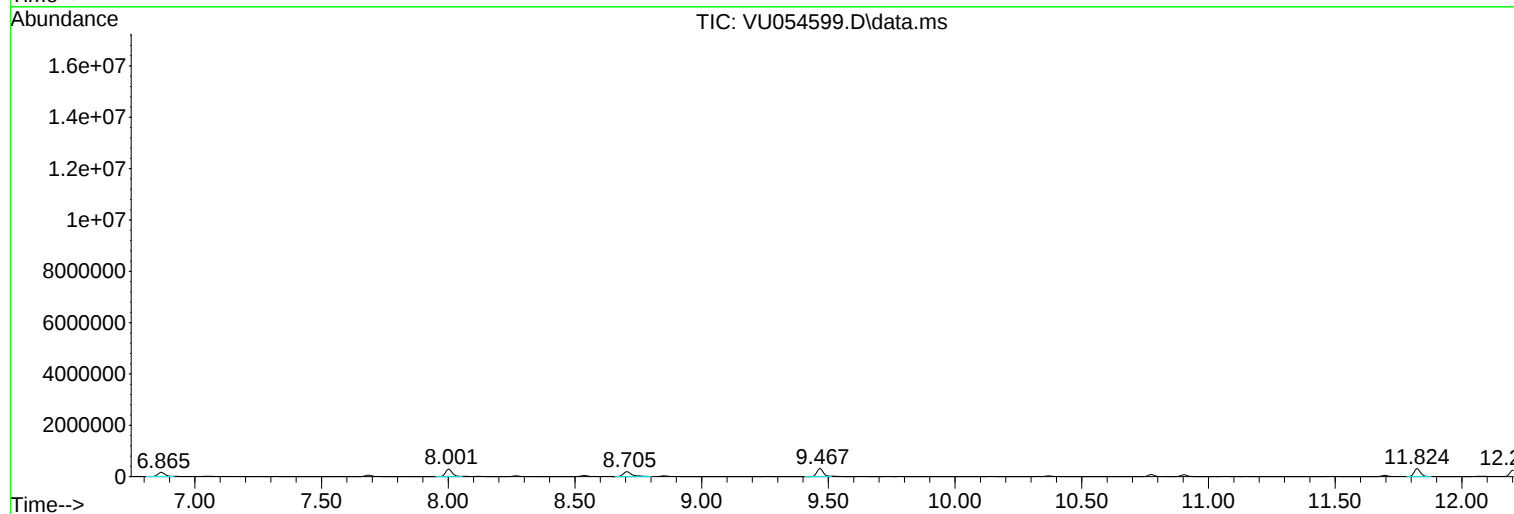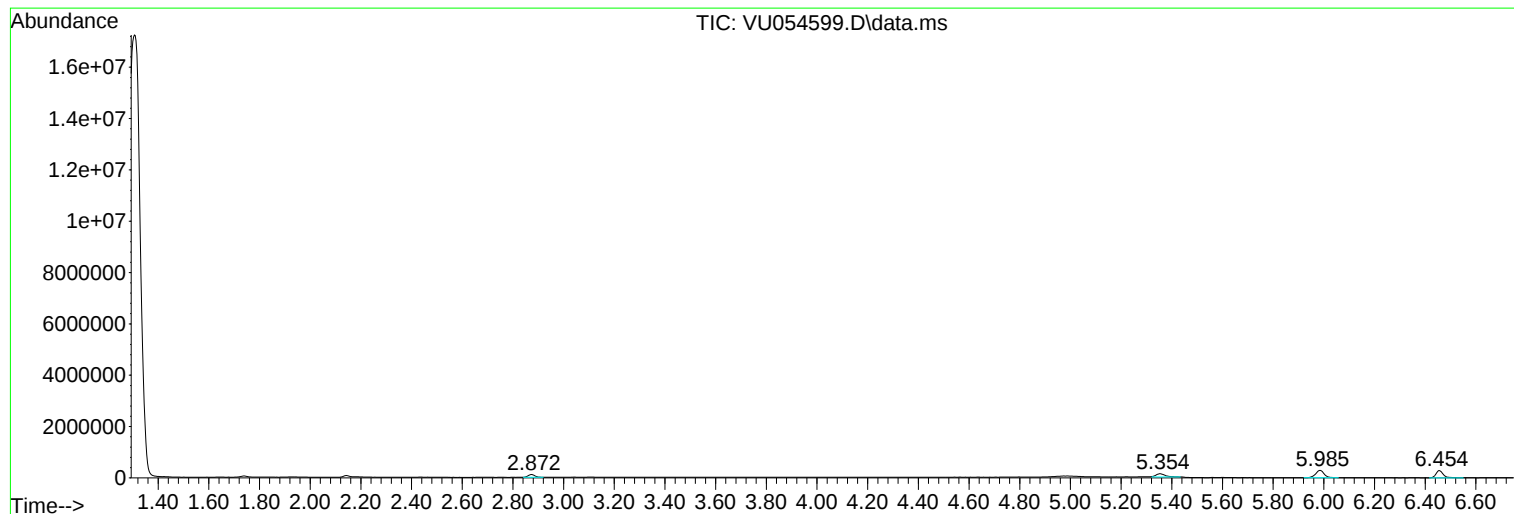

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054599.D
Acq On : 19 Jun 2023 16:19
Operator : MD/SY
Sample : 03258-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGX0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Methane-d, trichloro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.354	2.76 ug/L	308416	1,4-Difluorobenzene	6.454

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methane-d, trichloro-	119	CDCl3	000865-49-6	94
2			Methane-d, trichloro-	119	CDCl3	000865-49-6	80
3			2-Propenoic acid, 3-(dimethylami...	212	C11H20N2O2	049582-41-4	64
4			Methane-d, trichloro-	119	CDCl3	000865-49-6	50
5			Thiophene	84	C4H4S	000110-02-1	23

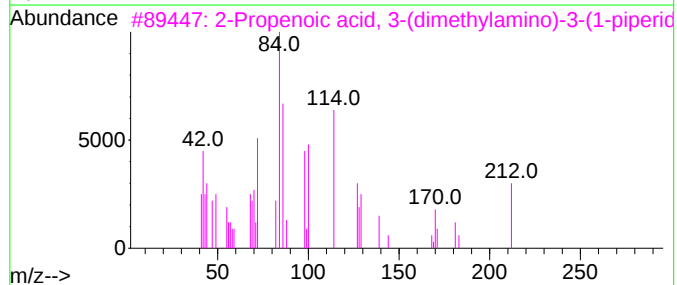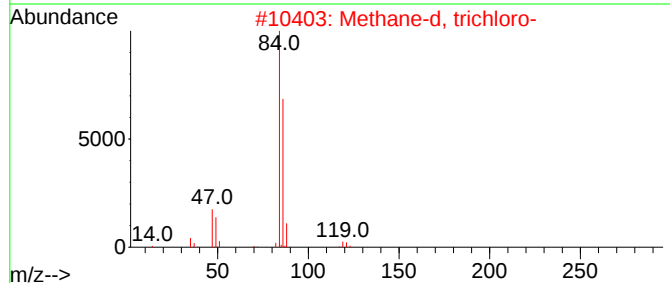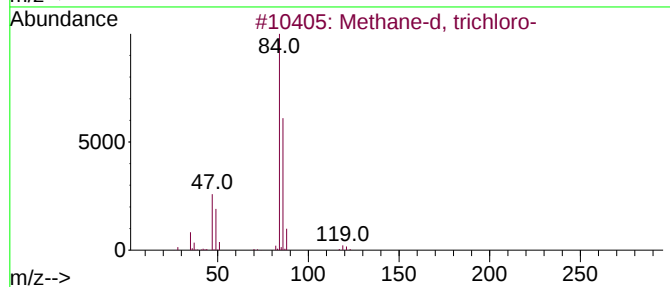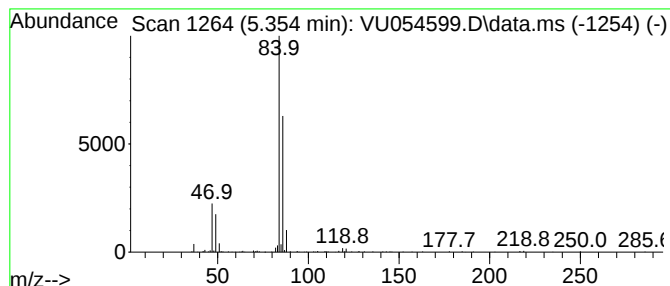

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
Data File : VU054599.D
Acq On : 19 Jun 2023 16:19
Operator : MD/SY
Sample : 03258-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCGX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Methane-d, tric...	5.354	2.8	ug/L	308416	1	6.454	558269	5.0