


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061923\
 Data File : VU054583.D
 Acq On : 19 Jun 2023 09:10
 Operator : MD/SY
 Sample : BFB021
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB021

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Sat Jun 17 06:10:25 2023

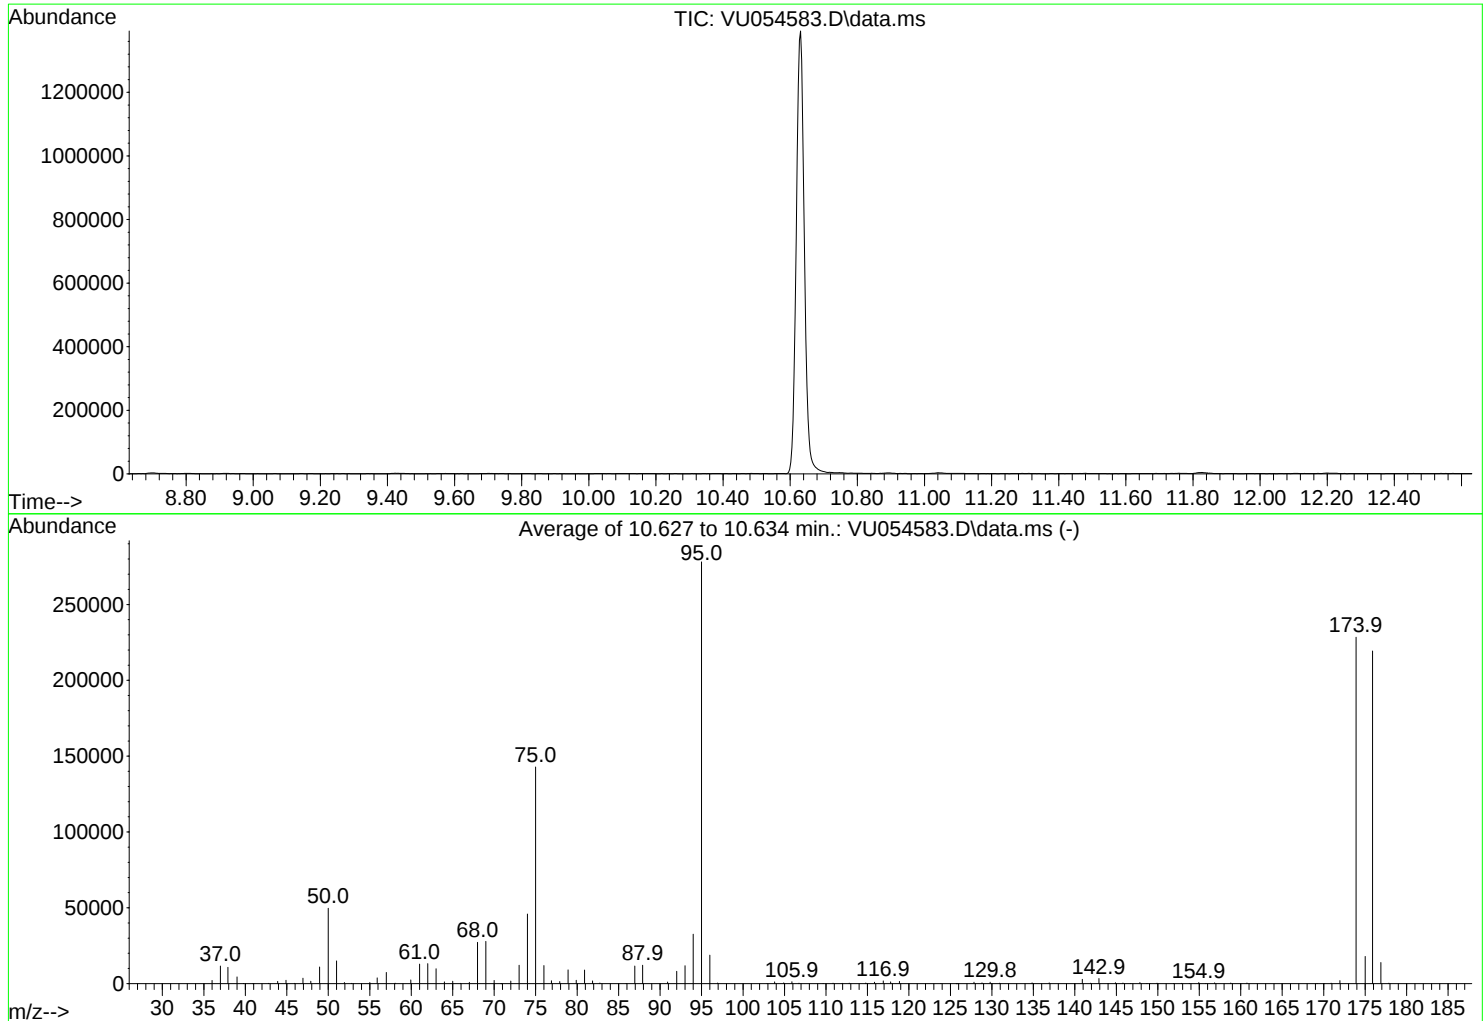

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	49685	PASS
75	95	30	80	51.4	142891	PASS
95	95	100	100	100.0	278144	PASS
96	95	5	9	6.8	18819	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.1	228459	PASS
175	174	5	9	7.9	17984	PASS
176	174	95	101	96.0	219392	PASS
177	176	5	9	6.4	13983	PASS

m/z	Abundance
35.70	105.0
39.80	252.0
43.90	606.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
36.00	2077.0
37.00	11894.0
37.90	11104.0
39.00	4824.0
39.80	429.0
42.70	302.0
43.90	2025.0
44.90	2141.0
45.90	223.0
46.90	3738.0
47.90	1699.0
48.90	11341.0
50.00	50368.0
51.00	15545.0
51.90	717.0
52.80	303.0
55.00	850.0
55.90	4046.0
57.00	7441.0
58.00	360.0
60.00	2538.0
61.00	12963.0
62.00	13414.0
63.00	10242.0
64.00	1309.0
65.00	1659.0
66.00	263.0
67.00	942.0
68.00	26920.0
69.00	27872.0
70.00	2275.0
70.80	120.0
72.00	1832.0
73.00	12316.0
74.00	46664.0
75.00	144512.0
76.00	12389.0
76.90	1916.0
77.90	1366.0
78.90	9075.0
79.90	2235.0
80.90	9518.0
81.80	1848.0
82.80	349.0
87.00	11564.0
87.90	12330.0
90.90	1114.0
92.00	8478.0
93.00	12318.0
94.00	32720.0
95.00	283648.0
96.00	19120.0
97.00	486.0
102.90	206.0
103.80	1244.0
104.90	493.0
105.90	1238.0
106.70	319.0
109.70	130.0
110.80	357.0
112.00	205.0
112.80	241.0
114.80	401.0
115.80	932.0
116.90	1865.0
117.80	1132.0
118.90	1559.0
123.90	117.0
125.70	100.0
127.90	980.0
128.80	590.0
129.80	886.0
131.00	336.0
134.80	599.0
136.90	609.0
140.00	185.0
140.90	2828.0
141.90	298.0
142.90	3539.0
144.00	138.0
144.90	602.0
145.80	486.0
146.80	162.0
147.80	740.0
148.70	202.0
149.00	211.0
149.90	327.0
151.90	135.0
152.80	223.0
153.80	153.0
155.00	806.0
156.80	498.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

158.80	503.0
160.80	432.0
170.00	114.0
170.90	326.0
172.00	2052.0
173.90	226176.0
175.00	18136.0
175.90	217728.0
176.90	13941.0
177.80	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
36.00	2103.0
37.00	11972.0
37.90	10995.0
39.00	4660.0
39.80	416.0
42.80	242.0
44.00	2084.0
44.90	2365.0
46.00	233.0
46.90	3726.0
47.90	1692.0
48.90	11223.0
50.00	51192.0
51.00	15354.0
52.00	728.0
52.80	240.0
55.00	783.0
55.90	3812.0
57.00	7657.0
58.10	357.0
59.90	2504.0
61.00	13185.0
62.00	13726.0
63.00	10015.0
64.00	1223.0
65.00	1654.0
65.90	171.0
67.00	874.0
68.00	28104.0
69.00	28872.0
70.00	2220.0
72.00	1773.0
73.00	12549.0
74.00	47344.0
75.00	147264.0
76.00	12333.0
76.90	1944.0
77.90	1437.0
78.90	9471.0
79.90	2315.0
80.90	9182.0
81.90	1842.0
82.70	435.0
86.90	11826.0
87.90	12697.0
90.90	1078.0
92.00	8329.0
93.00	12095.0
94.00	33480.0
95.00	286656.0
96.00	19264.0
97.00	439.0
102.90	172.0
103.80	1232.0
104.90	492.0
105.90	1282.0
106.80	324.0
109.70	123.0
110.80	402.0
112.00	195.0
112.80	325.0
114.80	376.0
115.90	972.0
116.90	1911.0
117.80	1199.0
118.80	1518.0
123.80	151.0
127.90	947.0
128.80	590.0
129.80	1012.0
130.90	363.0
134.80	560.0
136.90	615.0
140.90	2916.0
141.90	318.0
142.90	3499.0
144.00	152.0
144.90	645.0
145.80	413.0
146.80	159.0
147.90	725.0
148.70	164.0
149.10	125.0
149.90	334.0
151.90	172.0
152.90	172.0
153.80	171.0
155.00	825.0
155.80	129.0
156.80	571.0
158.80	471.0
160.70	416.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

169.20	126.0
170.00	142.0
170.90	315.0
172.00	2132.0
173.90	235200.0
175.00	18840.0
175.90	225856.0
176.90	14423.0
177.90	292.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

m/z	Abundance
36.00	2022.0
37.00	10931.0
37.90	10183.0
39.00	4000.0
39.80	394.0
40.90	102.0
42.90	228.0
44.00	2044.0
44.90	2300.0
45.90	290.0
47.00	3224.0
47.90	1482.0
49.00	10306.0
50.00	47496.0
51.00	14161.0
52.00	764.0
53.00	194.0
55.00	582.0
55.90	3442.0
57.00	7111.0
58.10	283.0
59.90	2309.0
61.00	12382.0
62.00	12443.0
63.00	9155.0
64.00	1105.0
65.00	1467.0
65.90	125.0
67.00	859.0
68.00	26744.0
69.00	26688.0
70.00	2028.0
72.00	1504.0
73.00	11689.0
74.00	43800.0
75.00	136896.0
76.00	11184.0
76.90	1859.0
77.90	1315.0
78.90	8664.0
79.90	2192.0
80.90	8144.0
81.90	1807.0
82.80	408.0
85.90	470.0
86.90	11561.0
87.90	11493.0
90.90	1043.0
92.00	7524.0
93.00	11096.0
94.00	31560.0
95.00	264128.0
96.00	18072.0
96.90	434.0
102.90	111.0
103.80	1108.0
104.90	471.0
105.90	1187.0
106.80	271.0
109.60	140.0
110.90	348.0
111.80	205.0
112.80	328.0
114.80	384.0
115.90	927.0
116.90	1750.0
117.80	1106.0
118.80	1476.0
123.80	169.0
125.90	102.0
127.80	883.0
128.80	530.0
129.80	1027.0
130.90	395.0
134.90	452.0
136.90	538.0
140.00	199.0
140.90	2725.0
141.90	314.0
142.90	3096.0
144.00	147.0
144.90	576.0
145.80	368.0
146.70	130.0
147.90	734.0
149.90	339.0
151.90	148.0
152.90	172.0
153.80	193.0
154.90	740.0
155.80	163.0
156.90	614.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021

158.80	364.0
160.70	385.0
169.20	123.0
170.10	124.0
170.90	259.0
171.90	1947.0
173.90	224000.0
175.00	16976.0
175.90	214592.0
176.90	13586.0
177.90	304.0

Instrument :
MSVOA_U
ClientSampleId :
BFB021