

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059344.D
Acq On : 19 Jun 2024 11:33
Operator : MD/SY
Sample : P2898-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G83

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	347	360	378	rVB	221665	359073	3.69%	2.559%
2	2.560	381	395	408	rBV	93383	152841	1.57%	1.089%
3	2.766	442	459	510	rBV	4370371	9739201	100.00%	69.402%
4	4.618	1022	1035	1066	rBV	81685	220130	2.26%	1.569%
5	5.055	1157	1171	1197	rBV	101125	239788	2.46%	1.709%
6	5.721	1359	1378	1407	rBV2	191356	511771	5.25%	3.647%
7	6.245	1529	1541	1567	rBV	165132	325202	3.34%	2.317%
8	6.685	1665	1678	1697	rBV	125238	246372	2.53%	1.756%
9	7.894	2041	2054	2067	rBV	218678	379529	3.90%	2.705%
10	8.628	2272	2282	2313	rBV	260031	523298	5.37%	3.729%
11	9.415	2512	2527	2546	rBV	246422	423885	4.35%	3.021%
12	10.750	2929	2942	2965	rBV	103998	171874	1.76%	1.225%
13	11.807	3259	3271	3292	rBV	226843	380549	3.91%	2.712%
14	12.190	3378	3390	3408	rBV	217552	359532	3.69%	2.562%




Sum of corrected areas: 14033045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059344.D
Acq On : 19 Jun 2024 11:33
Operator : MD/SY
Sample : P2898-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

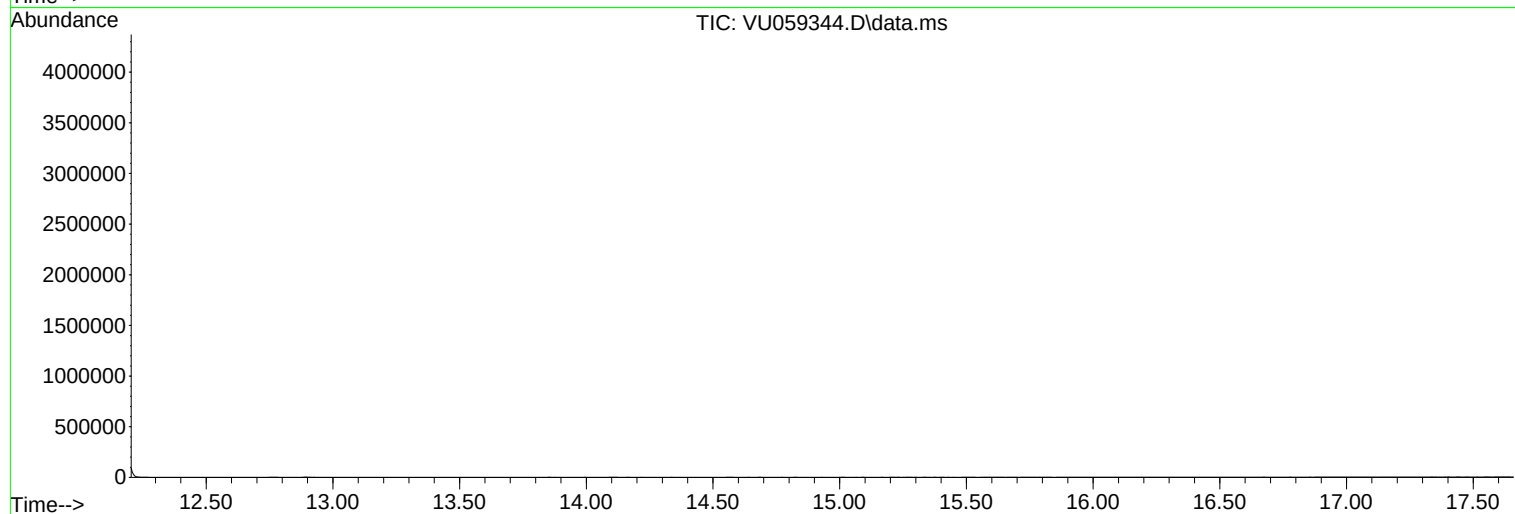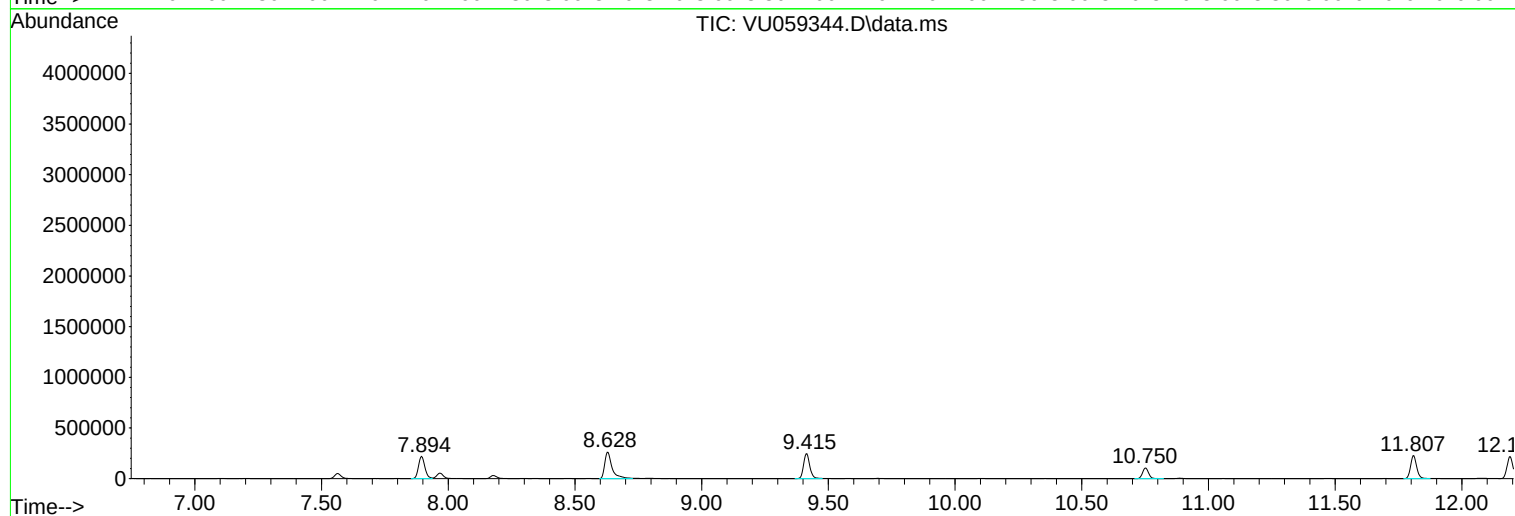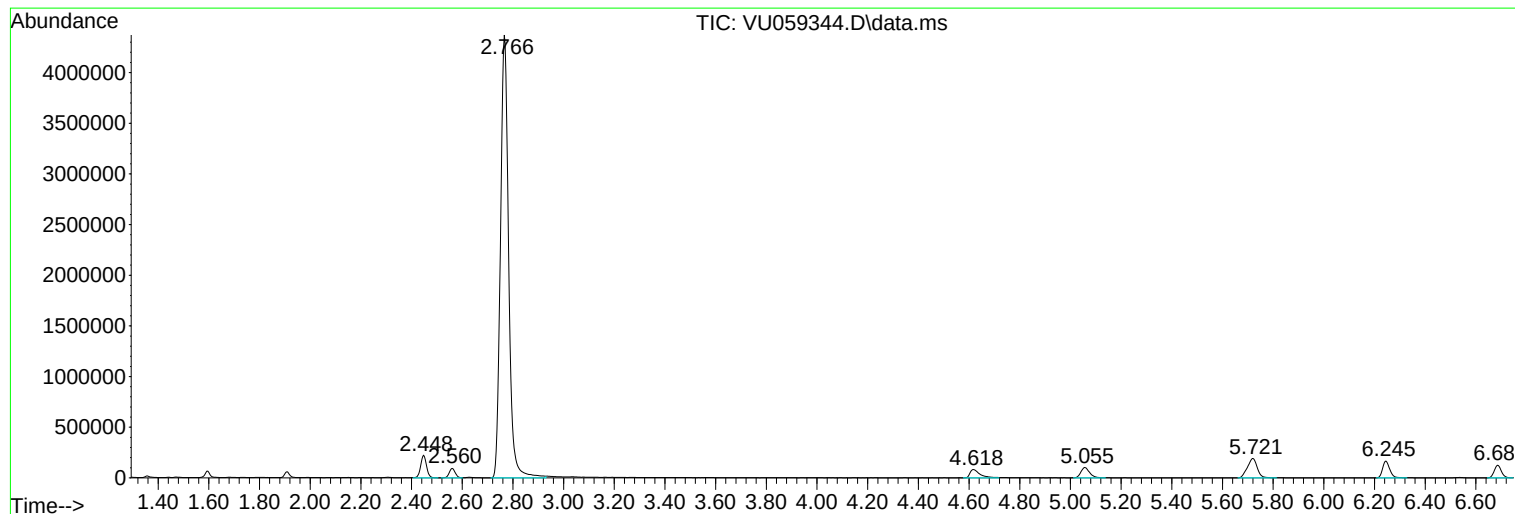

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059344.D
Acq On : 19 Jun 2024 11:33
Operator : MD/SY
Sample : P2898-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G83










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	5.52 ug/L	359073	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	72
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	64
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	42
4			2-Chloroethanol	80	C2H5ClO	000107-07-3	4
5			Hydrogen azide	43	HN3	007782-79-8	4

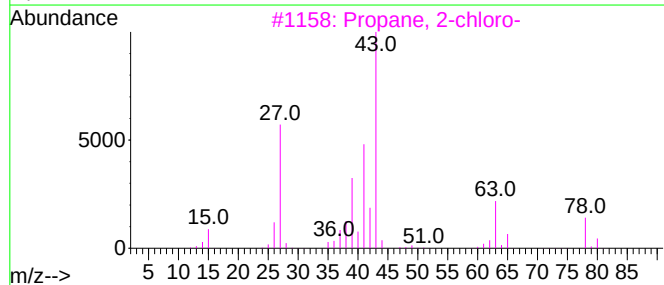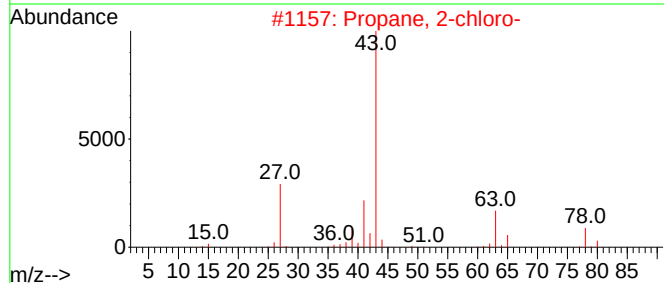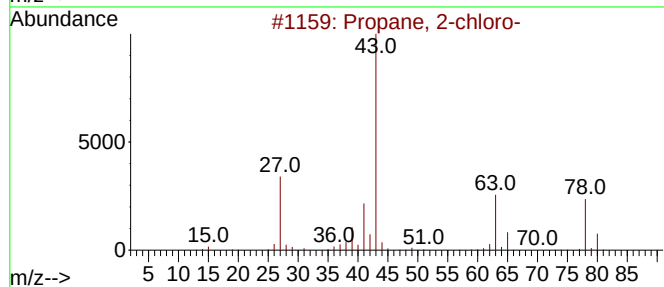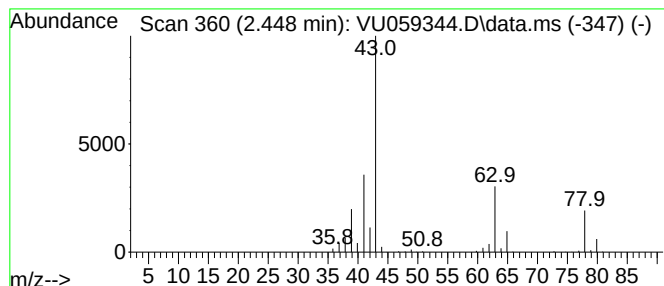

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059344.D
Acq On : 19 Jun 2024 11:33
Operator : MD/SY
Sample : P2898-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G83










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.766	149.74 ug/L	9739200	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

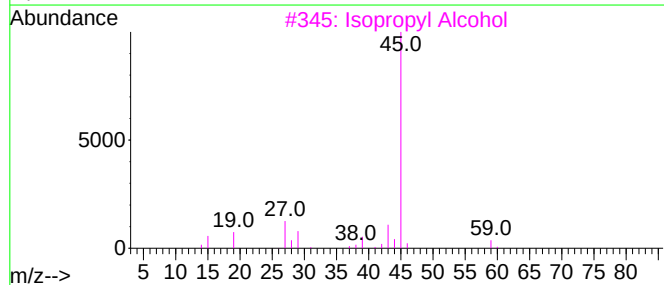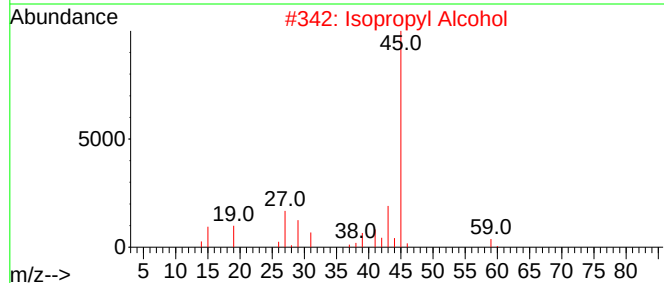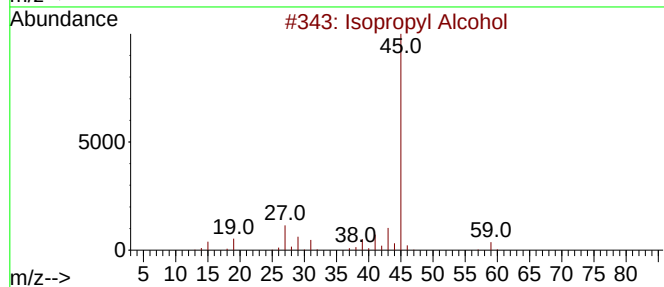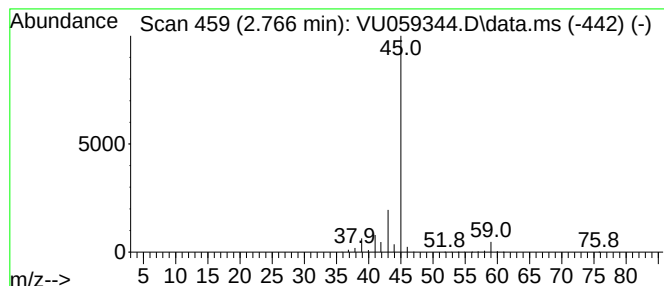

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059344.D
Acq On : 19 Jun 2024 11:33
Operator : MD/SY
Sample : P2898-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G83

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	5.5	ug/L	359073	1	6.245	325202	5.0
Isopropyl Alcohol	2.766	149.7	ug/L	9739200	1	6.245	325202	5.0