

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
 Data File : VU059345.D
 Acq On : 19 Jun 2024 11:57
 Operator : MD/SY
 Sample : P2898-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G84

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	84	95	110	rBV3	115568	159076	1.53%	0.840%
2	2.448	348	360	378	rVB	438312	707887	6.83%	3.736%
3	2.560	382	395	408	rBV2	101227	171130	1.65%	0.903%
4	2.772	442	461	522	rBV	4030615	10368926	100.00%	54.731%
5	4.656	1023	1047	1102	rBV2	1493267	3604847	34.77%	19.028%
6	5.058	1155	1172	1195	rBV	104660	249828	2.41%	1.319%
7	5.721	1359	1378	1408	rBV2	196096	536245	5.17%	2.831%
8	6.245	1528	1541	1566	rBV	175131	337922	3.26%	1.784%
9	6.537	1620	1632	1651	rBV	135840	260106	2.51%	1.373%
10	6.685	1665	1678	1703	rBV	125235	248230	2.39%	1.310%
11	7.894	2041	2054	2068	rBV	223994	388289	3.74%	2.050%
12	8.627	2271	2282	2319	rBV2	268468	541486	5.22%	2.858%
13	9.415	2512	2527	2551	rBV	254068	432823	4.17%	2.285%
14	10.753	2931	2943	2959	rBV2	105517	172113	1.66%	0.908%
15	11.811	3260	3272	3290	rBV	238163	393937	3.80%	2.079%
16	12.190	3378	3390	3407	rVB	223588	372383	3.59%	1.966%




Sum of corrected areas: 18945228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059345.D
Acq On : 19 Jun 2024 11:57
Operator : MD/SY
Sample : P2898-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

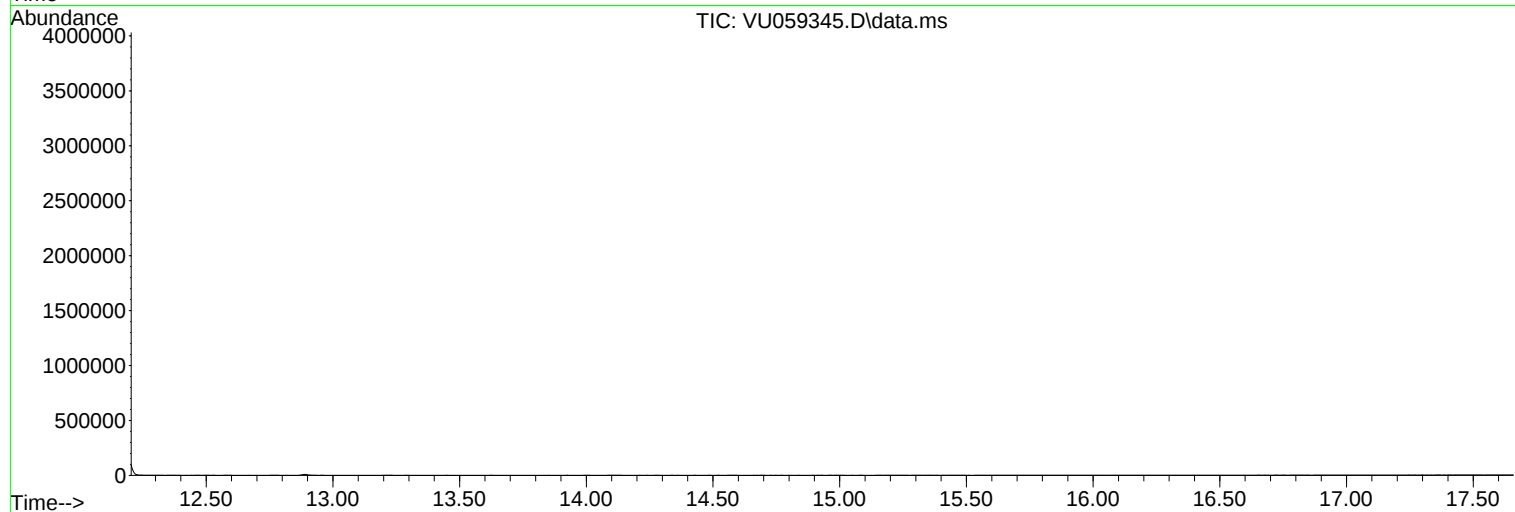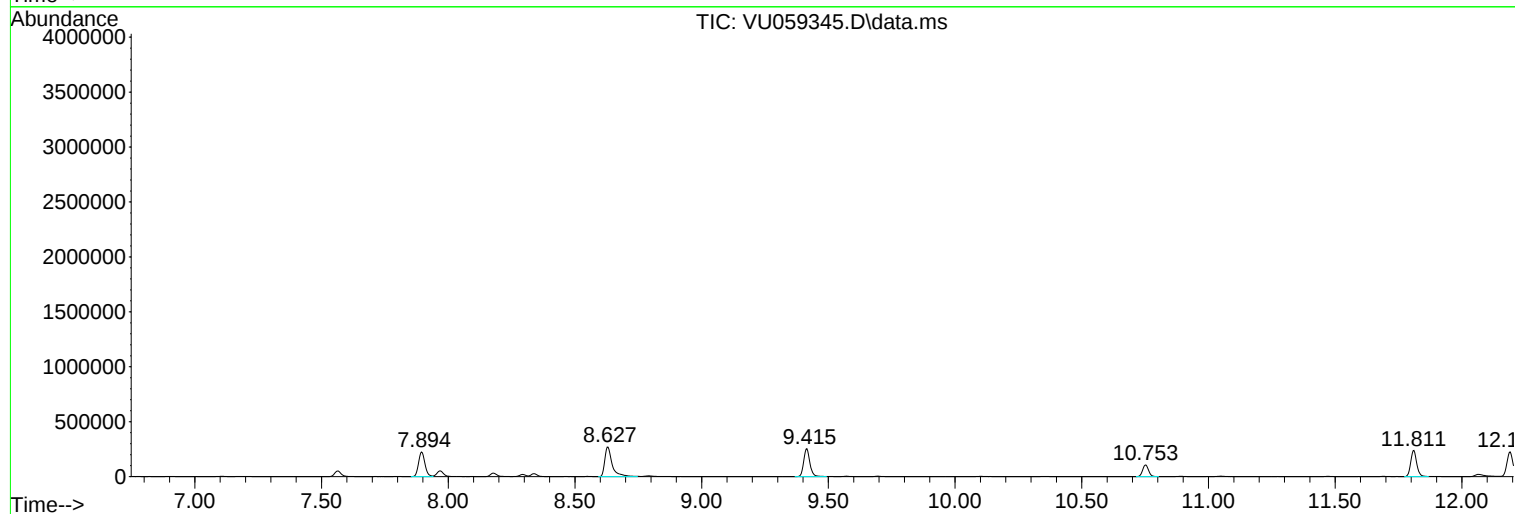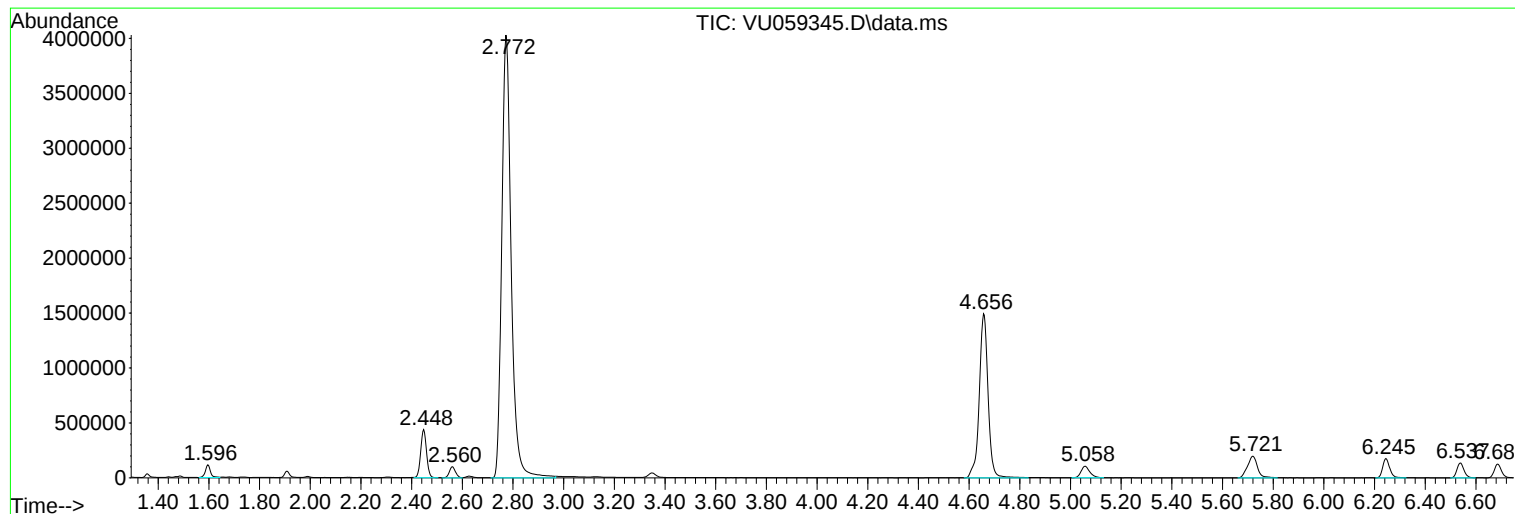

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059345.D
Acq On : 19 Jun 2024 11:57
Operator : MD/SY
Sample : P2898-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G84







Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	10.47 ug/L	707887	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

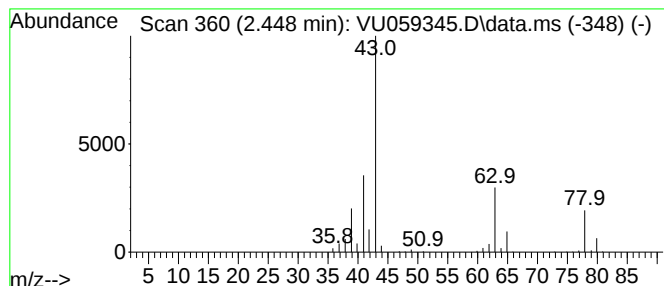

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059345.D
Acq On : 19 Jun 2024 11:57
Operator : MD/SY
Sample : P2898-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G84










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.772	153.42 ug/L	10368900	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	64

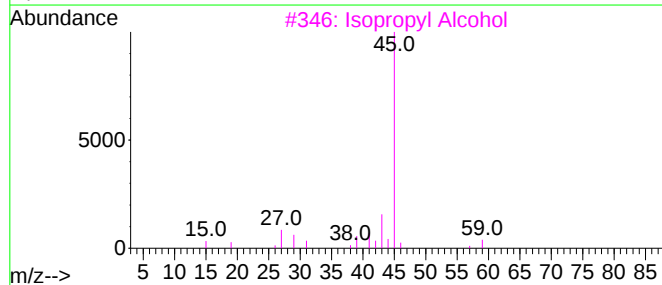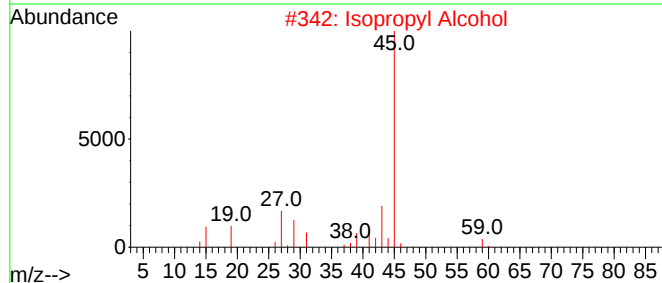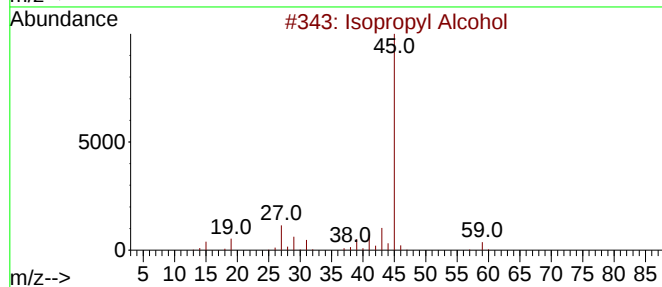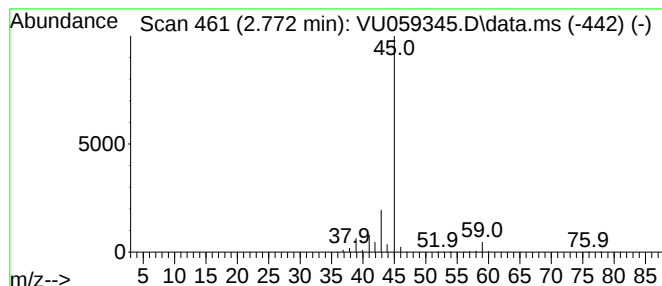

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059345.D
Acq On : 19 Jun 2024 11:57
Operator : MD/SY
Sample : P2898-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	10.5	ug/L	707887	1	6.245	337922	5.0
Isopropyl Alcohol	2.772	153.4	ug/L	10368900	1	6.245	337922	5.0