

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
 Data File : VU059346.D
 Acq On : 19 Jun 2024 12:20
 Operator : MD/SY
 Sample : P2898-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1G85

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	85	96	108	rBV2	163308	209348	2.44%	1.192%
2	2.448	349	360	374	rVB	118058	193854	2.26%	1.104%
3	2.560	381	395	405	rBV2	73868	130113	1.51%	0.741%
4	2.747	438	453	521	rBV	4633905	8596316	100.00%	48.938%
5	4.657	1023	1047	1085	rBV	1766545	4179615	48.62%	23.794%
6	5.059	1154	1172	1199	rVB	70631	164122	1.91%	0.934%
7	5.721	1357	1378	1414	rBV2	133561	391854	4.56%	2.231%
8	6.245	1529	1541	1565	rBV2	117355	227709	2.65%	1.296%
9	6.538	1618	1632	1663	rBV	850490	1608180	18.71%	9.155%
10	6.685	1666	1678	1692	rBV2	88799	167136	1.94%	0.951%
11	7.894	2043	2054	2068	rBV	147468	256130	2.98%	1.458%
12	8.628	2272	2282	2322	rBV	243514	497531	5.79%	2.832%
13	9.415	2515	2527	2552	rBV	170582	292678	3.40%	1.666%
14	10.753	2930	2943	2957	rBV	91595	147776	1.72%	0.841%
15	11.811	3260	3272	3292	rBV	154718	259763	3.02%	1.479%
16	12.190	3378	3390	3407	rBV	145755	243685	2.83%	1.387%




Sum of corrected areas: 17565810

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059346.D
Acq On : 19 Jun 2024 12:20
Operator : MD/SY
Sample : P2898-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

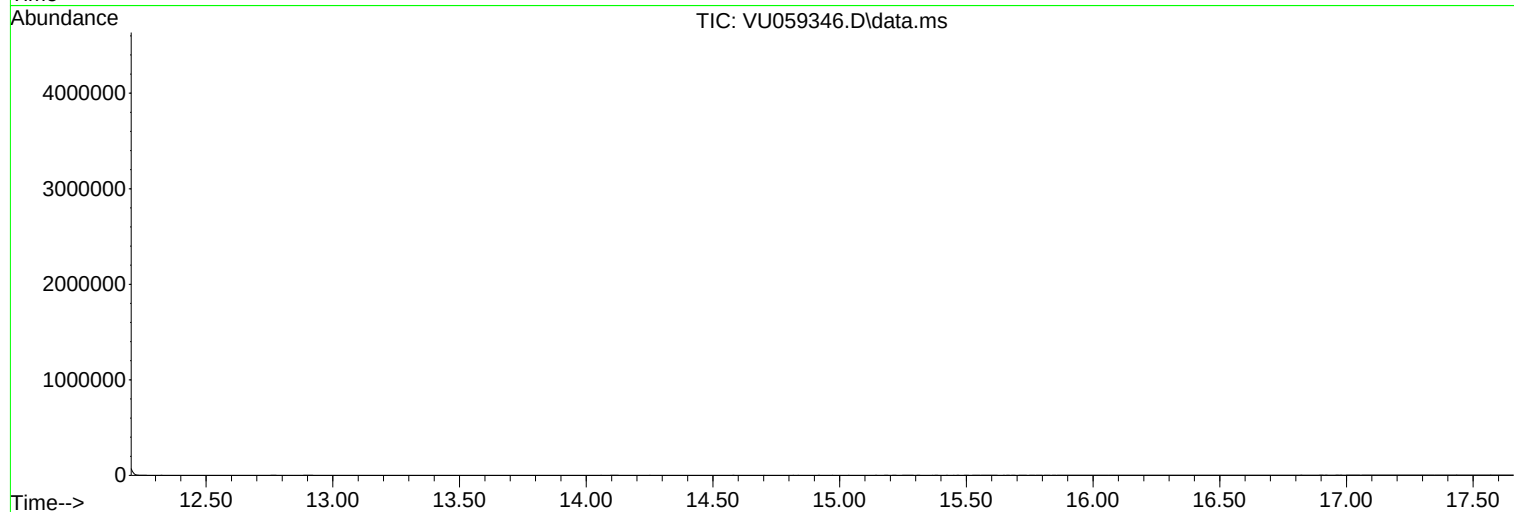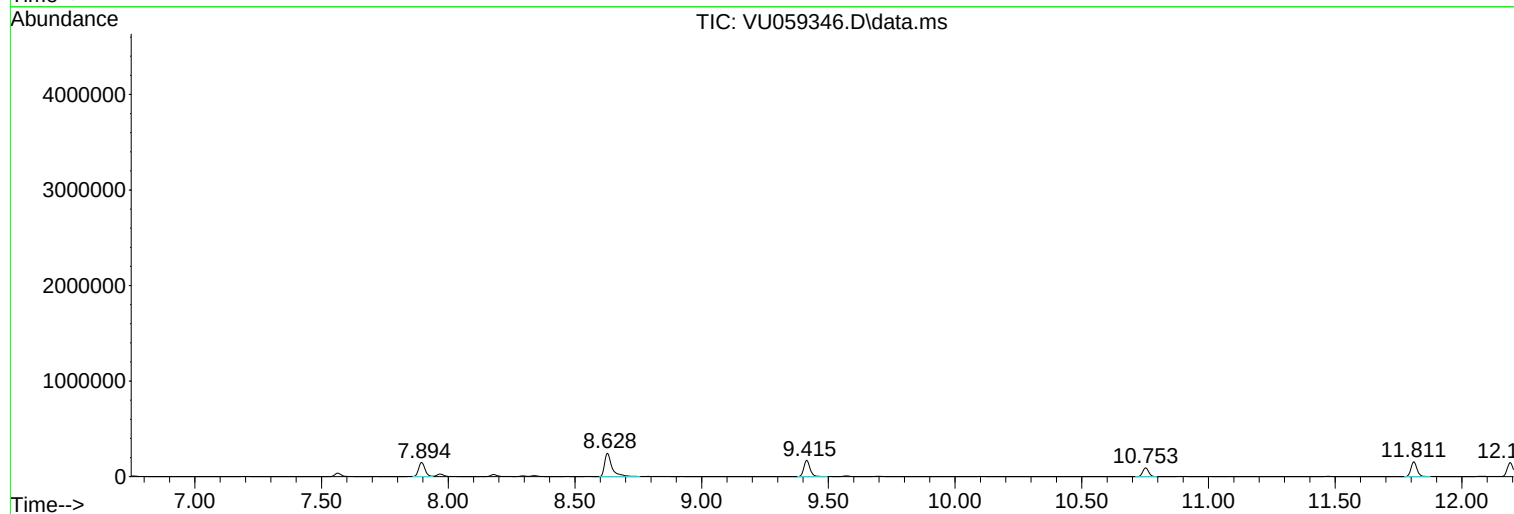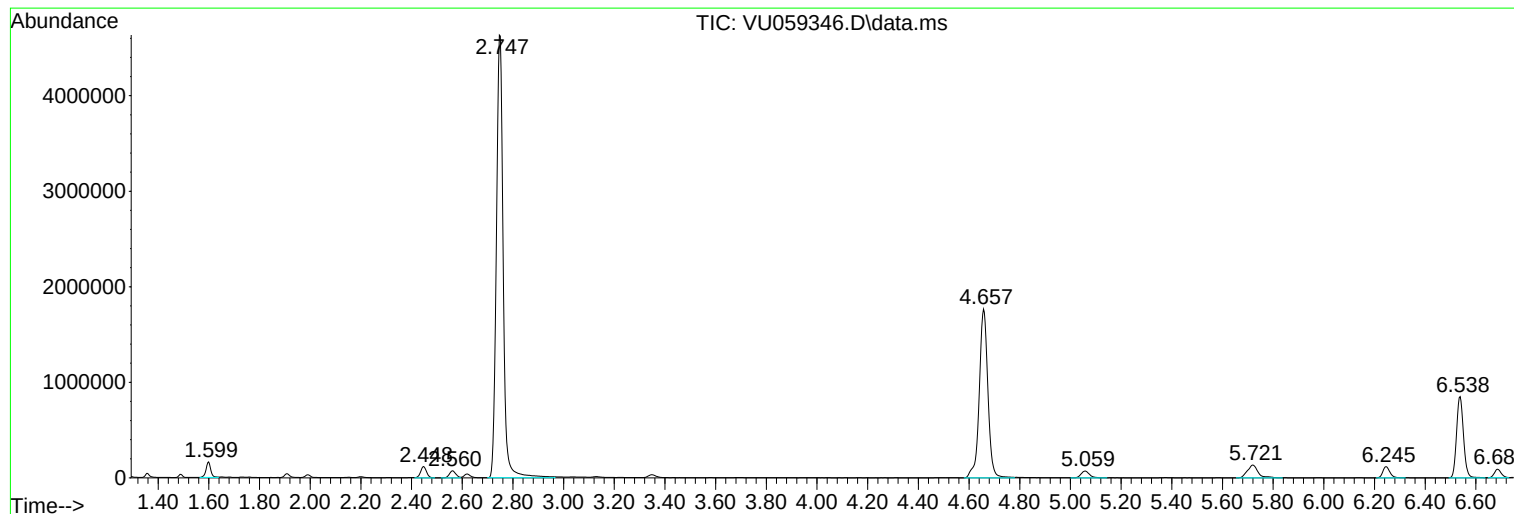

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059346.D
Acq On : 19 Jun 2024 12:20
Operator : MD/SY
Sample : P2898-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	4.26 ug/L	193854	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	83
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	50
4	2-Chloroethanol			80	C2H5ClO	000107-07-3	4
5	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	4

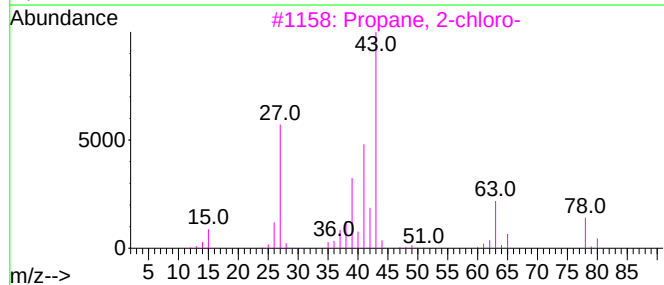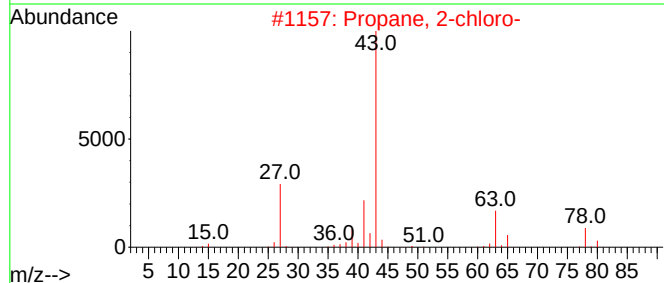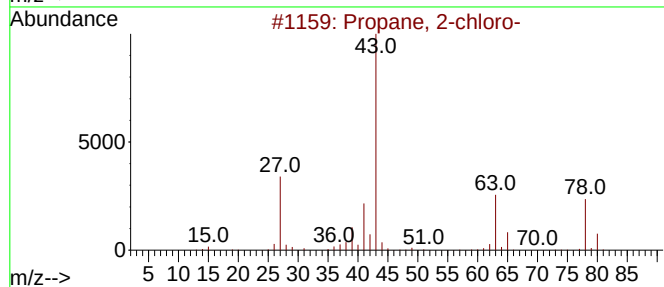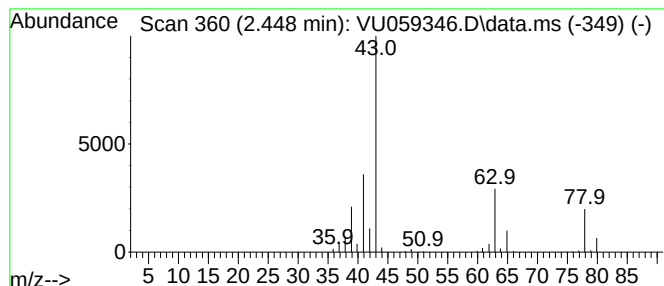

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059346.D
Acq On : 19 Jun 2024 12:20
Operator : MD/SY
Sample : P2898-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.747	188.76 ug/L	8596320	1,4-Difluorobenzene	6.245

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

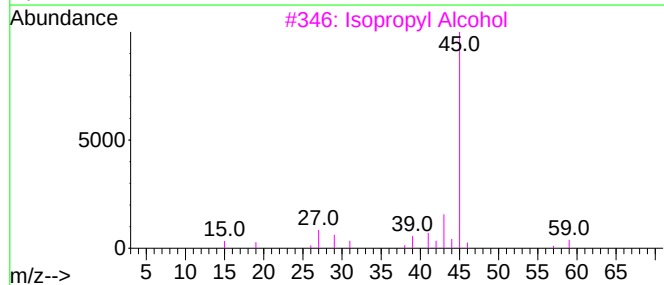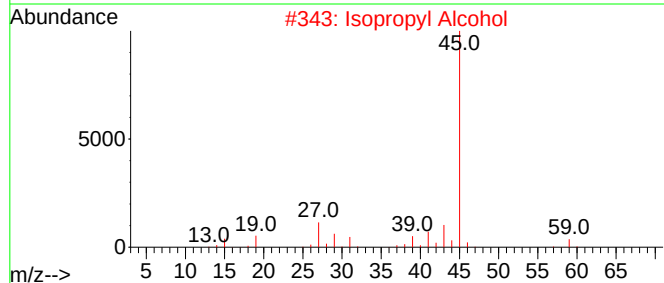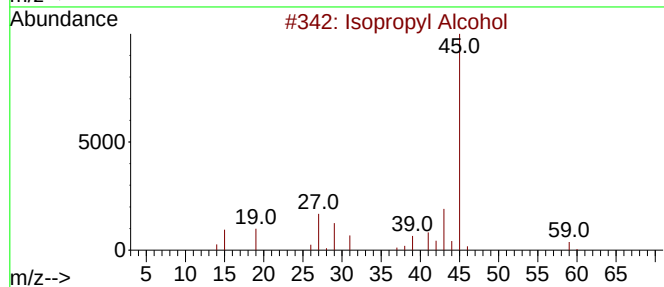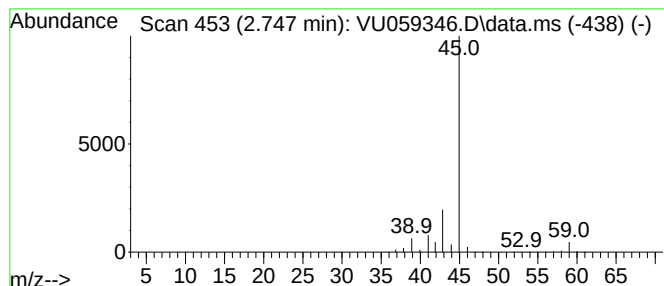

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059346.D
Acq On : 19 Jun 2024 12:20
Operator : MD/SY
Sample : P2898-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1G85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	4.3	ug/L	193854	1	6.245	227709	5.0
Isopropyl Alcohol	2.747	188.8	ug/L	8596320	1	6.245	227709	5.0