

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
 Data File : VU059359.D
 Acq On : 19 Jun 2024 17:29
 Operator : MD/SY
 Sample : P2960-01 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAS7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU059359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	110	rBV	56639	70226	10.54%	1.435%
2	1.907	183	192	206	rBV	53957	72868	10.93%	1.489%
3	2.560	380	395	410	rBV	90713	147087	22.07%	3.005%
4	3.042	533	545	558	rBV3	10045	19097	2.87%	0.390%
5	3.351	629	641	655	rBV3	3973	7922	1.19%	0.162%
6	4.656	1026	1047	1073	rBV2	211225	666395	100.00%	13.615%
7	5.055	1156	1171	1200	rBV	96960	216258	32.45%	4.418%
8	5.721	1358	1378	1403	rBV2	182358	479213	71.91%	9.791%
9	6.245	1528	1541	1562	rBV	165089	318054	47.73%	6.498%
10	6.541	1620	1633	1652	rBV4	41299	82405	12.37%	1.684%
11	6.685	1663	1678	1705	rBV2	115878	230771	34.63%	4.715%
12	7.563	1936	1951	1968	rBV2	45192	79718	11.96%	1.629%
13	7.894	2040	2054	2073	rBV	199296	351196	52.70%	7.175%
14	8.180	2133	2143	2155	rBV2	27502	46915	7.04%	0.959%
15	8.550	2245	2258	2273	rBV	196636	330214	49.55%	6.746%
16	8.631	2273	2283	2319	rVV	251392	508536	76.31%	10.390%
17	9.415	2515	2527	2549	rBV	245428	419443	62.94%	8.570%
18	10.753	2931	2943	2966	rVB	99912	162239	24.35%	3.315%
19	11.810	3260	3272	3291	rBV	216442	361881	54.30%	7.393%
20	12.190	3374	3390	3414	rBV	191773	324160	48.64%	6.623%




Sum of corrected areas: 4894598

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059359.D
Acq On : 19 Jun 2024 17:29
Operator : MD/SY
Sample : P2960-01 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

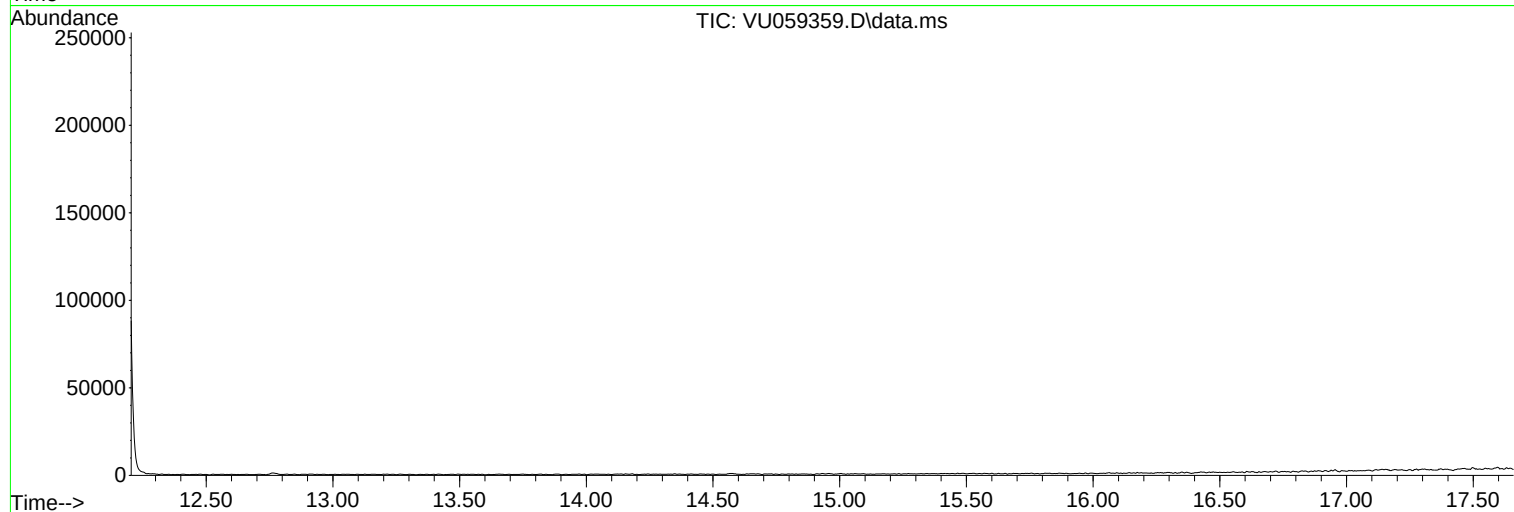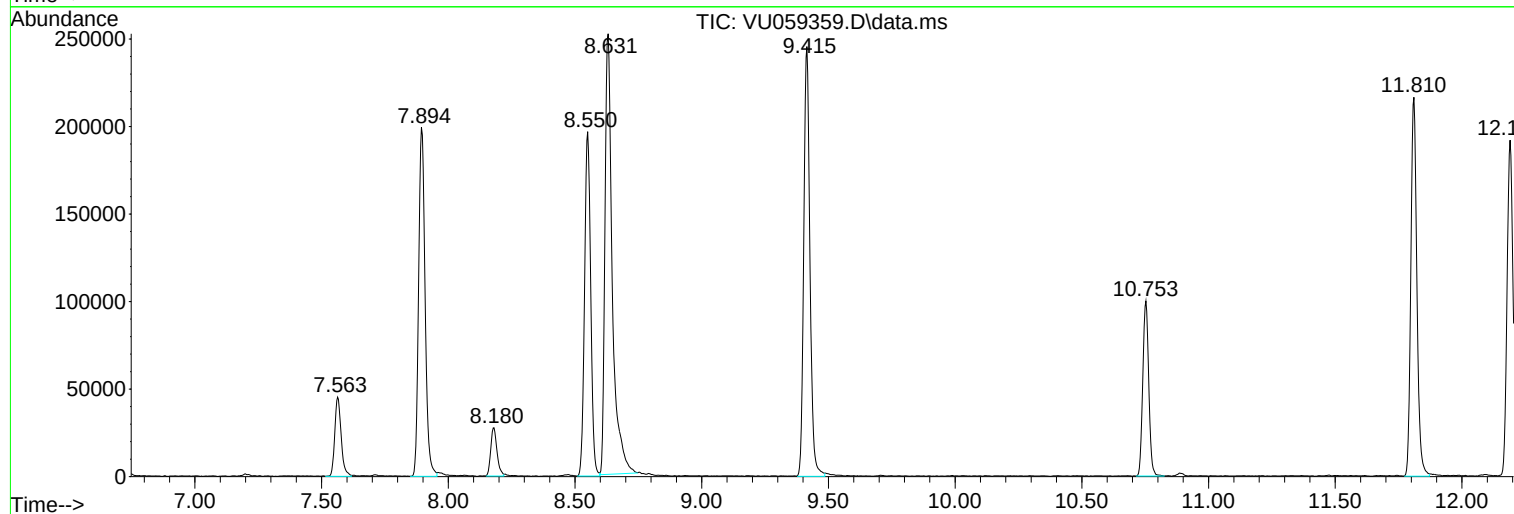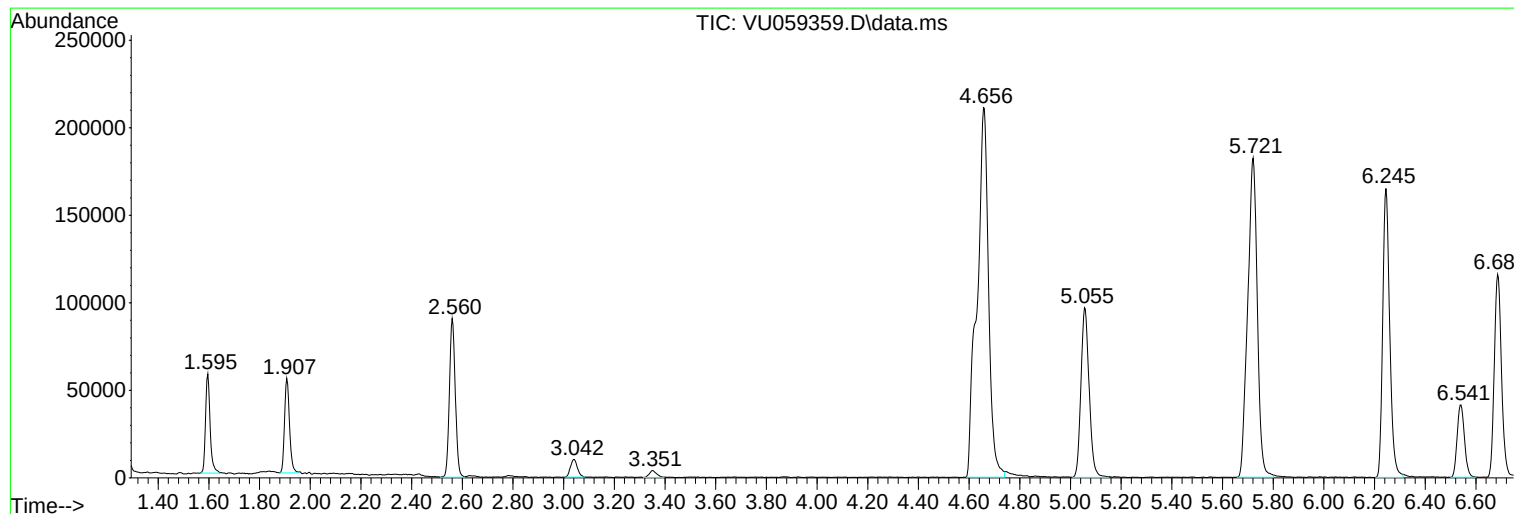

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059359.D
Acq On : 19 Jun 2024 17:29
Operator : MD/SY
Sample : P2960-01 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059359.D
Acq On : 19 Jun 2024 17:29
Operator : MD/SY
Sample : P2960-01 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc