

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
 Data File : VU059360.D
 Acq On : 19 Jun 2024 17:54
 Operator : MD/SY
 Sample : P2960-02 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAS8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU059360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	86	95	115	rBV	55550	72633	8.17%	1.341%
2	1.907	182	192	211	rBV	54250	74189	8.34%	1.370%
3	2.560	384	395	412	rBV	88054	146904	16.52%	2.713%
4	3.039	534	544	558	rBV3	9307	17350	1.95%	0.320%
5	4.656	1025	1047	1077	rBV3	198043	631898	71.06%	11.668%
6	5.055	1156	1171	1200	rBV2	94083	212934	23.95%	3.932%
7	5.721	1358	1378	1400	rBV2	184597	480117	53.99%	8.865%
8	6.245	1525	1541	1564	rBV	164757	320922	36.09%	5.926%
9	6.537	1621	1632	1650	rBV4	43021	84137	9.46%	1.554%
10	6.685	1665	1678	1698	rBV2	119218	234892	26.41%	4.337%
11	7.563	1940	1951	1968	rBV	47098	81325	9.15%	1.502%
12	7.894	2042	2054	2077	rBV	198149	346803	39.00%	6.404%
13	8.177	2133	2142	2158	rBV2	27594	46280	5.20%	0.855%
14	8.550	2245	2258	2273	rBV	523091	889258	100.00%	16.420%
15	8.630	2273	2283	2325	rVB2	246688	505172	56.81%	9.328%
16	9.415	2513	2527	2555	rBV	246676	423773	47.65%	7.825%
17	10.753	2931	2943	2966	rVB	99569	160804	18.08%	2.969%
18	11.810	3260	3272	3298	rBV	216317	364118	40.95%	6.723%
19	12.190	3378	3390	3419	rBV	189775	322160	36.23%	5.949%




Sum of corrected areas: 5415669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059360.D
Acq On : 19 Jun 2024 17:54
Operator : MD/SY
Sample : P2960-02 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

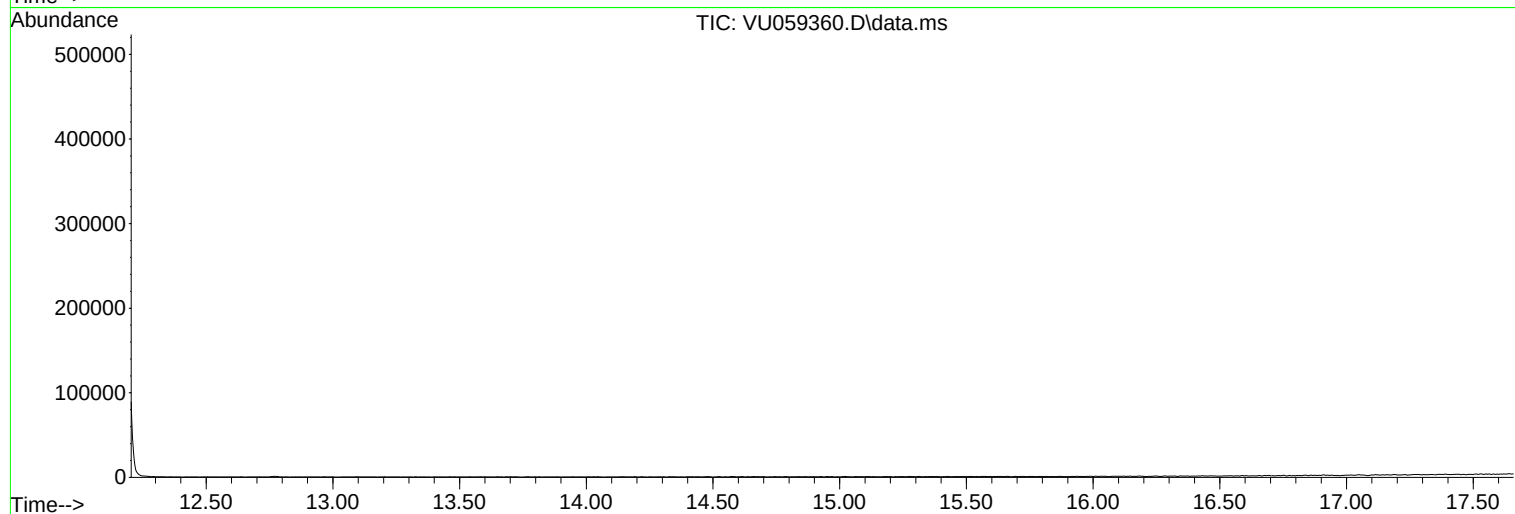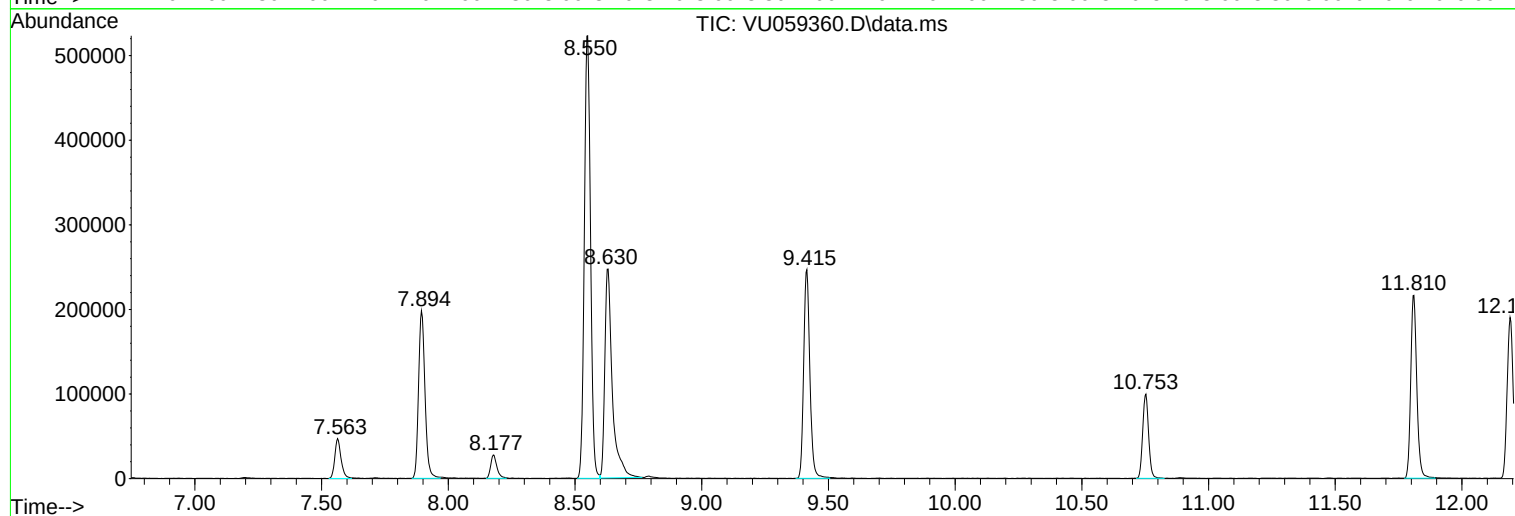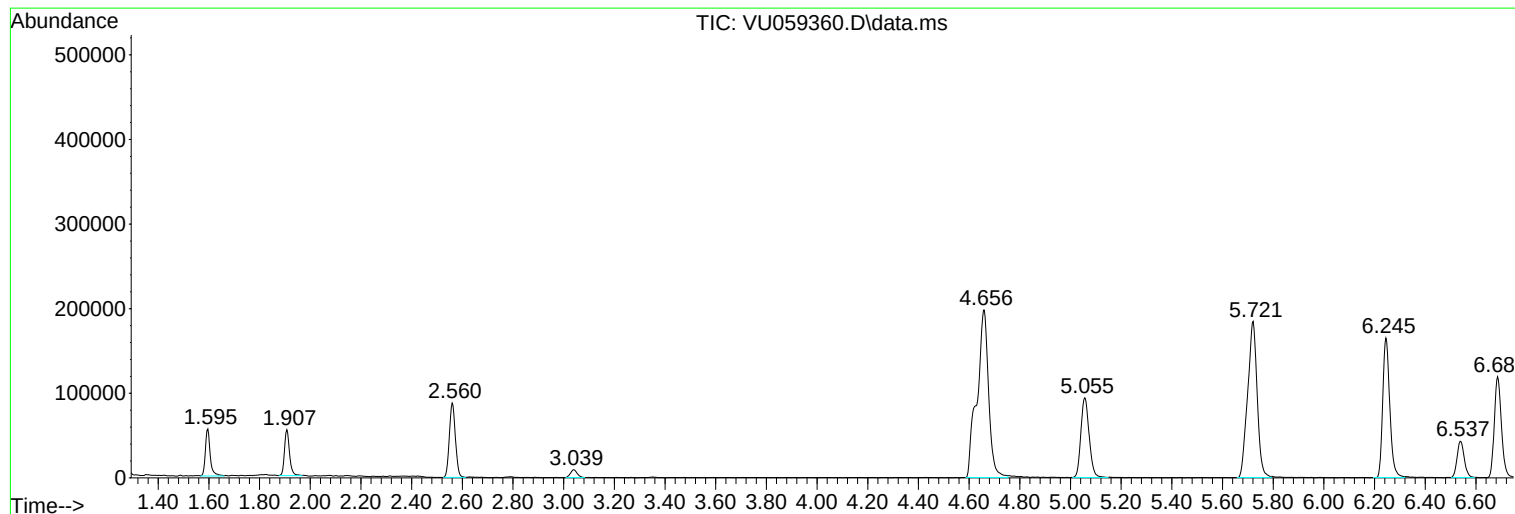

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059360.D
Acq On : 19 Jun 2024 17:54
Operator : MD/SY
Sample : P2960-02 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059360.D
Acq On : 19 Jun 2024 17:54
Operator : MD/SY
Sample : P2960-02 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc