


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU061924\
Data File : VU059336.D
Acq On : 19 Jun 2024 07:48
Operator : MD/SY
Sample : BFB163
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB163

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jun 17 12:07:46 2024

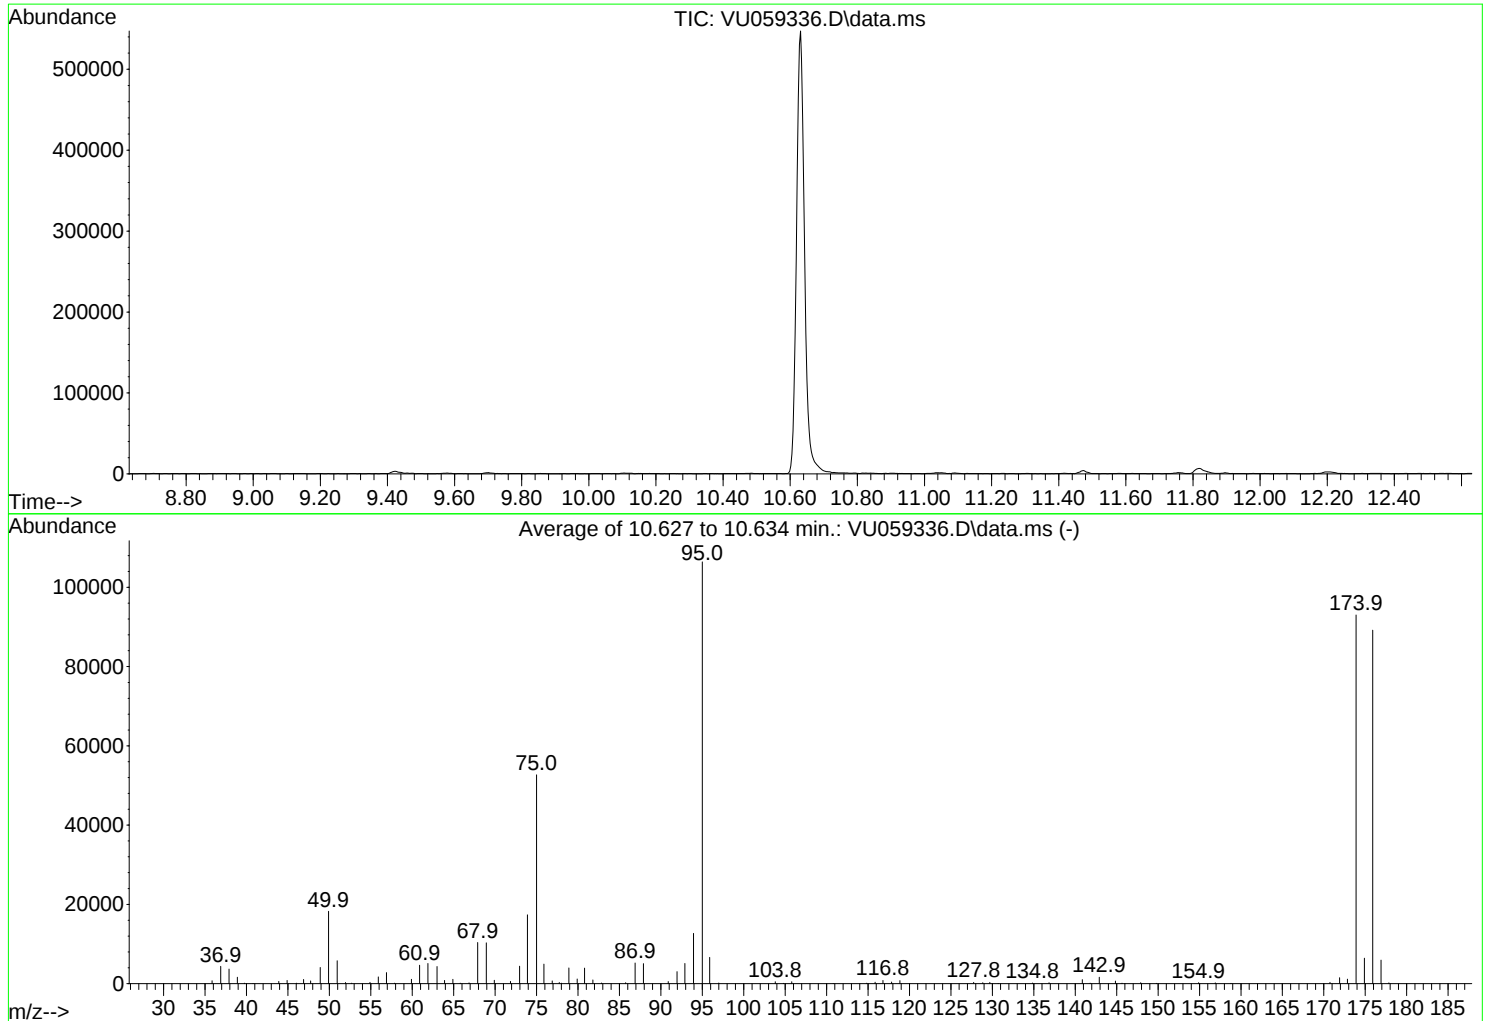

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	18232	PASS
75	95	30	80	49.5	52701	PASS
95	95	100	100	100.0	106429	PASS
96	95	5	9	6.2	6625	PASS
173	174	0.00	2	1.2	1114	PASS
174	95	50	120	87.4	93013	PASS
175	174	5	9	6.9	6433	PASS
176	174	95	101	95.9	89203	PASS
177	176	5	9	6.7	5957	PASS

m/z	Abundance
39.80	149.0
43.90	236.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
35.90	723.0
36.90	4347.0
37.90	3815.0
38.90	1677.0
39.70	199.0
40.80	100.0
43.90	857.0
44.90	770.0
46.00	132.0
46.90	1049.0
47.80	674.0
48.90	4361.0
49.90	18304.0
50.90	5953.0
51.90	278.0
52.70	124.0
54.90	308.0
55.90	1726.0
56.90	2737.0
57.90	113.0
59.90	1156.0
60.90	4523.0
61.90	5170.0
63.00	4488.0
63.90	842.0
64.90	1097.0
65.80	132.0
66.90	230.0
67.90	10589.0
69.00	10508.0
69.90	842.0
71.80	635.0
72.90	4619.0
73.90	17288.0
75.00	52928.0
75.90	5155.0
76.90	683.0
77.80	424.0
78.90	4164.0
79.90	1154.0
80.80	3986.0
81.80	968.0
82.90	186.0
85.80	225.0
86.90	5247.0
87.90	5066.0
90.90	498.0
92.00	3062.0
92.90	5106.0
93.90	12821.0
95.00	107576.0
95.90	6643.0
97.00	182.0
103.80	484.0
104.80	110.0
105.80	515.0
114.80	105.0
115.80	395.0
116.80	885.0
117.80	423.0
118.80	817.0
127.70	300.0
128.80	227.0
129.70	337.0
130.70	125.0
134.80	137.0
136.80	233.0
140.90	1119.0
141.80	119.0
142.90	1628.0
144.90	685.0
145.70	184.0
147.90	220.0
149.80	132.0
154.90	245.0
156.90	167.0
170.80	281.0
171.90	1380.0
172.90	1141.0
173.90	91368.0
174.90	6299.0
175.90	87784.0
176.90	6049.0
177.80	232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
35.80	778.0
36.90	4515.0
37.90	3796.0
38.90	1655.0
39.80	269.0
43.90	832.0
44.90	835.0
46.10	136.0
46.90	1101.0
47.70	743.0
48.90	4149.0
49.90	18680.0
51.00	6002.0
52.00	293.0
52.70	155.0
54.90	341.0
55.90	1762.0
56.90	2902.0
57.80	127.0
59.90	1120.0
60.90	4814.0
61.90	5174.0
63.00	4537.0
63.90	837.0
64.90	1124.0
65.80	136.0
66.80	215.0
67.90	10667.0
68.90	10587.0
69.90	900.0
71.80	566.0
72.90	4548.0
73.90	17888.0
75.00	54336.0
75.90	5097.0
76.90	698.0
77.70	437.0
78.00	415.0
78.90	4075.0
79.90	1282.0
80.80	3966.0
81.80	965.0
82.90	162.0
85.70	264.0
86.90	5346.0
87.90	5200.0
90.90	560.0
91.90	3085.0
92.90	5344.0
93.90	13112.0
95.00	109816.0
95.90	6816.0
97.00	173.0
103.80	528.0
104.80	105.0
105.80	496.0
110.80	108.0
114.90	145.0
115.80	365.0
116.80	874.0
117.80	419.0
118.80	771.0
127.80	323.0
128.80	251.0
129.70	325.0
134.90	162.0
136.80	272.0
140.90	1056.0
141.80	141.0
142.90	1716.0
144.80	664.0
145.60	172.0
147.90	271.0
149.80	102.0
154.90	267.0
156.90	185.0
158.80	134.0
170.80	326.0
171.90	1571.0
172.80	1133.0
173.90	95984.0
174.90	6557.0
175.90	92152.0
176.90	6162.0
177.80	211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163

m/z	Abundance
35.80	728.0
36.90	4173.0
37.90	3427.0
38.90	1486.0
39.80	290.0
43.90	704.0
44.90	808.0
46.10	107.0
46.90	1039.0
47.80	679.0
48.90	3680.0
49.90	17712.0
51.00	5401.0
52.00	267.0
52.70	148.0
54.90	377.0
55.90	1636.0
56.90	2729.0
57.80	124.0
59.90	948.0
60.90	4630.0
61.90	4884.0
63.00	3992.0
63.90	774.0
64.90	1057.0
65.80	128.0
66.90	224.0
67.90	9902.0
68.90	9764.0
69.90	843.0
71.90	512.0
73.00	4089.0
73.90	16896.0
75.00	50840.0
75.90	4478.0
76.90	657.0
78.90	3653.0
79.90	1143.0
80.80	3752.0
81.80	842.0
82.80	144.0
85.80	231.0
86.90	5025.0
87.90	4931.0
90.90	477.0
91.90	2903.0
92.90	4857.0
94.00	12048.0
95.00	101896.0
95.90	6416.0
97.00	154.0
103.80	472.0
105.80	414.0
114.90	151.0
115.90	308.0
116.80	727.0
117.90	360.0
118.90	698.0
127.70	368.0
128.90	257.0
129.70	288.0
134.80	183.0
136.90	249.0
140.80	895.0
141.80	131.0
142.90	1521.0
144.80	596.0
146.00	177.0
147.90	266.0
154.90	272.0
156.90	201.0
158.80	153.0
170.70	320.0
171.90	1516.0
172.80	1069.0
173.90	91688.0
174.90	6443.0
175.90	87672.0
176.90	5661.0
177.90	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB163