

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062019\
 Data File : VU032901.D
 Acq On : 20 Jun 2019 14:38
 Operator : JC/SP
 Sample : K3414-20
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALN6

Quant Time: Jun 21 07:16:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 21 05:28:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	89045	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	88312	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	45668	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	23393	4.04	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.80%
7) Chloroethane-d5	1.68	69	21480	4.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.80%
11) 1,1-Dichloroethene-d2	2.27	63	39902	3.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.00%
20) 2-Butanone-d5	4.19	46	96553	59.76	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.52%
24) Chloroform-d	4.64	84	54927	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.80%
26) 1,2-Dichloroethane-d4	5.30	65	33286	6.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	122.80%
32) Benzene-d6	5.33	84	103340	4.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.20%
36) 1,2-Dichloropropane-d6	6.32	67	34577	5.11	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.20%
41) Toluene-d8	7.56	98	90768	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	7.85	79	13137	4.54	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.80%
46) 2-Hexanone-d5	8.31	63	71688	49.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.94%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	31263	5.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	109.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	41555	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Ovalue
13) Acetone	2.32	43	1886	1.504 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062019\
Data File : VU032901.D
Acq On : 20 Jun 2019 14:38
Operator : JC/SP
Sample : K3414-20
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALN6

Quant Time: Jun 21 07:16:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 21 05:28:00 2019
Response via : Initial Calibration

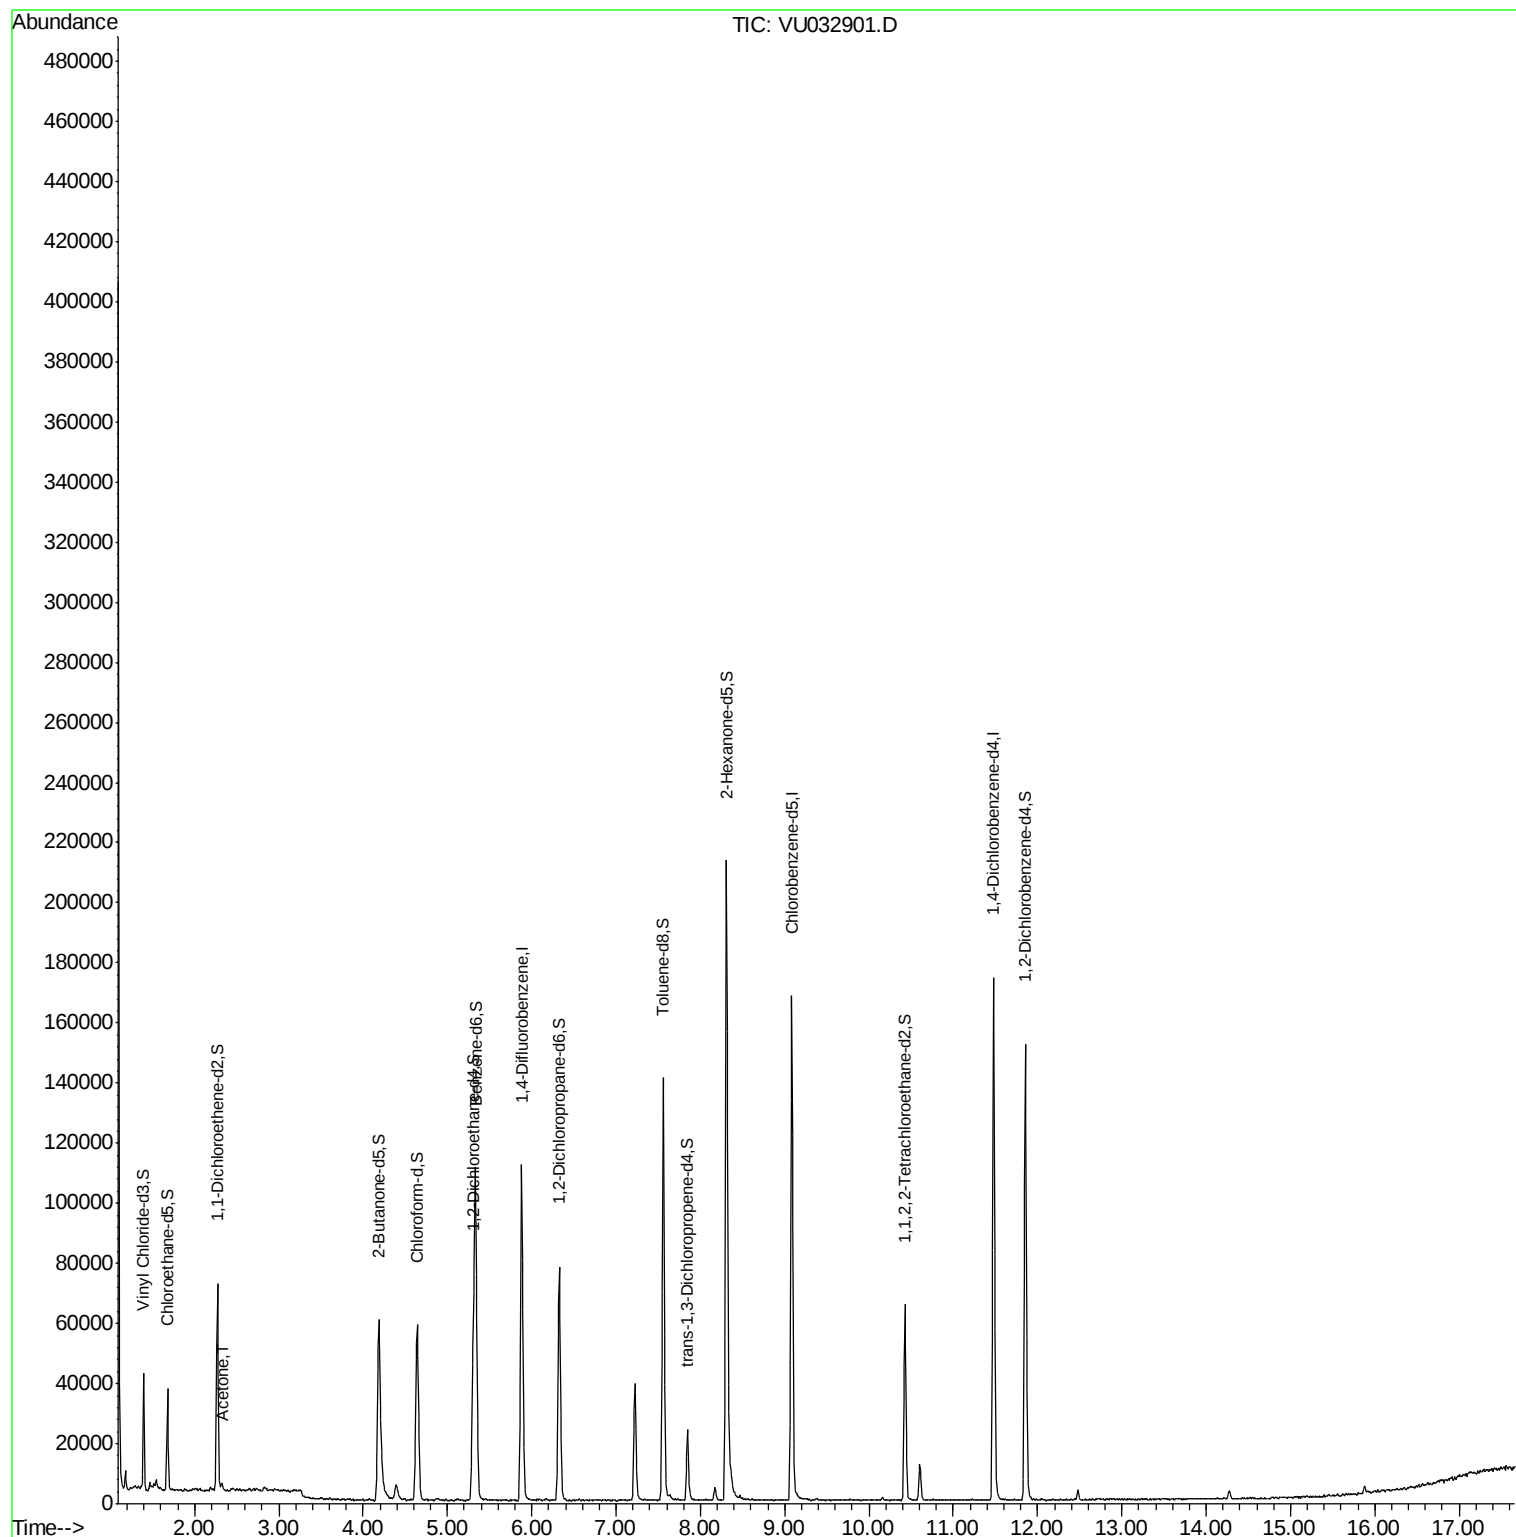

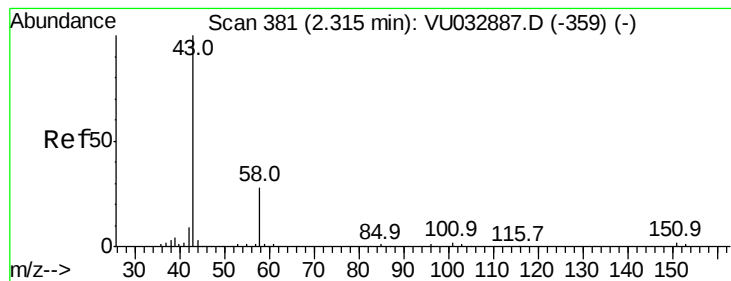

#13

Acetone

Concen: 1.504 ug/L

RT: 2.32 min Scan# 383

Delta R.T. 0.01 min

Lab File: VU032901.D

Acq: 20 Jun 2019 14:38

Instrument :

MSVOA_U

ClientSampleId :

GALN6

Tot Ion: 43 Resp: 1886

Ion Ratio Lower Upper

43 100

58 27.6 0.0 60.8

