

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062019\
 Data File : VU032907.D
 Acq On : 20 Jun 2019 18:02
 Operator : JC/SP
 Sample : K3413-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GALF1

Quant Time: Jun 21 07:50:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 21 07:36:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	84924	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	85068	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	42503	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	22356	4.05	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.00%
7) Chloroethane-d5	1.68	69	20328	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.20%
11) 1,1-Dichloroethene-d2	2.27	63	37870	3.38	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.60%
20) 2-Butanone-d5	4.18	46	99146	64.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	128.68%
24) Chloroform-d	4.64	84	53705	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.60%
26) 1,2-Dichloroethane-d4	5.31	65	32528	6.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	126.00%
32) Benzene-d6	5.33	84	101464	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.32	67	33847	5.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.80%
41) Toluene-d8	7.56	98	88575	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.85	79	13696	4.92	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.40%
46) 2-Hexanone-d5	8.31	63	73534	52.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.36%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	30651	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	39760	5.20	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	3504	2.930 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062019\
Data File : VU032907.D
Acq On : 20 Jun 2019 18:02
Operator : JC/SP
Sample : K3413-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GALF1

Quant Time: Jun 21 07:50:47 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 21 07:36:10 2019
Response via : Initial Calibration

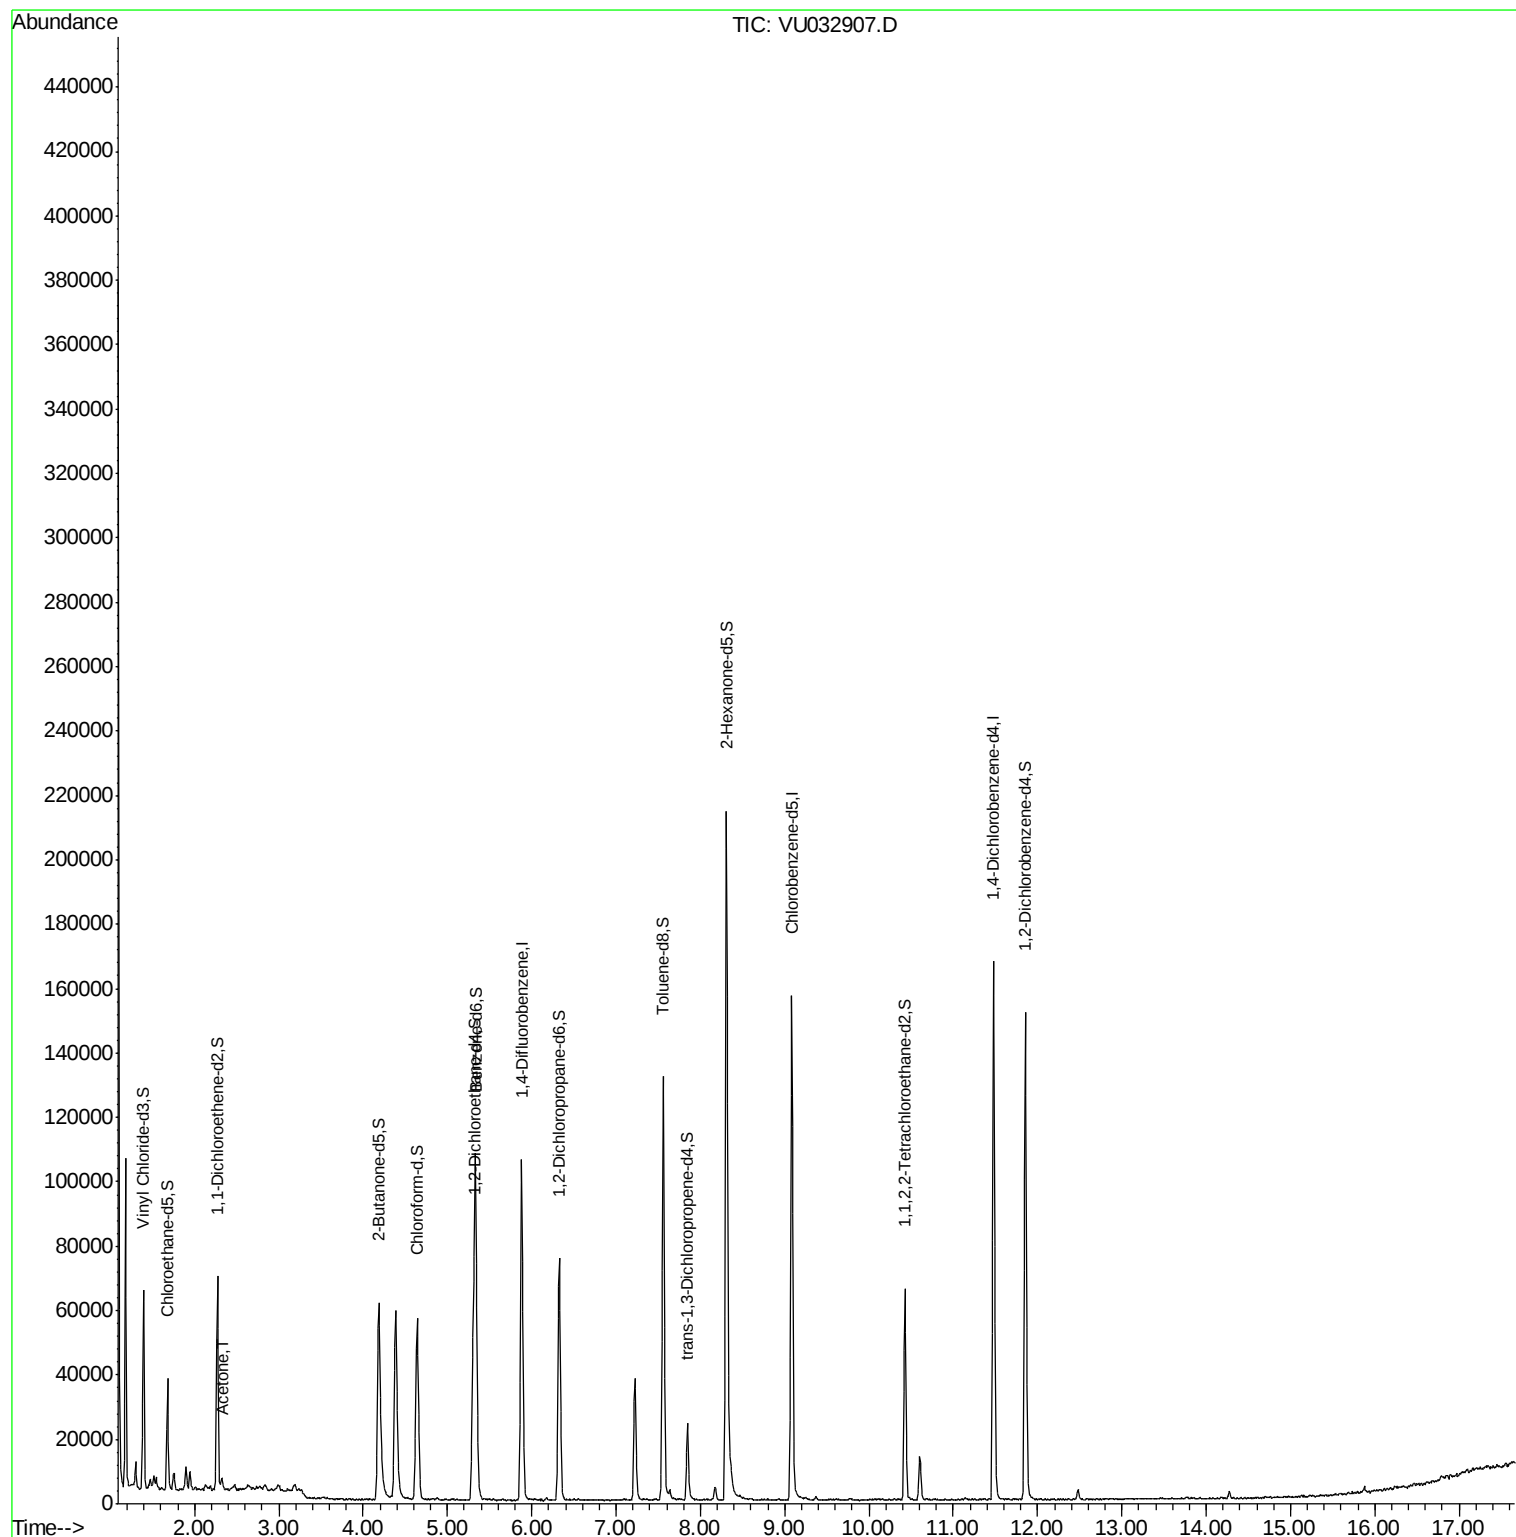

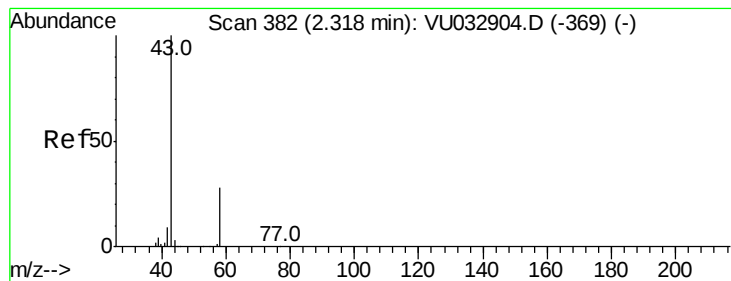

#13
 Acetone
 Concen: 2.930 ug/L
 RT: 2.32 min Scan# 382
 Delta R.T. 0.00 min
 Lab File: VU032907.D
 Acq: 20 Jun 2019 18:02

Instrument :
 MSVOA_U
 ClientSampleId :
 GALF1

Tot Ion: 43 Resp: 3504
 Ion Ratio Lower Upper
 43 100
 58 27.2 0.0 60.8

