


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062019\
Data File : VU032886.D
Acq On : 20 Jun 2019 08:25
Operator : JC/SP
Sample : BFB19
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB19

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Jun 21 07:36:10 2019

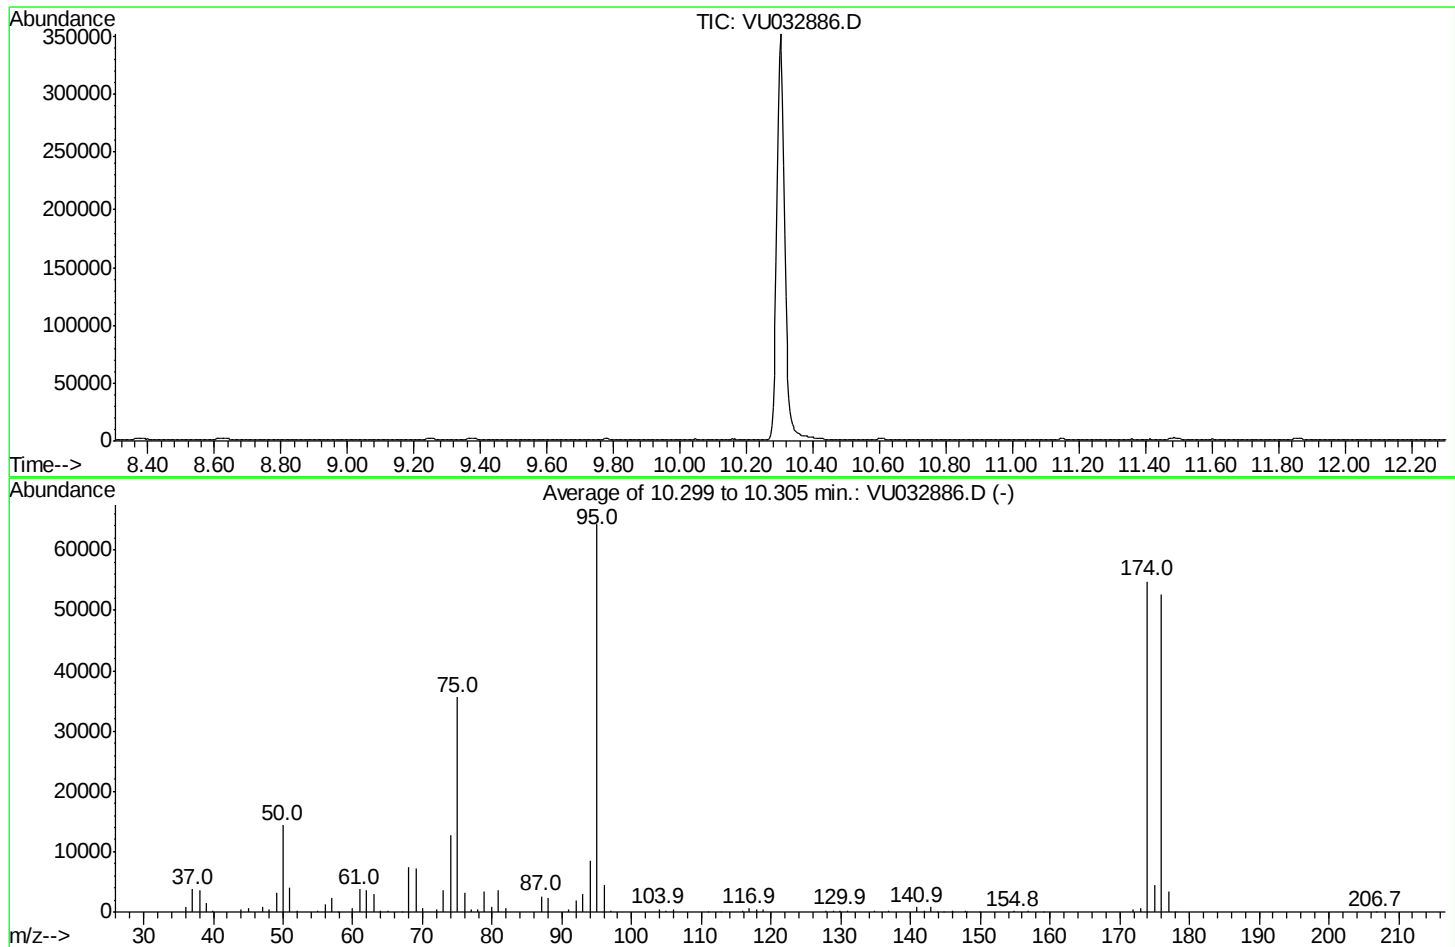

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	14354	PASS
75	95	30	80	55.3	35573	PASS
95	95	100	100	100.0	64272	PASS
96	95	5	9	7.0	4501	PASS
173	174	0.00	2	1.2	681	PASS
174	95	50	120	85.3	54848	PASS
175	174	5	9	8.0	4375	PASS
176	174	95	101	95.9	52597	PASS
177	176	5	9	6.4	3369	PASS

Scan 2851 (10.257 min): VU032886.D
BFB19

m/z	Abundance
39.90	978.0
44.00	292.0
207.10	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	764.0
37.00	3858.0
38.00	3642.0
39.00	1543.0
40.00	1148.0
44.00	799.0
44.90	738.0
47.00	824.0
47.90	516.0
49.00	3227.0
50.00	14291.0
51.00	4149.0
52.00	217.0
55.00	250.0
56.00	1231.0
57.00	2277.0
57.90	116.0
60.00	561.0
61.00	3755.0
62.00	3536.0
63.00	2933.0
64.00	289.0
65.00	268.0
67.00	167.0
68.00	7167.0
69.00	7345.0
70.00	706.0
72.10	398.0
73.00	3559.0
74.00	12433.0
75.00	35344.0
76.00	3076.0
77.00	390.0
77.90	324.0
78.90	3357.0
79.90	824.0
80.90	3531.0
81.90	652.0
87.00	2489.0
88.00	2327.0
90.90	342.0
92.00	2020.0
93.00	3036.0
94.00	8159.0
95.00	62984.0
96.00	4456.0
97.00	169.0
103.90	470.0
104.90	149.0
106.00	333.0
115.90	318.0
116.90	570.0
117.90	314.0
118.90	417.0
127.90	219.0
128.90	154.0
129.90	297.0
130.90	132.0
134.80	153.0
136.90	221.0
140.90	863.0
141.90	130.0
142.90	823.0
143.80	100.0
144.70	120.0
146.00	105.0
147.80	189.0
154.80	134.0
156.80	121.0
171.90	408.0
173.00	616.0
174.00	52496.0
175.00	4240.0
176.00	49440.0
177.00	3232.0
177.90	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
36.00	778.0
37.00	3944.0
38.00	3664.0
39.00	1528.0
40.00	1133.0
44.00	796.0
45.00	721.0
47.00	871.0
48.00	514.0
49.00	3172.0
50.00	14884.0
51.00	4222.0
52.00	208.0
55.00	280.0
56.00	1260.0
57.00	2285.0
57.90	100.0
60.00	671.0
61.00	3825.0
62.00	3731.0
63.00	3064.0
64.00	327.0
65.00	250.0
67.10	180.0
68.00	7598.0
69.00	7449.0
70.00	639.0
72.00	361.0
73.00	3627.0
74.00	13181.0
75.00	36568.0
76.00	3234.0
76.90	424.0
77.90	394.0
78.90	3590.0
79.90	858.0
80.90	3653.0
81.90	745.0
87.00	2637.0
88.00	2392.0
91.00	370.0
92.00	1988.0
93.00	3100.0
94.00	8686.0
95.00	66400.0
96.00	4640.0
97.00	152.0
103.90	540.0
104.90	169.0
106.00	370.0
110.90	108.0
112.70	119.0
115.90	313.0
116.90	575.0
117.90	351.0
118.80	465.0
127.90	220.0
129.00	139.0
129.90	284.0
130.90	144.0
134.90	149.0
136.90	230.0
140.90	835.0
141.90	138.0
142.90	845.0
144.80	101.0
146.00	137.0
147.80	202.0
150.00	104.0
154.80	139.0
156.80	142.0
171.90	468.0
173.00	694.0
174.00	56704.0
175.00	4551.0
176.00	54288.0
177.00	3469.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19

m/z	Abundance
35.90	731.0
37.00	3607.0
38.00	3288.0
39.00	1384.0
40.00	1138.0
44.00	738.0
45.00	666.0
47.00	822.0
48.00	499.0
49.00	2888.0
50.00	13889.0
51.00	3939.0
52.00	193.0
55.00	293.0
56.00	1199.0
57.00	2147.0
60.00	697.0
61.00	3616.0
62.00	3530.0
63.00	2896.0
64.00	322.0
65.00	217.0
68.00	7265.0
69.00	7102.0
70.00	528.0
72.00	304.0
73.00	3364.0
74.00	12736.0
75.00	34808.0
76.00	2996.0
77.00	412.0
77.90	398.0
78.90	3434.0
79.90	790.0
80.90	3381.0
81.90	755.0
87.00	2558.0
88.00	2221.0
91.00	348.0
91.90	1779.0
93.00	3015.0
94.00	8407.0
95.00	63432.0
96.00	4408.0
97.00	118.0
103.90	490.0
105.00	158.0
105.90	387.0
110.90	111.0
112.70	101.0
115.90	287.0
116.90	511.0
117.80	348.0
118.90	459.0
127.90	199.0
128.90	107.0
129.90	247.0
130.90	138.0
134.90	151.0
136.80	195.0
141.00	772.0
141.90	125.0
143.00	788.0
145.90	135.0
147.80	176.0
148.00	176.0
149.90	122.0
154.80	155.0
156.80	151.0
159.00	116.0
171.90	489.0
173.00	734.0
174.00	55344.0
175.00	4336.0
176.00	54064.0
177.00	3406.0
206.70	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB19