

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049296.D
 Acq On : 20 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0620WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	91	rVB	86046	91352	11.09%	1.286%
2	1.912	170	178	191	rVB	74335	96812	11.75%	1.363%
3	2.568	369	382	400	rBV	147187	243914	29.61%	3.434%
4	2.668	411	413	416	rVB3	470	216	0.03%	0.003%
5	2.694	418	421	424	rBV2	371	253	0.03%	0.004%
6	2.967	504	506	512	rVB2	391	315	0.04%	0.004%
7	3.041	526	529	532	rVV2	287	248	0.03%	0.003%
8	3.099	544	547	549	rBV3	290	212	0.03%	0.003%
9	3.179	564	572	573	rBV3	1810	1986	0.24%	0.028%
10	3.243	589	592	597	rVB3	287	229	0.03%	0.003%
11	3.356	625	627	630	rBV3	447	257	0.03%	0.004%
12	3.745	745	748	750	rBV2	302	196	0.02%	0.003%
13	3.780	756	759	765	rVB	371	310	0.04%	0.004%
14	3.809	765	768	773	rVB	335	203	0.02%	0.003%
15	3.919	799	802	806	rVB2	424	304	0.04%	0.004%
16	4.137	866	870	876	rVB2	408	458	0.06%	0.006%
17	4.314	922	925	930	rVV2	395	393	0.05%	0.006%
18	4.382	942	946	951	rVV2	229	263	0.03%	0.004%
19	4.420	953	958	961	rVV2	247	200	0.02%	0.003%
20	4.526	988	991	994	rBV2	337	310	0.04%	0.004%
21	4.623	1008	1021	1051	rBV	112570	298034	36.19%	4.196%
22	4.896	1104	1106	1111	rVB4	316	211	0.03%	0.003%
23	4.973	1125	1130	1133	rBV2	346	339	0.04%	0.005%
24	5.063	1142	1158	1179	rBV	153283	333481	40.49%	4.695%
25	5.253	1214	1217	1219	rBV2	337	232	0.03%	0.003%
26	5.298	1229	1231	1236	rVV3	400	318	0.04%	0.004%
27	5.324	1236	1239	1242	rVB2	296	221	0.03%	0.003%
28	5.356	1242	1249	1251	rBV	366	324	0.04%	0.005%
29	5.369	1251	1253	1260	rVV2	352	283	0.03%	0.004%
30	5.449	1273	1278	1281	rVB3	271	251	0.03%	0.004%
31	5.722	1343	1363	1387	rBV2	299181	823629	100.00%	11.597%
32	5.970	1436	1440	1447	rVB4	468	577	0.07%	0.008%
33	6.009	1447	1452	1459	rBV4	476	627	0.08%	0.009%
34	6.250	1512	1527	1550	rBV	313436	599528	72.79%	8.441%
35	6.533	1604	1615	1622	rBV8	2454	4415	0.54%	0.062%
36	6.600	1633	1636	1640	rVB	379	251	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049296.D
 Acq On : 20 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0620WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1685	rBV2	201463	395541	48.02%	5.569%
38	6.806	1695	1700	1706	rVB2	659	720	0.09%	0.010%
39	6.989	1753	1757	1758	rBV2	357	234	0.03%	0.003%
40	7.015	1762	1765	1770	rVV3	316	346	0.04%	0.005%
41	7.185	1810	1818	1828	rVB2	2378	3588	0.44%	0.051%
42	7.230	1828	1832	1834	rBV2	285	226	0.03%	0.003%
43	7.349	1866	1869	1875	rBV3	246	266	0.03%	0.004%
44	7.462	1898	1904	1907	rBV2	292	351	0.04%	0.005%
45	7.501	1913	1916	1918	rBV	317	218	0.03%	0.003%
46	7.565	1922	1936	1954	rBV	107244	192667	23.39%	2.713%
47	7.664	1964	1967	1969	rBV2	463	335	0.04%	0.005%
48	7.745	1990	1992	2000	rVB2	444	487	0.06%	0.007%
49	7.790	2000	2006	2007	rBV4	953	958	0.12%	0.013%
50	7.896	2026	2039	2057	rVV	353689	623678	75.72%	8.781%
51	7.967	2057	2061	2073	rVB5	4504	7031	0.85%	0.099%
52	8.099	2099	2102	2105	rBV2	296	225	0.03%	0.003%
53	8.179	2114	2127	2146	rBV	75706	130402	15.83%	1.836%
54	8.398	2192	2195	2198	rVB2	318	229	0.03%	0.003%
55	8.632	2255	2268	2301	rBV	313849	596325	72.40%	8.396%
56	8.787	2314	2316	2320	rVB4	588	328	0.04%	0.005%
57	8.835	2329	2331	2335	rVB3	293	197	0.02%	0.003%
58	8.915	2352	2356	2364	rVB4	600	741	0.09%	0.010%
59	9.047	2390	2397	2398	rBV3	271	299	0.04%	0.004%
60	9.073	2401	2405	2408	rVV2	420	363	0.04%	0.005%
61	9.124	2417	2421	2424	rBV2	213	223	0.03%	0.003%
62	9.169	2432	2435	2439	rBV2	337	273	0.03%	0.004%
63	9.266	2460	2465	2470	rBV3	370	518	0.06%	0.007%
64	9.417	2499	2512	2540	rBV	439792	739440	89.78%	10.411%
65	9.700	2594	2600	2609	rVB4	810	1218	0.15%	0.017%
66	9.748	2610	2615	2618	rBV2	298	290	0.04%	0.004%
67	9.825	2635	2639	2642	rBV2	325	247	0.03%	0.003%
68	10.102	2721	2725	2730	rBV4	523	614	0.07%	0.009%
69	10.484	2838	2844	2847	rBV3	539	586	0.07%	0.008%
70	10.574	2869	2872	2874	rBV	332	245	0.03%	0.003%
71	10.610	2880	2883	2887	rBV2	383	338	0.04%	0.005%
72	10.639	2888	2892	2896	rVB3	428	377	0.05%	0.005%
73	10.668	2896	2901	2908	rBV2	833	1123	0.14%	0.016%
74	10.754	2916	2928	2945	rBV	301527	490660	59.57%	6.909%
75	10.922	2975	2980	2981	rBV	425	349	0.04%	0.005%
76	11.092	3031	3033	3039	rVB2	532	398	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049296.D
 Acq On : 20 Jun 2022 11:27
 Operator : SY/MD
 Sample : VU0620WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK144

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.250	3079	3082	3084	rBV2	337	228	0.03%	0.003%
78	11.301	3096	3098	3105	rVB2	322	225	0.03%	0.003%
79	11.462	3140	3148	3149	rBV4	1122	1131	0.14%	0.016%
80	11.587	3183	3187	3192	rBV	521	418	0.05%	0.006%
81	11.693	3215	3220	3221	rBV	392	302	0.04%	0.004%
82	11.748	3231	3237	3244	rBV4	1438	2022	0.25%	0.028%
83	11.812	3244	3257	3278	rBV	458122	736429	89.41%	10.369%
84	11.934	3293	3295	3297	rBV	437	216	0.03%	0.003%
85	12.118	3350	3352	3355	rBV2	366	208	0.03%	0.003%
86	12.192	3363	3375	3396	rBV	374872	609834	74.04%	8.587%
87	12.349	3420	3424	3425	rBV2	289	208	0.03%	0.003%
88	12.465	3458	3460	3467	rVB3	412	418	0.05%	0.006%
89	12.616	3503	3507	3509	rBV2	237	213	0.03%	0.003%
90	12.995	3622	3625	3628	rVB3	445	324	0.04%	0.005%
91	13.050	3638	3642	3645	rBV2	276	258	0.03%	0.004%
92	13.073	3646	3649	3651	rBV3	312	231	0.03%	0.003%
93	13.166	3674	3678	3679	rBV	350	260	0.03%	0.004%
94	13.221	3687	3695	3705	rBV6	2355	3406	0.41%	0.048%
95	13.449	3763	3766	3770	rVB2	469	342	0.04%	0.005%
96	13.468	3770	3772	3776	rBV2	243	212	0.03%	0.003%
97	13.844	3881	3889	3899	rBV4	5521	8221	1.00%	0.116%
98	14.089	3956	3965	3977	rBV	21178	33265	4.04%	0.468%
99	14.333	4032	4041	4049	rBV5	6285	9761	1.19%	0.137%
100	14.635	4132	4135	4138	rBV3	361	289	0.04%	0.004%




Sum of corrected areas: 7102227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049296.D
Acq On : 20 Jun 2022 11:27
Operator : SY/MD
Sample : VU0620WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

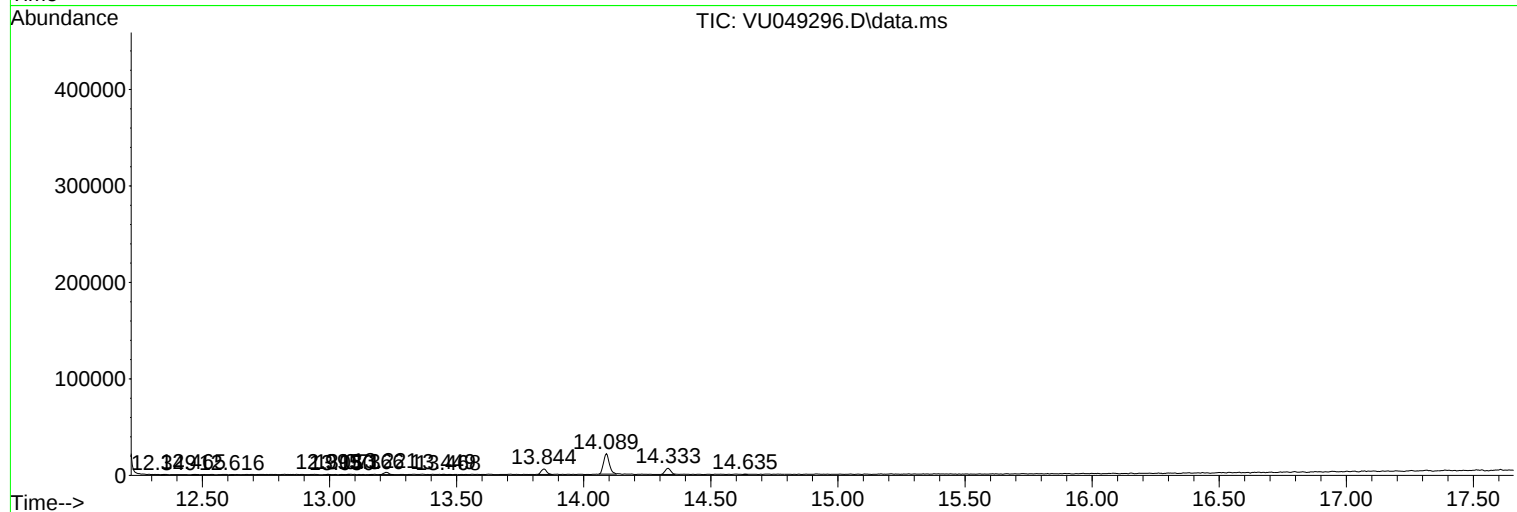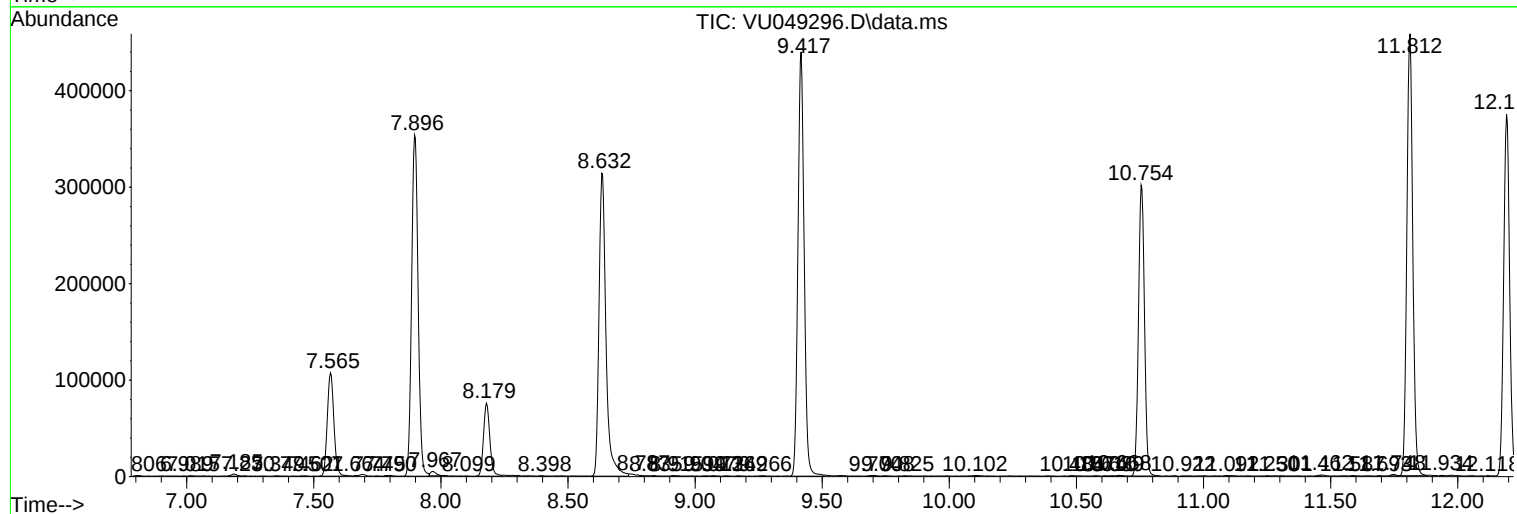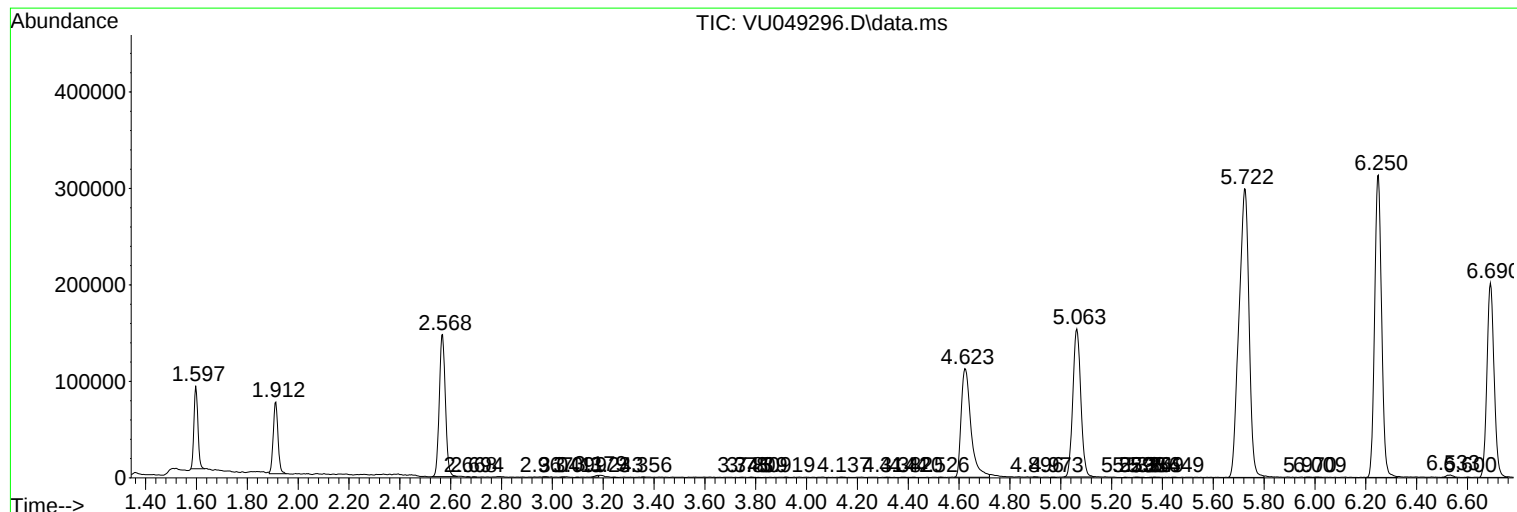

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049296.D
Acq On : 20 Jun 2022 11:27
Operator : SY/MD
Sample : VU0620WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049296.D
Acq On : 20 Jun 2022 11:27
Operator : SY/MD
Sample : VU0620WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK144

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------