

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049302.D
 Acq On : 20 Jun 2022 13:51
 Operator : SY/MD
 Sample : N3395-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	75	80	97	rVB	72076	81665	10.78%	1.185%
2	1.912	171	178	192	rVB	65593	83991	11.09%	1.218%
3	2.568	371	382	397	rBV2	138905	242013	31.96%	3.510%
4	3.044	527	530	535	rBV2	284	318	0.04%	0.005%
5	3.099	545	547	549	rBV2	172	97	0.01%	0.001%
6	3.183	567	573	580	rBV3	860	1430	0.19%	0.021%
7	3.273	598	601	604	rBV2	305	262	0.03%	0.004%
8	3.385	631	636	640	rBV3	340	332	0.04%	0.005%
9	3.456	654	658	660	rBV3	257	166	0.02%	0.002%
10	3.623	707	710	712	rBV	252	203	0.03%	0.003%
11	3.810	763	768	770	rBV2	332	245	0.03%	0.004%
12	3.871	773	787	805	rVV2	38310	88206	11.65%	1.279%
13	4.121	862	865	867	rVB	193	112	0.01%	0.002%
14	4.141	867	871	878	rBV2	266	332	0.04%	0.005%
15	4.253	904	906	910	rVB2	271	194	0.03%	0.003%
16	4.289	915	917	919	rBV	185	123	0.02%	0.002%
17	4.353	934	937	940	rBV2	235	159	0.02%	0.002%
18	4.372	940	943	948	rVB2	236	157	0.02%	0.002%
19	4.398	949	951	955	rBV2	260	211	0.03%	0.003%
20	4.417	955	957	962	rVB	260	157	0.02%	0.002%
21	4.478	974	976	978	rBV	274	169	0.02%	0.002%
22	4.620	1006	1020	1043	rBV	108094	262181	34.62%	3.803%
23	5.063	1142	1158	1175	rBV	143801	311940	41.19%	4.525%
24	5.247	1211	1215	1218	rVB3	349	247	0.03%	0.004%
25	5.317	1218	1237	1251	rBV	44287	98958	13.07%	1.435%
26	5.408	1260	1265	1268	rBV3	202	209	0.03%	0.003%
27	5.481	1284	1288	1291	rBV2	404	300	0.04%	0.004%
28	5.501	1291	1294	1295	rBV2	155	109	0.01%	0.002%
29	5.726	1342	1364	1387	rBV2	275021	757279	100.00%	10.984%
30	6.067	1466	1470	1472	rBV2	318	213	0.03%	0.003%
31	6.131	1483	1490	1494	rBV4	357	410	0.05%	0.006%
32	6.163	1498	1500	1508	rVB3	224	213	0.03%	0.003%
33	6.195	1508	1510	1512	rBV2	245	132	0.02%	0.002%
34	6.247	1512	1526	1548	rBV	312327	596965	78.83%	8.659%
35	6.369	1562	1564	1568	rBV2	283	179	0.02%	0.003%
36	6.530	1606	1614	1622	rBV7	1979	3536	0.47%	0.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049302.D
 Acq On : 20 Jun 2022 13:51
 Operator : SY/MD
 Sample : N3395-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.626	1638	1644	1645	rBV2	145	123	0.02%	0.002%
38	6.690	1650	1664	1686	rVV	193130	370013	48.86%	5.367%
39	6.813	1696	1702	1708	rBV5	790	1102	0.15%	0.016%
40	6.870	1715	1720	1724	rVB2	336	301	0.04%	0.004%
41	6.890	1724	1726	1730	rBV	248	152	0.02%	0.002%
42	6.925	1730	1737	1741	rBV3	365	477	0.06%	0.007%
43	6.996	1756	1759	1762	rBV	175	172	0.02%	0.002%
44	7.073	1779	1783	1786	rBV3	392	296	0.04%	0.004%
45	7.179	1808	1816	1828	rBV4	1760	3240	0.43%	0.047%
46	7.227	1829	1831	1836	rVB4	466	286	0.04%	0.004%
47	7.256	1836	1840	1844	rBV3	282	328	0.04%	0.005%
48	7.366	1867	1874	1876	rBV2	444	494	0.07%	0.007%
49	7.411	1886	1888	1893	rVB3	210	128	0.02%	0.002%
50	7.436	1893	1896	1899	rBV	273	199	0.03%	0.003%
51	7.475	1904	1908	1911	rBV2	251	241	0.03%	0.003%
52	7.565	1924	1936	1956	rBV	104056	179679	23.73%	2.606%
53	7.690	1967	1975	1983	rBV4	1422	2526	0.33%	0.037%
54	7.764	1996	1998	2000	rBV2	229	150	0.02%	0.002%
55	7.800	2007	2009	2014	rVB2	483	345	0.05%	0.005%
56	7.829	2014	2018	2021	rBV3	206	217	0.03%	0.003%
57	7.896	2026	2039	2056	rBV	327331	570029	75.27%	8.268%
58	8.086	2095	2098	2104	rVB4	482	412	0.05%	0.006%
59	8.179	2115	2127	2144	rVV2	71536	120683	15.94%	1.750%
60	8.362	2181	2184	2185	rBV	257	123	0.02%	0.002%
61	8.526	2232	2235	2237	rBV	209	138	0.02%	0.002%
62	8.568	2244	2248	2249	rBV	184	152	0.02%	0.002%
63	8.632	2255	2268	2298	rBV2	279664	547054	72.24%	7.935%
64	8.896	2347	2350	2355	rBV2	499	417	0.06%	0.006%
65	8.938	2361	2363	2364	rBV2	255	108	0.01%	0.002%
66	8.989	2376	2379	2380	rBV	205	127	0.02%	0.002%
67	9.022	2384	2389	2392	rVB2	276	261	0.03%	0.004%
68	9.044	2392	2396	2398	rBV	338	238	0.03%	0.003%
69	9.140	2417	2426	2428	rBV2	502	507	0.07%	0.007%
70	9.285	2468	2471	2474	rVB2	311	213	0.03%	0.003%
71	9.359	2485	2494	2498	rBV2	401	627	0.08%	0.009%
72	9.417	2498	2512	2530	rBV	445292	740959	97.84%	10.747%
73	9.562	2555	2557	2558	rBV	337	140	0.02%	0.002%
74	9.636	2573	2580	2582	rBV2	318	291	0.04%	0.004%
75	9.655	2582	2586	2588	rBV3	316	222	0.03%	0.003%
76	9.732	2607	2610	2611	rBV	240	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049302.D
 Acq On : 20 Jun 2022 13:51
 Operator : SY/MD
 Sample : N3395-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.880	2653	2656	2658	rVB2	209	114	0.02%	0.002%
78	9.896	2658	2661	2663	rBV	219	131	0.02%	0.002%
79	9.948	2674	2677	2679	rVB2	304	192	0.03%	0.003%
80	9.960	2679	2681	2683	rBV2	211	141	0.02%	0.002%
81	10.102	2721	2725	2726	rBV	448	315	0.04%	0.005%
82	10.173	2744	2747	2749	rBV2	176	112	0.01%	0.002%
83	10.292	2777	2784	2790	rBV3	365	521	0.07%	0.008%
84	10.382	2809	2812	2815	rBV3	331	211	0.03%	0.003%
85	10.433	2825	2828	2833	rBV3	268	256	0.03%	0.004%
86	10.558	2863	2867	2871	rVB3	321	331	0.04%	0.005%
87	10.581	2871	2874	2877	rBV3	271	210	0.03%	0.003%
88	10.755	2916	2928	2950	rBV	295420	478964	63.25%	6.947%
89	10.890	2962	2970	2972	rBV3	749	964	0.13%	0.014%
90	10.947	2985	2988	2993	rVB3	262	222	0.03%	0.003%
91	11.050	3017	3020	3023	rBV	303	228	0.03%	0.003%
92	11.330	3104	3107	3116	rVB3	377	473	0.06%	0.007%
93	11.636	3200	3202	3206	rVB	293	184	0.02%	0.003%
94	11.697	3216	3221	3225	rBV2	498	500	0.07%	0.007%
95	11.742	3232	3235	3240	rVB3	698	536	0.07%	0.008%
96	11.812	3243	3257	3281	rBV	462562	746795	98.62%	10.832%
97	11.941	3294	3297	3301	rBV3	543	506	0.07%	0.007%
98	12.076	3337	3339	3341	rBV2	251	125	0.02%	0.002%
99	12.192	3363	3375	3395	rBV	358414	585372	77.30%	8.491%
100	12.317	3411	3414	3415	rBV2	309	168	0.02%	0.002%




Sum of corrected areas: 6894299

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049302.D
Acq On : 20 Jun 2022 13:51
Operator : SY/MD
Sample : N3395-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

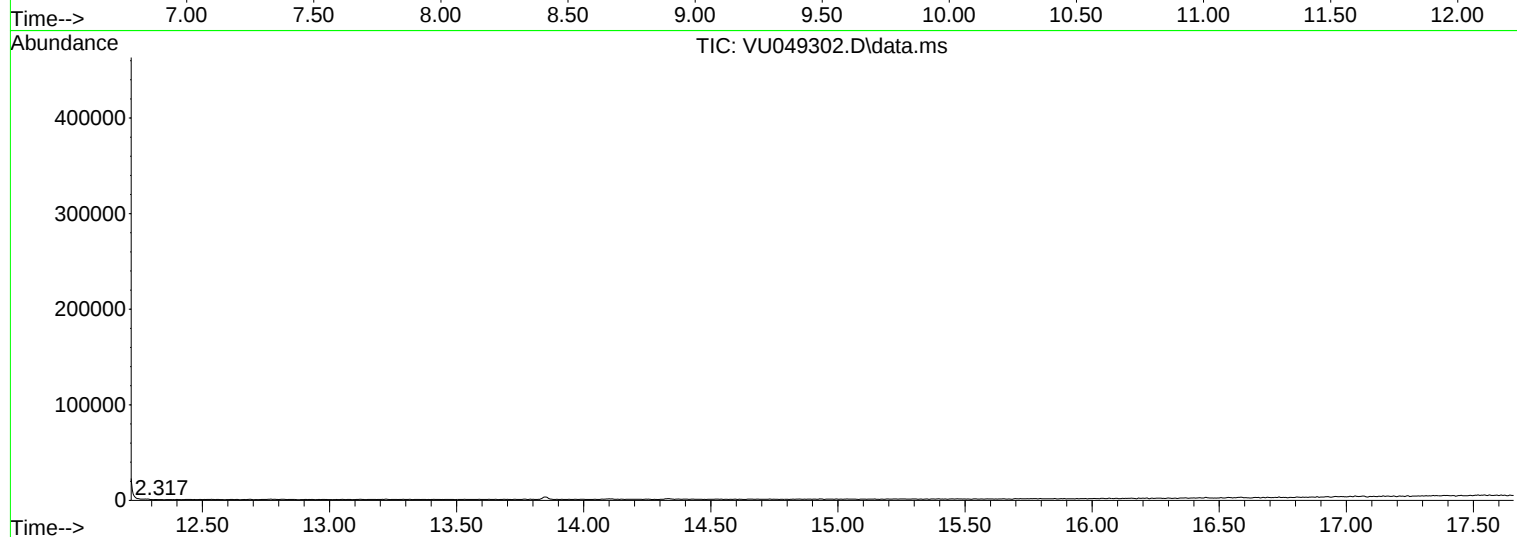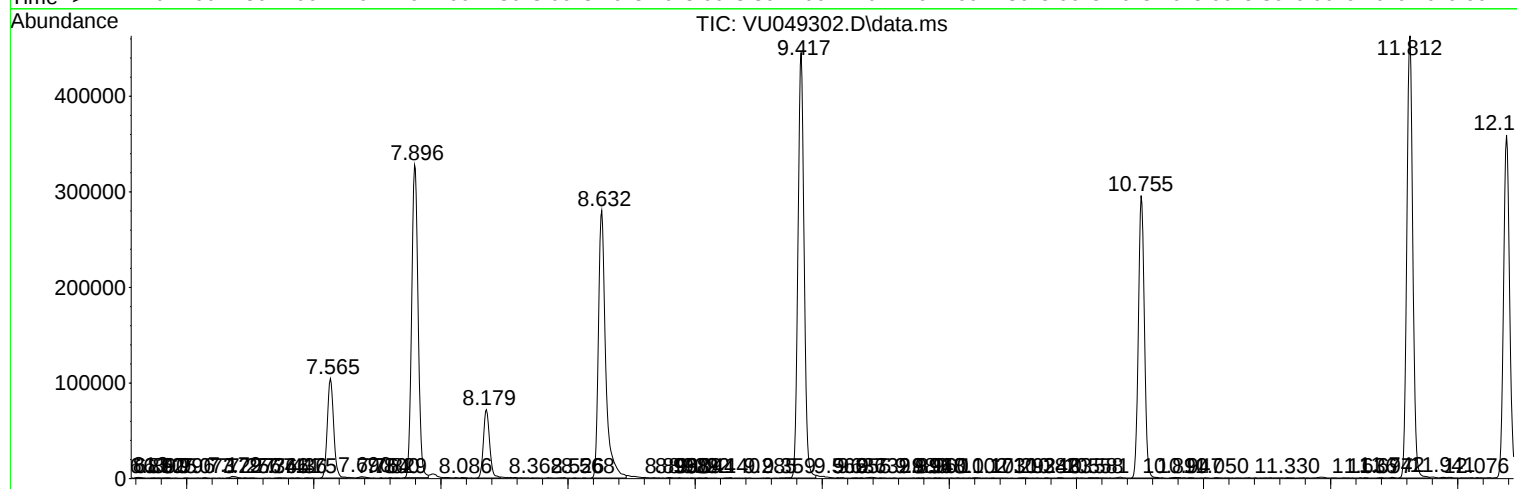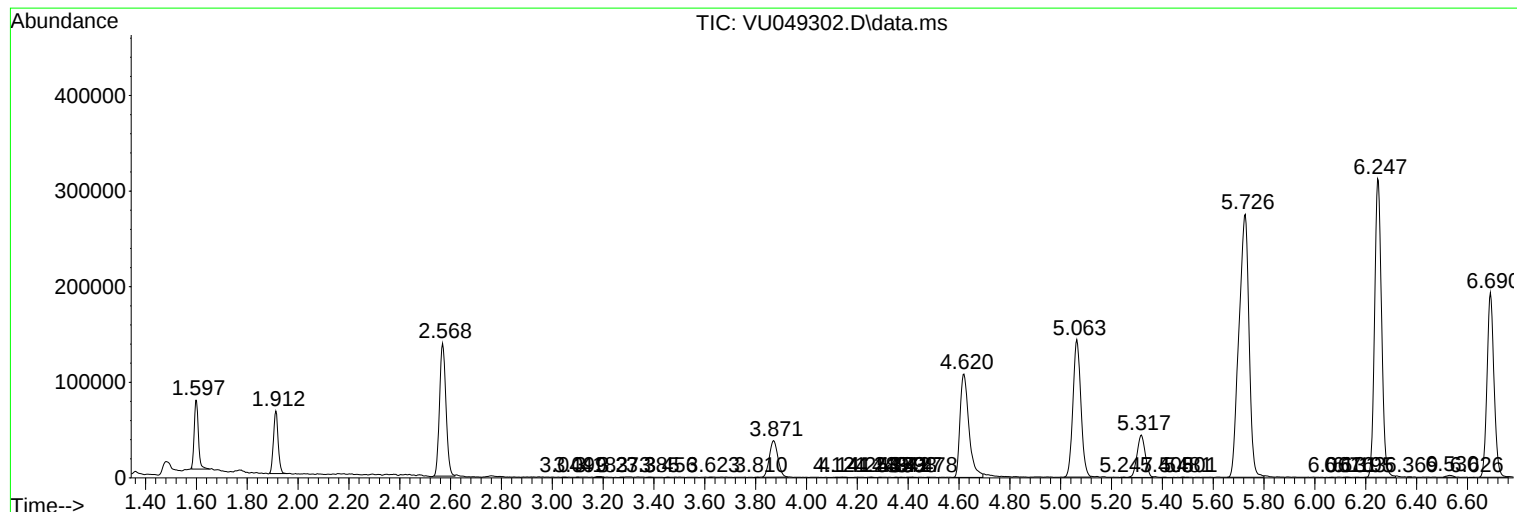

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049302.D
Acq On : 20 Jun 2022 13:51
Operator : SY/MD
Sample : N3395-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049302.D
Acq On : 20 Jun 2022 13:51
Operator : SY/MD
Sample : N3395-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0158

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------