

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049303.D
 Acq On : 20 Jun 2022 14:15
 Operator : SY/MD
 Sample : N3395-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	102	rVB	127498	147881	14.11%	1.688%
2	1.912	170	178	193	rVB	104257	133214	12.71%	1.520%
3	2.568	370	382	396	rBV	197969	320617	30.60%	3.659%
4	2.932	492	495	497	rBV2	305	185	0.02%	0.002%
5	3.044	527	530	531	rBV2	387	226	0.02%	0.003%
6	3.137	556	559	564	rVB2	428	346	0.03%	0.004%
7	3.163	564	567	570	rBV3	420	282	0.03%	0.003%
8	3.263	593	598	604	rBV3	456	638	0.06%	0.007%
9	3.385	633	636	641	rBV3	238	249	0.02%	0.003%
10	3.645	714	717	721	rBV2	241	207	0.02%	0.002%
11	3.707	732	736	737	rBV2	327	212	0.02%	0.002%
12	3.774	752	757	758	rBV3	199	138	0.01%	0.002%
13	3.819	769	771	776	rVB2	252	156	0.01%	0.002%
14	3.845	776	779	780	rBV2	268	142	0.01%	0.002%
15	3.887	790	792	794	rBV	160	68	0.01%	0.001%
16	3.909	797	799	803	rBV	266	163	0.02%	0.002%
17	3.957	810	814	819	rBV2	421	554	0.05%	0.006%
18	4.006	827	829	835	rVB2	346	246	0.02%	0.003%
19	4.035	835	838	839	rBV	142	84	0.01%	0.001%
20	4.063	844	847	852	rBV2	252	265	0.03%	0.003%
21	4.108	857	861	865	rBV3	265	254	0.02%	0.003%
22	4.153	873	875	877	rBV	178	102	0.01%	0.001%
23	4.166	877	879	882	rVB2	210	72	0.01%	0.001%
24	4.208	888	892	896	rBV2	271	213	0.02%	0.002%
25	4.237	899	901	903	rBV2	143	71	0.01%	0.001%
26	4.250	903	905	908	rVB	285	175	0.02%	0.002%
27	4.279	908	914	917	rBV2	293	266	0.03%	0.003%
28	4.305	920	922	928	rBV3	218	199	0.02%	0.002%
29	4.359	934	939	941	rBV2	285	270	0.03%	0.003%
30	4.404	951	953	956	rBV	112	75	0.01%	0.001%
31	4.424	956	959	962	rBV2	374	299	0.03%	0.003%
32	4.501	980	983	987	rVB	368	250	0.02%	0.003%
33	4.620	1007	1020	1057	rBV	130200	314673	30.03%	3.592%
34	5.063	1142	1158	1180	rBV	185808	411431	39.27%	4.696%
35	5.247	1212	1215	1218	rVB2	467	290	0.03%	0.003%
36	5.311	1233	1235	1239	rVB2	362	185	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049303.D
 Acq On : 20 Jun 2022 14:15
 Operator : SY/MD
 Sample : N3395-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.372	1239	1254	1286	rBV	224195	464351	44.32%	5.300%
38	5.497	1290	1293	1294	rBV	274	141	0.01%	0.002%
39	5.549	1304	1309	1315	rBV4	565	633	0.06%	0.007%
40	5.575	1315	1317	1322	rVB	182	118	0.01%	0.001%
41	5.600	1322	1325	1327	rBV2	195	116	0.01%	0.001%
42	5.616	1327	1330	1333	rBV2	179	123	0.01%	0.001%
43	5.726	1341	1364	1384	rBV2	382568	1047730	100.00%	11.959%
44	5.960	1434	1437	1443	rBV4	375	289	0.03%	0.003%
45	6.038	1458	1461	1464	rBV2	241	148	0.01%	0.002%
46	6.057	1464	1467	1469	rBV2	248	143	0.01%	0.002%
47	6.070	1469	1471	1473	rBV	121	36	0.00%	0.000%
48	6.089	1474	1477	1478	rBV	185	88	0.01%	0.001%
49	6.186	1505	1507	1511	rVB	140	84	0.01%	0.001%
50	6.250	1511	1527	1560	rBV	339626	651060	62.14%	7.431%
51	6.530	1602	1614	1622	rBV5	2324	4620	0.44%	0.053%
52	6.690	1648	1664	1687	rBV	256227	494531	47.20%	5.645%
53	6.890	1722	1726	1729	rBV	307	214	0.02%	0.002%
54	6.948	1742	1744	1746	rBV	151	69	0.01%	0.001%
55	6.964	1746	1749	1751	rVB	206	126	0.01%	0.001%
56	6.977	1751	1753	1756	rBV2	293	176	0.02%	0.002%
57	7.034	1769	1771	1772	rBV2	422	212	0.02%	0.002%
58	7.079	1783	1785	1786	rBV2	280	133	0.01%	0.002%
59	7.131	1799	1801	1807	rVB2	208	135	0.01%	0.002%
60	7.179	1807	1816	1833	rBV8	2127	4050	0.39%	0.046%
61	7.247	1833	1837	1838	rBV	328	222	0.02%	0.003%
62	7.288	1848	1850	1852	rBV	125	65	0.01%	0.001%
63	7.407	1882	1887	1892	rVB2	320	278	0.03%	0.003%
64	7.436	1892	1896	1897	rBV2	204	120	0.01%	0.001%
65	7.481	1908	1910	1913	rBV3	194	109	0.01%	0.001%
66	7.517	1919	1921	1922	rBV	180	75	0.01%	0.001%
67	7.565	1923	1936	1958	rVV	138736	243083	23.20%	2.775%
68	7.751	1990	1994	1998	rBV2	395	346	0.03%	0.004%
69	7.838	2018	2021	2024	rBV2	342	258	0.02%	0.003%
70	7.896	2026	2039	2056	rBV	454606	796511	76.02%	9.091%
71	8.179	2115	2127	2150	rBV	92894	162090	15.47%	1.850%
72	8.362	2182	2184	2185	rBV	207	62	0.01%	0.001%
73	8.394	2192	2194	2196	rBV2	208	112	0.01%	0.001%
74	8.436	2202	2207	2209	rBV3	367	334	0.03%	0.004%
75	8.632	2255	2268	2303	rBV	336330	657616	62.77%	7.506%
76	8.886	2344	2347	2348	rBV2	267	138	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049303.D
 Acq On : 20 Jun 2022 14:15
 Operator : SY/MD
 Sample : N3395-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0161

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	8.947	2364	2366	2368	rBV	127	71	0.01%	0.001%
78	8.999	2379	2382	2386	rBV2	225	145	0.01%	0.002%
79	9.304	2473	2477	2481	rVB2	274	203	0.02%	0.002%
80	9.417	2499	2512	2533	rBV	480337	795238	75.90%	9.077%
81	9.623	2572	2576	2578	rBV3	337	324	0.03%	0.004%
82	9.738	2610	2612	2618	rVB	316	227	0.02%	0.003%
83	9.764	2618	2620	2624	rBV2	242	173	0.02%	0.002%
84	9.857	2646	2649	2652	rBV2	191	121	0.01%	0.001%
85	10.005	2693	2695	2697	rBV	170	118	0.01%	0.001%
86	10.073	2713	2716	2717	rBV	144	79	0.01%	0.001%
87	10.259	2771	2774	2778	rBV2	274	176	0.02%	0.002%
88	10.507	2847	2851	2854	rBV2	300	307	0.03%	0.004%
89	10.584	2872	2875	2877	rBV2	363	223	0.02%	0.003%
90	10.616	2881	2885	2891	rVV2	410	456	0.04%	0.005%
91	10.671	2895	2902	2910	rVB3	1291	1715	0.16%	0.020%
92	10.755	2916	2928	2946	rBV	358273	582567	55.60%	6.649%
93	11.430	3136	3138	3142	rBV2	337	216	0.02%	0.002%
94	11.459	3142	3147	3149	rBV3	752	697	0.07%	0.008%
95	11.526	3165	3168	3170	rBV	351	246	0.02%	0.003%
96	11.565	3175	3180	3183	rBV2	308	333	0.03%	0.004%
97	11.652	3204	3207	3210	rBV2	365	337	0.03%	0.004%
98	11.812	3244	3257	3277	rBV	464118	756690	72.22%	8.637%
99	12.044	3325	3329	3332	rBV	442	403	0.04%	0.005%
100	12.192	3362	3375	3397	rBV	460057	754771	72.04%	8.615%




Sum of corrected areas: 8761279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049303.D
Acq On : 20 Jun 2022 14:15
Operator : SY/MD
Sample : N3395-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

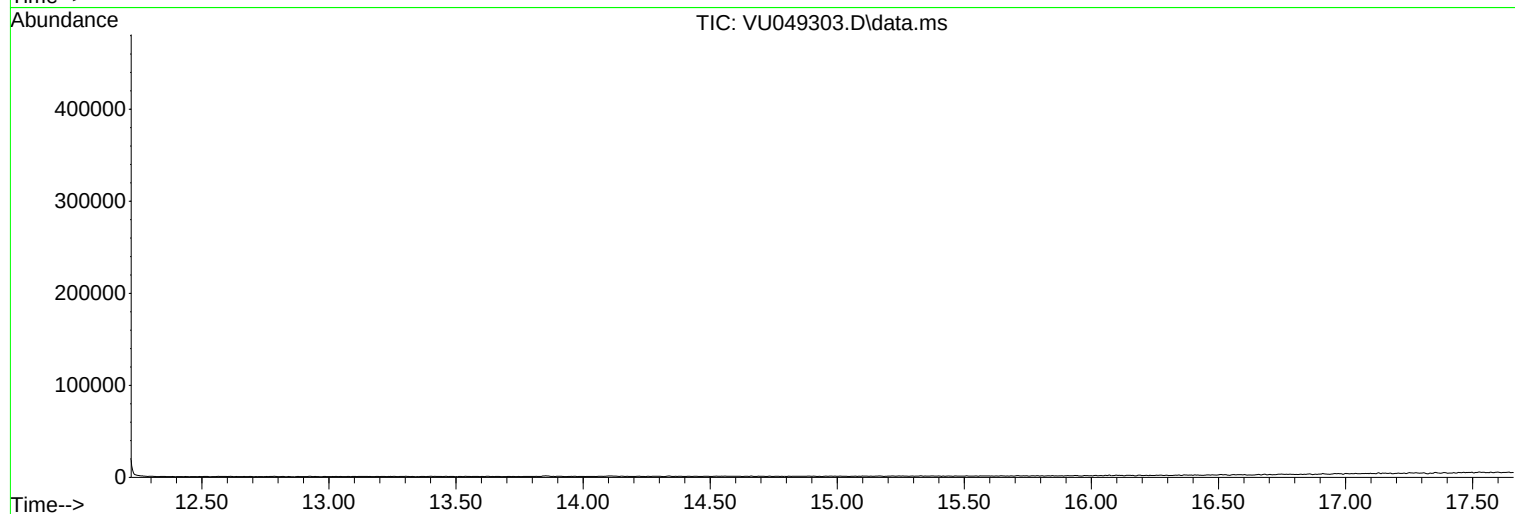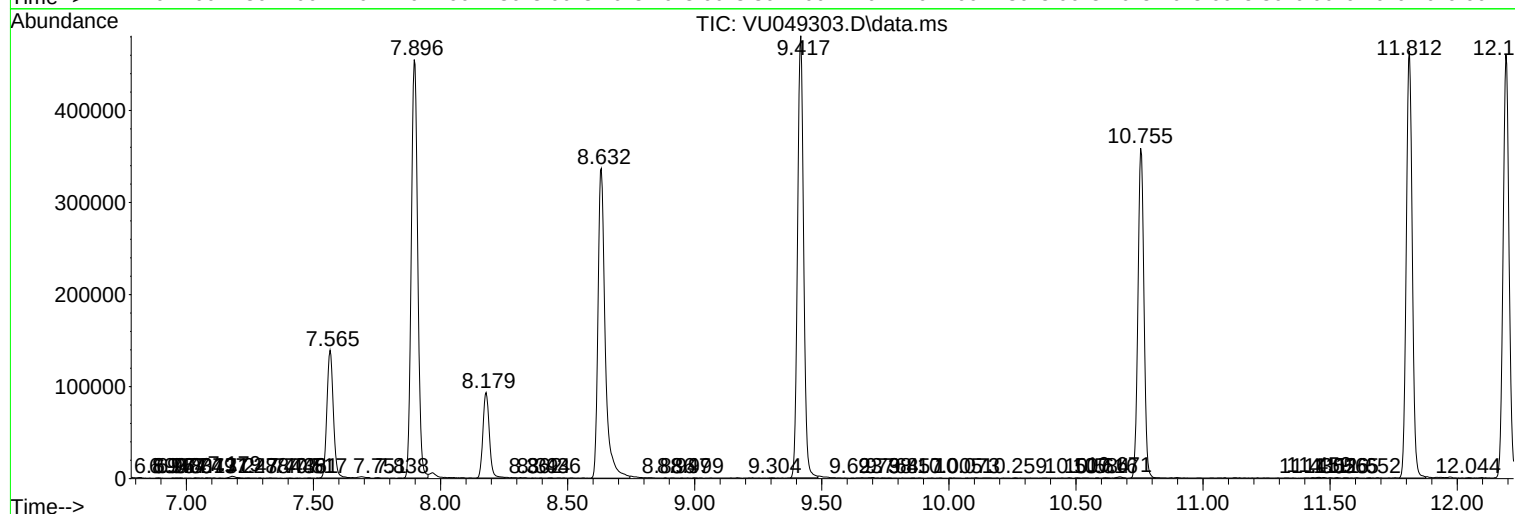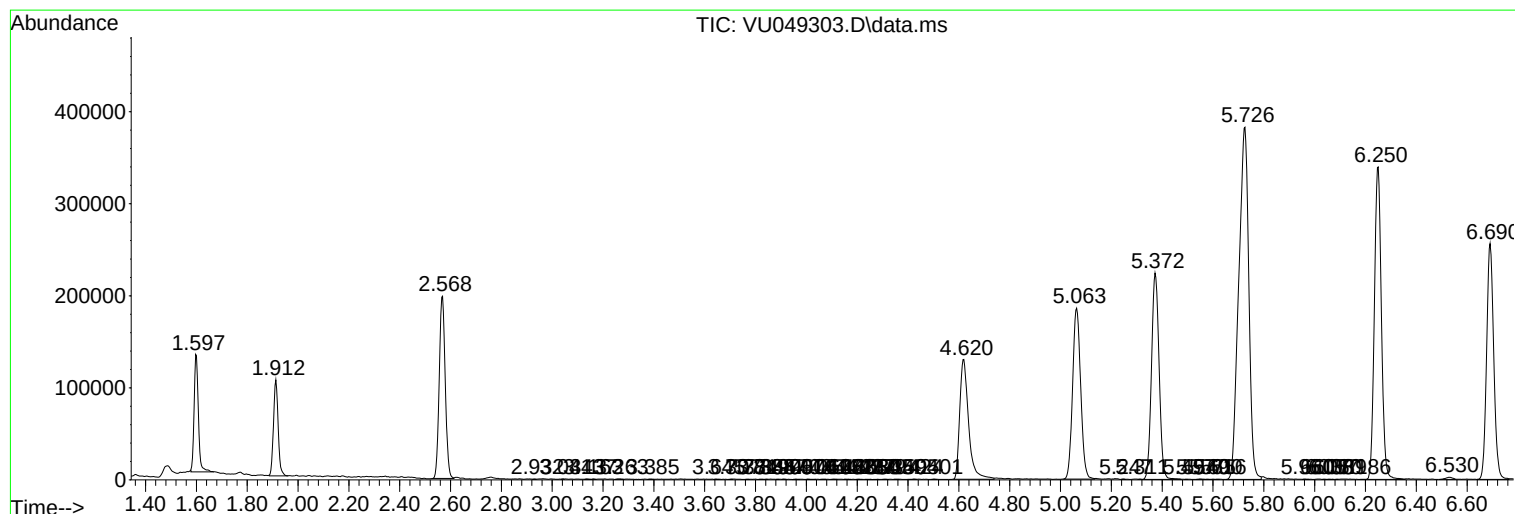

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049303.D
Acq On : 20 Jun 2022 14:15
Operator : SY/MD
Sample : N3395-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049303.D
Acq On : 20 Jun 2022 14:15
Operator : SY/MD
Sample : N3395-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0161

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc