

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049304.D
 Acq On : 20 Jun 2022 14:38
 Operator : SY/MD
 Sample : N3395-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0159

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	75	80	94	rVB	74570	82246	10.19%	1.177%
2	1.912	171	178	191	rVB	67998	88423	10.96%	1.265%
3	2.568	370	382	396	rBV	130892	217291	26.93%	3.109%
4	3.308	608	612	614	rBV2	248	207	0.03%	0.003%
5	3.456	654	658	662	rBV3	255	173	0.02%	0.002%
6	3.555	685	689	692	rBV2	233	195	0.02%	0.003%
7	3.674	723	726	729	rBV	293	277	0.03%	0.004%
8	3.899	794	796	797	rBV	136	69	0.01%	0.001%
9	4.018	831	833	835	rVB2	182	77	0.01%	0.001%
10	4.034	835	838	840	rBV2	256	183	0.02%	0.003%
11	4.182	881	884	886	rBV2	255	165	0.02%	0.002%
12	4.195	886	888	891	rVB	345	155	0.02%	0.002%
13	4.231	897	899	903	rBV2	162	101	0.01%	0.001%
14	4.250	903	905	906	rBV	216	118	0.01%	0.002%
15	4.340	930	933	935	rBV	165	103	0.01%	0.001%
16	4.362	938	940	941	rVV	180	77	0.01%	0.001%
17	4.382	944	946	949	rVB	181	77	0.01%	0.001%
18	4.465	969	972	975	rBV3	194	160	0.02%	0.002%
19	4.485	975	978	982	rVV2	273	199	0.02%	0.003%
20	4.575	1003	1006	1008	rBV2	278	155	0.02%	0.002%
21	4.623	1008	1021	1054	rBV	111887	282710	35.03%	4.045%
22	5.063	1142	1158	1185	rBV	149507	329763	40.86%	4.718%
23	5.215	1202	1205	1210	rBV2	339	305	0.04%	0.004%
24	5.276	1221	1224	1226	rBV	364	220	0.03%	0.003%
25	5.314	1230	1236	1237	rBV3	530	446	0.06%	0.006%
26	5.375	1248	1255	1257	rBV3	844	1023	0.13%	0.015%
27	5.536	1301	1305	1307	rBV	240	147	0.02%	0.002%
28	5.575	1315	1317	1321	rVB2	356	250	0.03%	0.004%
29	5.607	1321	1327	1329	rBV	307	293	0.04%	0.004%
30	5.623	1329	1332	1335	rVB2	258	191	0.02%	0.003%
31	5.726	1342	1364	1395	rBV2	293508	807017	100.00%	11.547%
32	5.886	1411	1414	1416	rVB2	380	229	0.03%	0.003%
33	5.906	1416	1420	1428	rVB4	267	313	0.04%	0.004%
34	6.002	1447	1450	1453	rVB	327	187	0.02%	0.003%
35	6.028	1455	1458	1460	rBV2	171	96	0.01%	0.001%
36	6.041	1460	1462	1465	rVB2	271	138	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049304.D
 Acq On : 20 Jun 2022 14:38
 Operator : SY/MD
 Sample : N3395-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0159

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.063	1465	1469	1472	rBV	266	221	0.03%	0.003%
38	6.105	1479	1482	1484	rBV2	363	285	0.04%	0.004%
39	6.179	1503	1505	1508	rBV2	284	149	0.02%	0.002%
40	6.250	1508	1527	1546	rBV	321502	615724	76.30%	8.810%
41	6.436	1583	1585	1587	rVB	208	86	0.01%	0.001%
42	6.481	1596	1599	1604	rVB3	397	299	0.04%	0.004%
43	6.536	1604	1616	1630	rBV5	4505	10685	1.32%	0.153%
44	6.690	1650	1664	1682	rBV	199195	390523	48.39%	5.588%
45	6.841	1708	1711	1714	rVB2	200	132	0.02%	0.002%
46	6.858	1714	1716	1720	rVB2	222	96	0.01%	0.001%
47	6.886	1720	1725	1727	rBV	290	263	0.03%	0.004%
48	6.922	1733	1736	1739	rBV2	176	116	0.01%	0.002%
49	6.970	1748	1751	1753	rVB	191	104	0.01%	0.001%
50	6.986	1753	1756	1757	rBV	167	107	0.01%	0.002%
51	7.022	1764	1767	1770	rBV2	281	234	0.03%	0.003%
52	7.124	1797	1799	1802	rBV	141	105	0.01%	0.002%
53	7.182	1812	1817	1826	rVB3	1887	2664	0.33%	0.038%
54	7.266	1840	1843	1846	rBV2	188	159	0.02%	0.002%
55	7.346	1864	1868	1870	rBV2	293	227	0.03%	0.003%
56	7.359	1870	1872	1874	rVV2	304	153	0.02%	0.002%
57	7.388	1877	1881	1888	rBV2	337	458	0.06%	0.007%
58	7.433	1893	1895	1898	rBV2	156	97	0.01%	0.001%
59	7.565	1923	1936	1953	rBV	105657	187037	23.18%	2.676%
60	7.816	2012	2014	2016	rBV	237	121	0.01%	0.002%
61	7.896	2026	2039	2057	rBV	346740	598781	74.20%	8.567%
62	8.179	2116	2127	2142	rBV2	72421	122776	15.21%	1.757%
63	8.546	2237	2241	2245	rVB2	361	334	0.04%	0.005%
64	8.575	2245	2250	2256	rBV2	394	578	0.07%	0.008%
65	8.632	2256	2268	2303	rBV2	311809	596371	73.90%	8.533%
66	8.816	2322	2325	2329	rVB3	563	388	0.05%	0.006%
67	8.906	2347	2353	2359	rBV4	468	704	0.09%	0.010%
68	9.095	2409	2412	2413	rBV	231	141	0.02%	0.002%
69	9.140	2424	2426	2429	rBV2	252	115	0.01%	0.002%
70	9.166	2431	2434	2435	rBV2	331	224	0.03%	0.003%
71	9.208	2444	2447	2448	rBV	251	159	0.02%	0.002%
72	9.288	2470	2472	2476	rVB	310	132	0.02%	0.002%
73	9.333	2482	2486	2488	rBV2	403	299	0.04%	0.004%
74	9.417	2499	2512	2536	rBV	454986	761994	94.42%	10.903%
75	9.690	2594	2597	2598	rBV	462	284	0.04%	0.004%
76	9.812	2633	2635	2637	rBV2	215	140	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049304.D
 Acq On : 20 Jun 2022 14:38
 Operator : SY/MD
 Sample : N3395-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0159

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.870	2651	2653	2656	rBV	213	158	0.02%	0.002%
78	10.137	2732	2736	2739	rBV	327	287	0.04%	0.004%
79	10.224	2761	2763	2766	rBV2	188	124	0.02%	0.002%
80	10.391	2813	2815	2818	rBV	167	97	0.01%	0.001%
81	10.494	2845	2847	2849	rBV2	321	176	0.02%	0.003%
82	10.754	2916	2928	2947	rBV	309058	498999	61.83%	7.140%
83	10.838	2952	2954	2957	rVB	239	102	0.01%	0.001%
84	10.883	2963	2968	2969	rBV	449	404	0.05%	0.006%
85	11.044	3014	3018	3021	rVB2	317	297	0.04%	0.004%
86	11.066	3021	3025	3026	rBV	279	175	0.02%	0.003%
87	11.092	3030	3033	3036	rBV2	294	215	0.03%	0.003%
88	11.176	3057	3059	3061	rBV2	224	130	0.02%	0.002%
89	11.282	3088	3092	3096	rBV	413	301	0.04%	0.004%
90	11.336	3106	3109	3113	rVB2	298	268	0.03%	0.004%
91	11.420	3132	3135	3138	rVB2	324	219	0.03%	0.003%
92	11.452	3138	3145	3146	rBV3	645	630	0.08%	0.009%
93	11.510	3160	3163	3164	rBV2	304	176	0.02%	0.003%
94	11.693	3217	3220	3223	rBV2	427	277	0.03%	0.004%
95	11.812	3244	3257	3275	rBV	479575	760962	94.29%	10.888%
96	12.012	3317	3319	3320	rBV	344	167	0.02%	0.002%
97	12.192	3362	3375	3399	rBV	378351	616453	76.39%	8.820%
98	12.722	3535	3540	3544	rBV2	431	477	0.06%	0.007%
99	13.584	3806	3808	3813	rBV3	290	268	0.03%	0.004%
100	13.848	3887	3890	3894	rBV2	627	507	0.06%	0.007%




Sum of corrected areas: 6989113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049304.D
Acq On : 20 Jun 2022 14:38
Operator : SY/MD
Sample : N3395-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0159

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

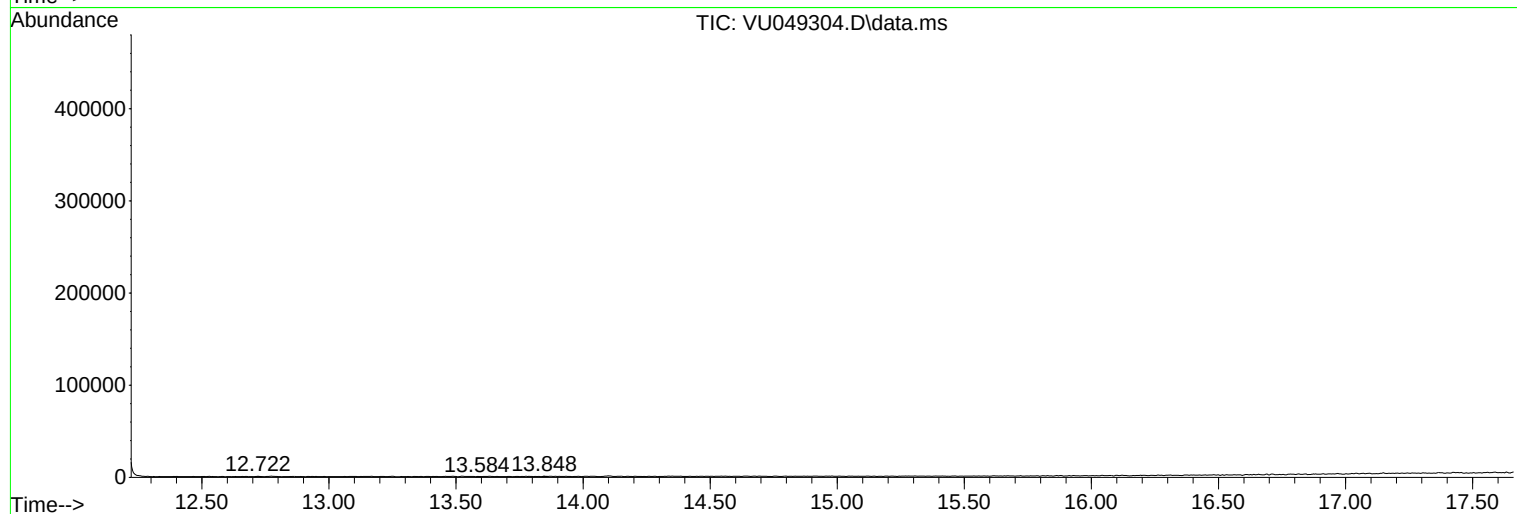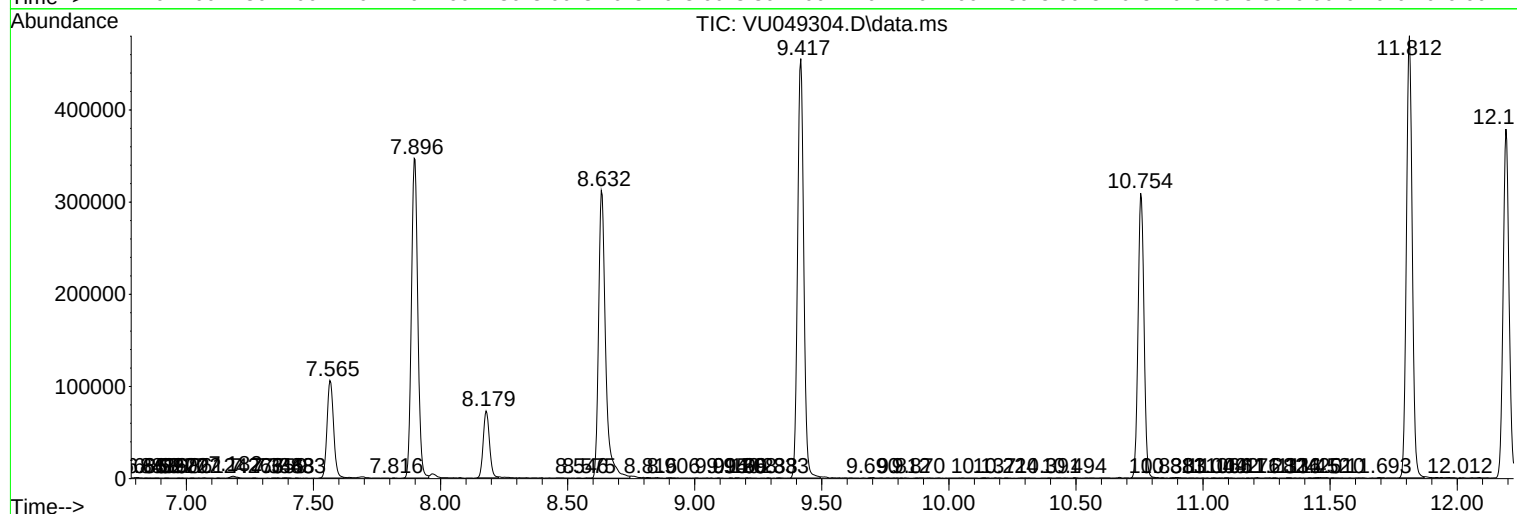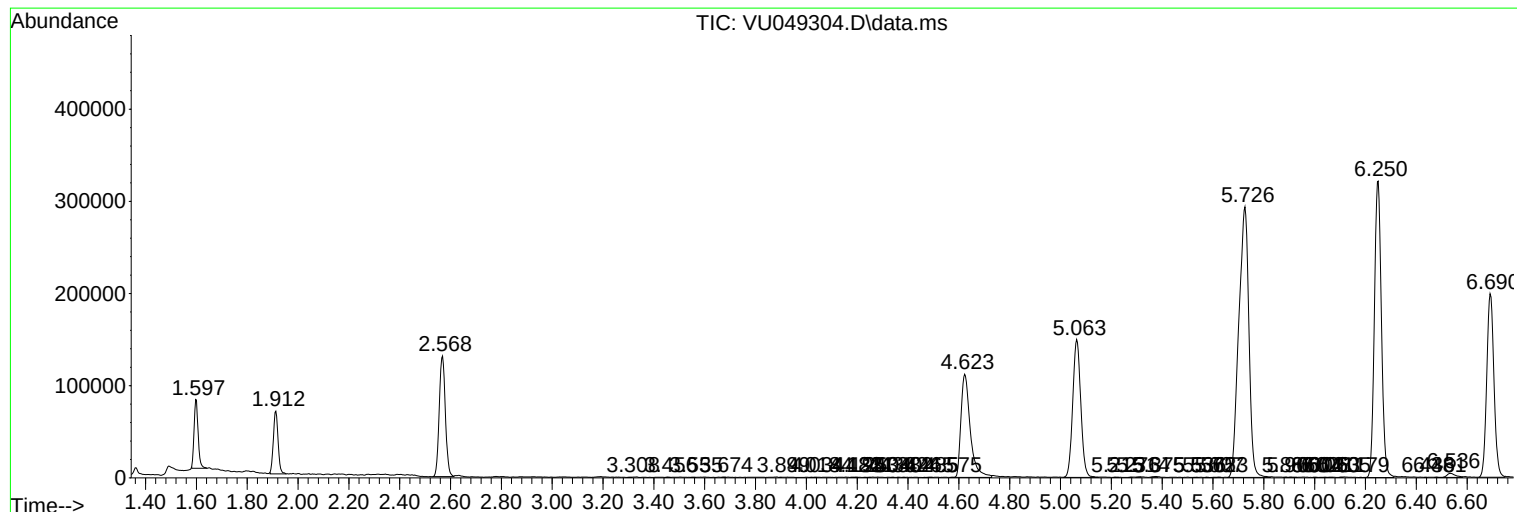

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049304.D
Acq On : 20 Jun 2022 14:38
Operator : SY/MD
Sample : N3395-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0159

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049304.D
Acq On : 20 Jun 2022 14:38
Operator : SY/MD
Sample : N3395-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0159

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------