

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049305.D
 Acq On : 20 Jun 2022 15:01
 Operator : SY/MD
 Sample : N3395-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M

Title : VOC Analysis

Signal : TIC: VU049305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	126467	145263	14.38%	1.663%
2	1.913	170	178	196	rVB	97520	127842	12.66%	1.463%
3	2.565	369	381	396	rBV	193373	312330	30.93%	3.575%
4	2.704	421	424	426	rVB2	300	179	0.02%	0.002%
5	2.771	438	445	446	rBV3	429	438	0.04%	0.005%
6	2.794	446	452	457	rVV4	997	1269	0.13%	0.015%
7	2.874	476	477	481	rBV2	380	309	0.03%	0.004%
8	3.192	572	576	577	rBV2	265	190	0.02%	0.002%
9	3.244	587	592	595	rBV3	299	290	0.03%	0.003%
10	3.459	652	659	662	rBV	339	370	0.04%	0.004%
11	3.777	751	758	767	rVB3	299	539	0.05%	0.006%
12	3.861	781	784	787	rBV	233	196	0.02%	0.002%
13	3.925	803	804	808	rVB	379	196	0.02%	0.002%
14	3.961	808	815	819	rBV3	418	669	0.07%	0.008%
15	3.990	819	824	827	rBV3	324	276	0.03%	0.003%
16	4.253	903	906	909	rBV2	348	264	0.03%	0.003%
17	4.417	953	957	961	rVV2	278	269	0.03%	0.003%
18	4.552	996	999	1002	rBV2	299	182	0.02%	0.002%
19	4.626	1006	1022	1061	rBV	120920	314630	31.16%	3.601%
20	4.932	1115	1117	1120	rVB2	436	199	0.02%	0.002%
21	4.951	1120	1123	1126	rBV2	294	179	0.02%	0.002%
22	4.970	1127	1129	1132	rVB3	429	222	0.02%	0.003%
23	5.064	1140	1158	1182	rBV	183565	405798	40.18%	4.645%
24	5.260	1217	1219	1223	rBV	270	228	0.02%	0.003%
25	5.292	1226	1229	1233	rBV2	442	285	0.03%	0.003%
26	5.372	1236	1254	1275	rBV	235278	481675	47.70%	5.513%
27	5.726	1342	1364	1396	rVV2	369300	1009865	100.00%	11.559%
28	5.835	1396	1398	1405	rVB3	672	598	0.06%	0.007%
29	5.893	1411	1416	1421	rBV3	347	408	0.04%	0.005%
30	6.115	1482	1485	1492	rVB2	370	330	0.03%	0.004%
31	6.250	1510	1527	1549	rBV	349198	660839	65.44%	7.564%
32	6.408	1571	1576	1581	rBV2	295	318	0.03%	0.004%
33	6.462	1589	1593	1596	rVB3	512	421	0.04%	0.005%
34	6.527	1607	1613	1621	rVB6	1631	2940	0.29%	0.034%
35	6.559	1621	1623	1628	rVB2	401	301	0.03%	0.003%
36	6.594	1628	1634	1635	rBV	203	185	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049305.D
 Acq On : 20 Jun 2022 15:01
 Operator : SY/MD
 Sample : N3395-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.690	1650	1664	1684	rBV	248960	485917	48.12%	5.562%
38	6.803	1694	1699	1700	rBV2	604	383	0.04%	0.004%
39	6.887	1722	1725	1732	rBV2	237	220	0.02%	0.003%
40	7.009	1760	1763	1772	rBV3	246	342	0.03%	0.004%
41	7.137	1799	1803	1808	rVB2	371	395	0.04%	0.005%
42	7.189	1808	1819	1829	rBV5	1490	2758	0.27%	0.032%
43	7.330	1860	1863	1865	rBV2	315	201	0.02%	0.002%
44	7.362	1870	1873	1876	rBV2	257	180	0.02%	0.002%
45	7.504	1914	1917	1919	rBV	391	242	0.02%	0.003%
46	7.565	1923	1936	1954	rBV	134107	236998	23.47%	2.713%
47	7.842	2018	2022	2024	rBV	262	216	0.02%	0.002%
48	7.896	2026	2039	2057	rBV	462367	803991	79.61%	9.203%
49	8.079	2092	2096	2098	rVB2	332	283	0.03%	0.003%
50	8.128	2106	2111	2112	rBV	244	238	0.02%	0.003%
51	8.179	2116	2127	2147	rVV	91948	157472	15.59%	1.802%
52	8.301	2161	2165	2167	rVB3	677	480	0.05%	0.005%
53	8.372	2184	2187	2195	rVB3	342	392	0.04%	0.004%
54	8.420	2198	2202	2204	rBV3	339	254	0.03%	0.003%
55	8.565	2242	2247	2250	rBV3	325	361	0.04%	0.004%
56	8.633	2256	2268	2314	rBV2	361088	696281	68.95%	7.970%
57	9.092	2407	2411	2415	rBV	299	283	0.03%	0.003%
58	9.163	2431	2433	2442	rVB3	297	337	0.03%	0.004%
59	9.202	2442	2445	2449	rBV3	226	212	0.02%	0.002%
60	9.240	2453	2457	2460	rBV2	314	243	0.02%	0.003%
61	9.321	2478	2482	2486	rBV3	353	427	0.04%	0.005%
62	9.369	2492	2497	2499	rBV	386	332	0.03%	0.004%
63	9.417	2499	2512	2533	rBV	479787	790873	78.31%	9.053%
64	9.787	2621	2627	2630	rBV3	347	335	0.03%	0.004%
65	9.858	2644	2649	2654	rVV2	317	286	0.03%	0.003%
66	10.025	2696	2701	2709	rVB3	394	729	0.07%	0.008%
67	10.105	2721	2726	2729	rBV2	361	309	0.03%	0.004%
68	10.131	2729	2734	2736	rBV2	318	283	0.03%	0.003%
69	10.298	2783	2786	2789	rVB2	354	256	0.03%	0.003%
70	10.356	2801	2804	2809	rBV2	307	283	0.03%	0.003%
71	10.481	2837	2843	2847	rBV	396	444	0.04%	0.005%
72	10.755	2915	2928	2950	rBV	349711	562708	55.72%	6.441%
73	10.864	2960	2962	2966	rBV2	230	203	0.02%	0.002%
74	10.951	2986	2989	2992	rVB2	300	195	0.02%	0.002%
75	11.121	3038	3042	3047	rBV2	369	436	0.04%	0.005%
76	11.549	3171	3175	3183	rVB3	331	425	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049305.D
 Acq On : 20 Jun 2022 15:01
 Operator : SY/MD
 Sample : N3395-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0160

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	11.607	3189	3193	3195	rBV2	272	237	0.02%	0.003%
78	11.665	3208	3211	3216	rVB3	242	232	0.02%	0.003%
79	11.812	3243	3257	3275	rBV	472787	758904	75.15%	8.687%
80	11.954	3298	3301	3303	rBV	379	225	0.02%	0.003%
81	11.973	3303	3307	3311	rVB2	257	250	0.02%	0.003%
82	12.115	3348	3351	3354	rVB	381	243	0.02%	0.003%
83	12.192	3362	3375	3391	rBV	459809	745359	73.81%	8.532%
84	12.430	3446	3449	3453	rBV2	421	353	0.03%	0.004%
85	12.526	3477	3479	3482	rBV	318	208	0.02%	0.002%
86	12.587	3493	3498	3499	rBV	251	213	0.02%	0.002%
87	12.600	3499	3502	3505	rVV2	316	243	0.02%	0.003%
88	12.719	3537	3539	3545	rVB2	325	253	0.03%	0.003%
89	12.751	3546	3549	3551	rBV2	277	210	0.02%	0.002%
90	12.957	3606	3613	3614	rBV3	391	442	0.04%	0.005%
91	12.986	3619	3622	3624	rBV2	279	177	0.02%	0.002%
92	13.050	3634	3642	3646	rBV2	530	738	0.07%	0.008%
93	13.214	3690	3693	3696	rBV	272	203	0.02%	0.002%
94	13.269	3707	3710	3712	rBV2	446	344	0.03%	0.004%
95	13.658	3828	3831	3834	rVB2	397	253	0.03%	0.003%
96	13.677	3834	3837	3838	rBV	289	188	0.02%	0.002%
97	13.841	3885	3888	3890	rBV2	319	223	0.02%	0.003%
98	13.970	3925	3928	3930	rBV2	325	222	0.02%	0.003%
99	14.089	3957	3965	3980	rBV4	5016	8703	0.86%	0.100%
100	15.629	4441	4444	4446	rBV2	608	386	0.04%	0.004%




Sum of corrected areas: 8736504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049305.D
Acq On : 20 Jun 2022 15:01
Operator : SY/MD
Sample : N3395-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

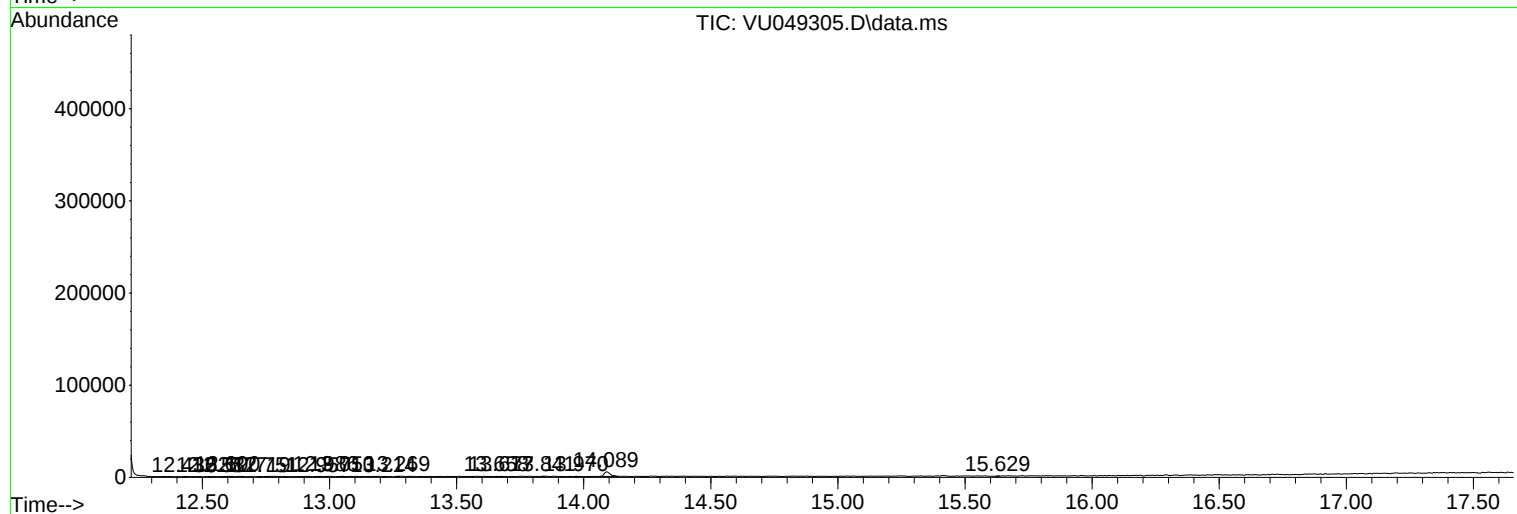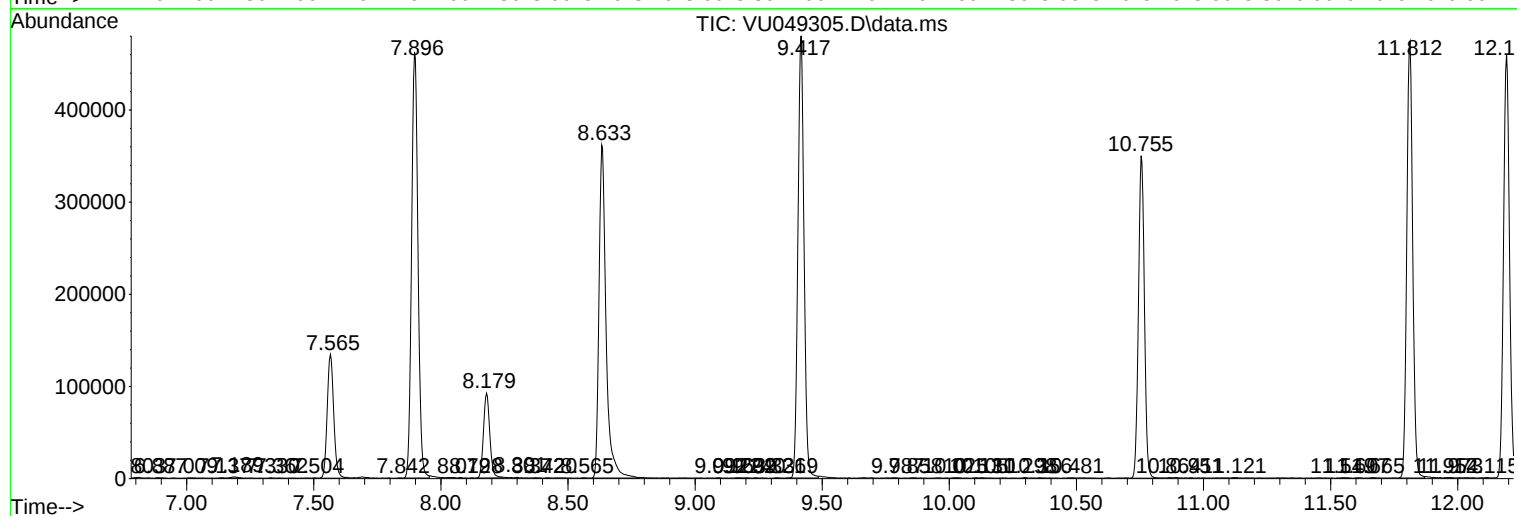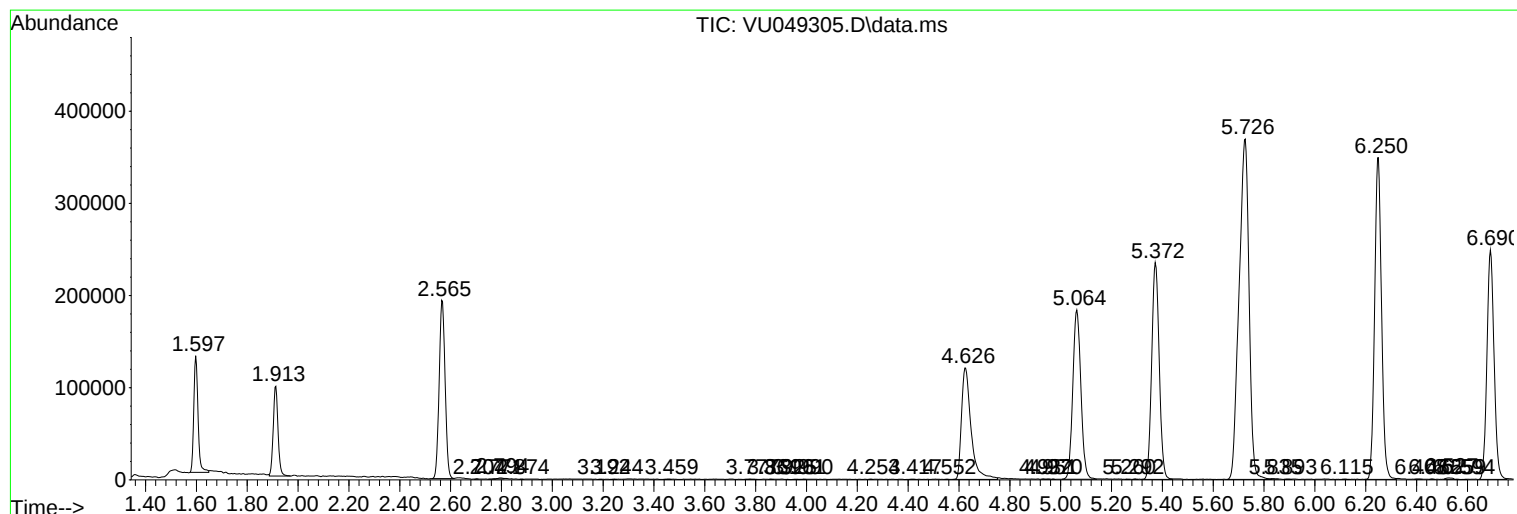

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049305.D
Acq On : 20 Jun 2022 15:01
Operator : SY/MD
Sample : N3395-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049305.D
Acq On : 20 Jun 2022 15:01
Operator : SY/MD
Sample : N3395-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0160

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc