

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049306.D
 Acq On : 20 Jun 2022 15:25
 Operator : SY/MD
 Sample : N3395-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	98	rBV	97336	109811	12.02%	1.441%
2	1.912	171	178	195	rVB	81806	105894	11.59%	1.390%
3	2.565	370	381	397	rBV	161259	261634	28.65%	3.434%
4	2.948	498	500	502	rVB	217	108	0.01%	0.001%
5	2.967	502	506	508	rBV	365	268	0.03%	0.004%
6	3.417	640	646	652	rBV3	461	556	0.06%	0.007%
7	3.446	652	655	656	rBV	187	121	0.01%	0.002%
8	3.497	669	671	673	rBV	148	99	0.01%	0.001%
9	3.588	695	699	701	rBV	261	171	0.02%	0.002%
10	3.690	725	731	734	rBV2	372	306	0.03%	0.004%
11	3.710	734	737	740	rVV2	201	138	0.02%	0.002%
12	3.790	758	762	764	rBV2	268	182	0.02%	0.002%
13	3.915	798	801	805	rVB2	263	167	0.02%	0.002%
14	3.941	808	809	810	rBV2	91	19	0.00%	0.000%
15	3.960	810	815	820	rBV3	337	396	0.04%	0.005%
16	3.989	821	824	828	rVB2	291	178	0.02%	0.002%
17	4.012	828	831	832	rBV	149	68	0.01%	0.001%
18	4.067	841	848	852	rBV3	465	592	0.06%	0.008%
19	4.102	857	859	861	rBV2	157	85	0.01%	0.001%
20	4.169	877	880	883	rBV	369	182	0.02%	0.002%
21	4.221	890	896	902	rBV2	359	530	0.06%	0.007%
22	4.263	906	909	914	rVB2	261	215	0.02%	0.003%
23	4.285	914	916	918	rBV	105	52	0.01%	0.001%
24	4.414	954	956	959	rVB	283	139	0.02%	0.002%
25	4.446	963	966	971	rVB	390	283	0.03%	0.004%
26	4.472	971	974	976	rVB2	179	109	0.01%	0.001%
27	4.488	976	979	982	rBV	228	140	0.02%	0.002%
28	4.507	982	985	987	rBV	186	147	0.02%	0.002%
29	4.620	1007	1020	1051	rBV	123187	295651	32.37%	3.880%
30	4.964	1123	1127	1130	rBV2	463	464	0.05%	0.006%
31	5.002	1137	1139	1142	rVB3	297	124	0.01%	0.002%
32	5.063	1142	1158	1177	rBV	171049	375348	41.10%	4.926%
33	5.372	1247	1254	1269	rBV6	1082	2198	0.24%	0.029%
34	5.433	1269	1273	1277	rBV2	297	252	0.03%	0.003%
35	5.533	1303	1304	1306	rBV2	189	88	0.01%	0.001%
36	5.626	1328	1333	1334	rBV	245	212	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049306.D
 Acq On : 20 Jun 2022 15:25
 Operator : SY/MD
 Sample : N3395-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1393	rBV2	332793	913361	100.00%	11.987%
38	5.906	1416	1420	1424	rBV4	485	404	0.04%	0.005%
39	5.964	1435	1438	1441	rBV2	216	125	0.01%	0.002%
40	6.034	1454	1460	1465	rBV2	327	420	0.05%	0.006%
41	6.067	1468	1470	1471	rBV2	150	67	0.01%	0.001%
42	6.176	1498	1504	1508	rBV4	405	405	0.04%	0.005%
43	6.250	1512	1527	1548	rBV	319190	603735	66.10%	7.923%
44	6.526	1605	1613	1629	rBV5	4986	10490	1.15%	0.138%
45	6.690	1650	1664	1689	rBV	228559	445280	48.75%	5.844%
46	6.857	1713	1716	1719	rVB	370	242	0.03%	0.003%
47	6.880	1721	1723	1724	rBV	116	47	0.01%	0.001%
48	6.912	1732	1733	1734	rBV	97	36	0.00%	0.000%
49	7.005	1758	1762	1766	rBV2	360	298	0.03%	0.004%
50	7.028	1766	1769	1774	rVV2	251	237	0.03%	0.003%
51	7.050	1774	1776	1779	rBV2	119	87	0.01%	0.001%
52	7.089	1786	1788	1790	rBV	138	75	0.01%	0.001%
53	7.105	1790	1793	1795	rBV	154	109	0.01%	0.001%
54	7.115	1795	1796	1798	rBV2	121	58	0.01%	0.001%
55	7.179	1813	1816	1818	rBV3	782	558	0.06%	0.007%
56	7.253	1836	1839	1843	rBV3	229	192	0.02%	0.003%
57	7.275	1843	1846	1849	rBV2	218	218	0.02%	0.003%
58	7.369	1873	1875	1877	rBV	204	82	0.01%	0.001%
59	7.391	1877	1882	1883	rBV2	196	162	0.02%	0.002%
60	7.462	1901	1904	1909	rBV2	238	255	0.03%	0.003%
61	7.565	1924	1936	1955	rBV	125909	221325	24.23%	2.905%
62	7.687	1969	1974	1984	rVB5	745	1326	0.15%	0.017%
63	7.787	2001	2005	2006	rBV2	401	263	0.03%	0.003%
64	7.832	2017	2019	2022	rBV3	269	123	0.01%	0.002%
65	7.896	2026	2039	2058	rBV	411097	712668	78.03%	9.353%
66	8.179	2116	2127	2147	rBV	86380	147548	16.15%	1.936%
67	8.414	2195	2200	2206	rBV3	313	341	0.04%	0.004%
68	8.443	2207	2209	2212	rBV2	189	125	0.01%	0.002%
69	8.552	2242	2243	2247	rVB	213	70	0.01%	0.001%
70	8.632	2256	2268	2307	rBV2	331604	647972	70.94%	8.504%
71	8.835	2328	2331	2337	rBV2	517	570	0.06%	0.007%
72	8.893	2346	2349	2353	rVB3	365	256	0.03%	0.003%
73	9.021	2385	2389	2394	rVB2	297	290	0.03%	0.004%
74	9.047	2394	2397	2402	rBV3	336	359	0.04%	0.005%
75	9.099	2410	2413	2419	rBV2	362	412	0.05%	0.005%
76	9.127	2419	2422	2425	rVB2	304	193	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049306.D
 Acq On : 20 Jun 2022 15:25
 Operator : SY/MD
 Sample : N3395-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0162

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.163	2430	2433	2436	rBV2	234	135	0.01%	0.002%
78	9.176	2436	2437	2438	rBV2	297	77	0.01%	0.001%
79	9.221	2448	2451	2452	rBV2	256	103	0.01%	0.001%
80	9.417	2499	2512	2529	rBV	449625	749157	82.02%	9.832%
81	9.610	2569	2572	2576	rBV2	281	178	0.02%	0.002%
82	9.687	2592	2596	2599	rBV3	621	594	0.07%	0.008%
83	9.738	2607	2612	2615	rBV3	271	267	0.03%	0.004%
84	10.050	2707	2709	2711	rBV3	141	68	0.01%	0.001%
85	10.066	2712	2714	2718	rBV	234	91	0.01%	0.001%
86	10.092	2719	2722	2723	rBV2	302	169	0.02%	0.002%
87	10.147	2735	2739	2742	rBV3	346	284	0.03%	0.004%
88	10.201	2750	2756	2759	rBV2	201	225	0.02%	0.003%
89	10.346	2797	2801	2805	rBV2	310	290	0.03%	0.004%
90	10.439	2826	2830	2833	rVB	378	247	0.03%	0.003%
91	10.587	2873	2876	2879	rBV2	175	127	0.01%	0.002%
92	10.616	2882	2885	2887	rBV	281	177	0.02%	0.002%
93	10.690	2906	2908	2911	rBV3	260	202	0.02%	0.003%
94	10.754	2915	2928	2945	rBV	333174	539756	59.10%	7.084%
95	10.861	2957	2961	2962	rBV	282	213	0.02%	0.003%
96	11.250	3079	3082	3087	rBV2	375	387	0.04%	0.005%
97	11.812	3244	3257	3277	rBV	474608	761081	83.33%	9.988%
98	12.192	3363	3375	3394	rBV	424369	697587	76.38%	9.155%
99	12.397	3437	3439	3441	rBV2	243	93	0.01%	0.001%
100	12.587	3494	3498	3500	rBV	462	403	0.04%	0.005%




Sum of corrected areas: 7619622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049306.D
Acq On : 20 Jun 2022 15:25
Operator : SY/MD
Sample : N3395-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

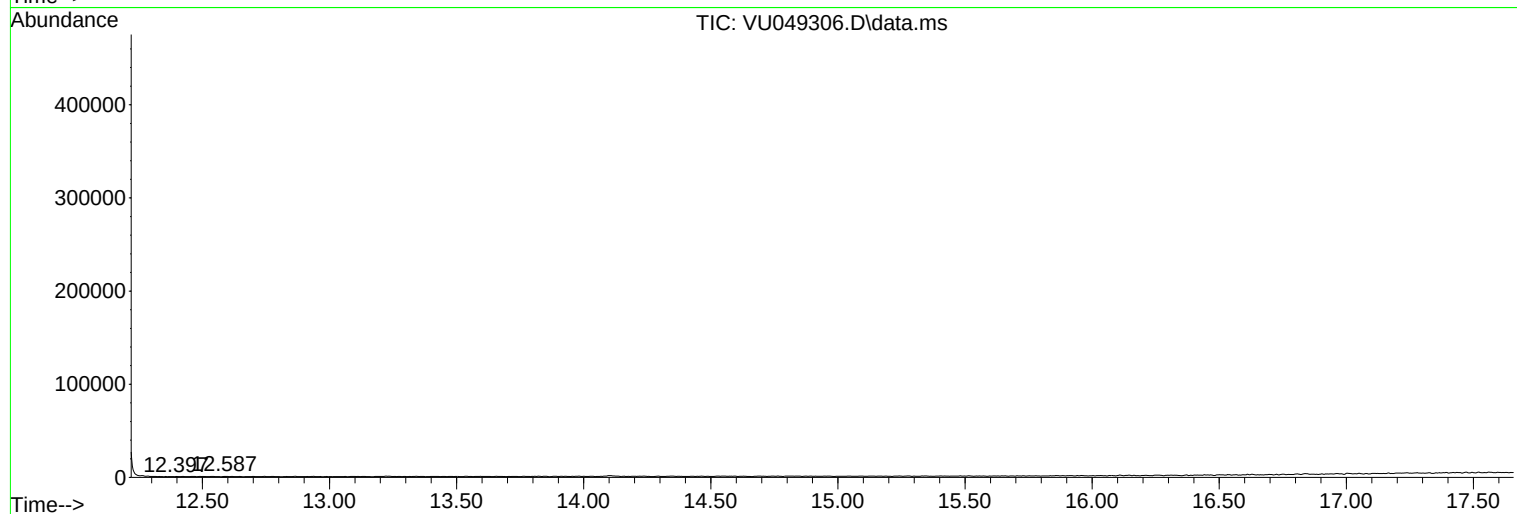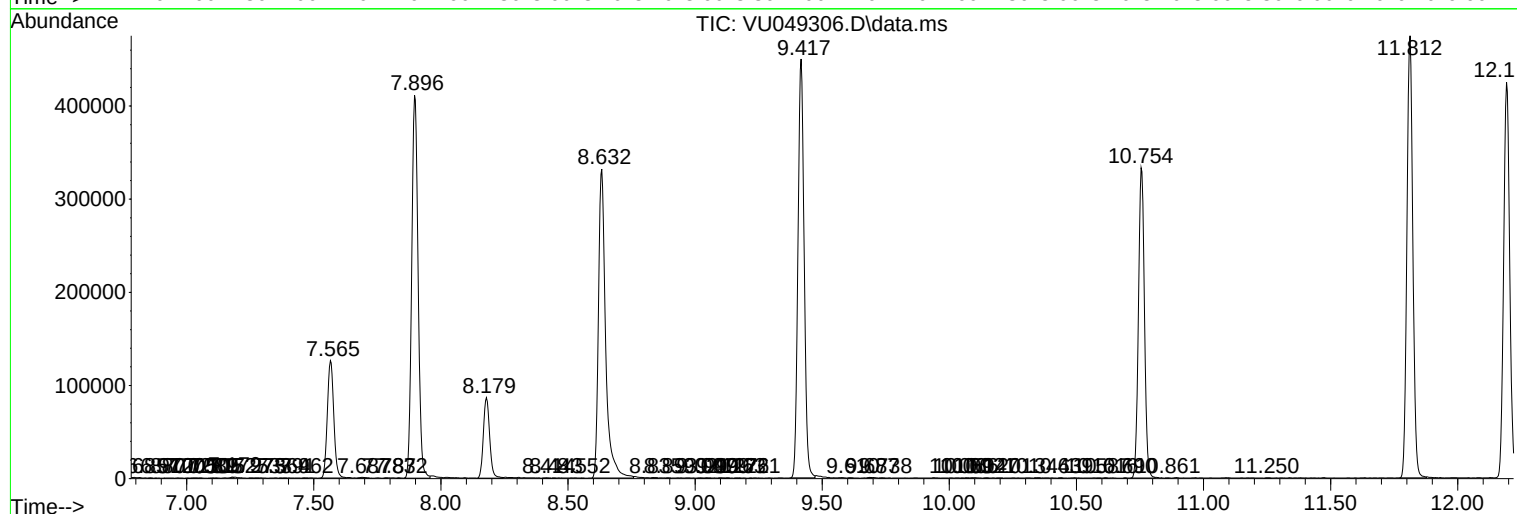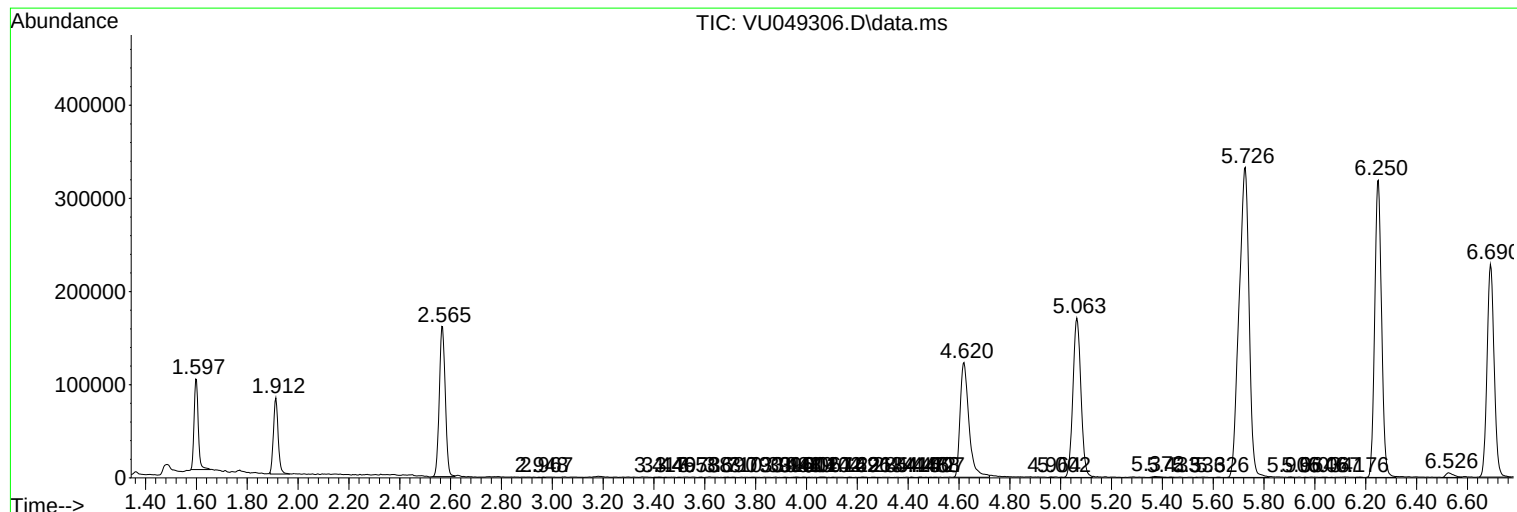

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049306.D
Acq On : 20 Jun 2022 15:25
Operator : SY/MD
Sample : N3395-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049306.D
Acq On : 20 Jun 2022 15:25
Operator : SY/MD
Sample : N3395-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0162

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc