

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049307.D
 Acq On : 20 Jun 2022 15:48
 Operator : SY/MD
 Sample : N3395-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	100	rVB	96583	108703	12.03%	1.438%
2	1.912	171	178	190	rVB	78598	101945	11.28%	1.349%
3	2.565	371	381	397	rVB	159188	255926	28.33%	3.387%
4	3.182	569	573	574	rBV	327	188	0.02%	0.002%
5	3.481	662	666	670	rVB2	350	327	0.04%	0.004%
6	3.507	670	674	675	rBV	281	202	0.02%	0.003%
7	3.591	697	700	702	rBV3	229	119	0.01%	0.002%
8	3.655	717	720	722	rBV2	282	190	0.02%	0.003%
9	3.681	725	728	732	rVV2	239	151	0.02%	0.002%
10	3.735	742	745	749	rVB2	221	133	0.01%	0.002%
11	3.755	749	751	754	rBV2	166	117	0.01%	0.002%
12	3.829	770	774	778	rVB	202	182	0.02%	0.002%
13	3.867	782	786	789	rBV3	264	227	0.03%	0.003%
14	3.903	795	797	803	rVB3	256	226	0.03%	0.003%
15	3.932	803	806	808	rBV2	209	151	0.02%	0.002%
16	4.105	857	860	861	rBV	249	127	0.01%	0.002%
17	4.208	888	892	895	rBV3	432	383	0.04%	0.005%
18	4.240	899	902	908	rVB3	349	281	0.03%	0.004%
19	4.272	909	912	914	rBV	248	157	0.02%	0.002%
20	4.330	927	930	932	rBV2	233	157	0.02%	0.002%
21	4.452	964	968	970	rBV2	246	207	0.02%	0.003%
22	4.478	973	976	978	rVV2	191	120	0.01%	0.002%
23	4.494	978	981	984	rVV	164	125	0.01%	0.002%
24	4.571	1000	1005	1008	rBV2	259	215	0.02%	0.003%
25	4.620	1008	1020	1051	rBV	124158	303155	33.55%	4.012%
26	5.063	1143	1158	1179	rBV	168135	368871	40.83%	4.881%
27	5.192	1196	1198	1202	rBV3	283	220	0.02%	0.003%
28	5.214	1202	1205	1209	rVB	591	333	0.04%	0.004%
29	5.359	1246	1250	1251	rBV	341	207	0.02%	0.003%
30	5.411	1264	1266	1271	rBV	221	163	0.02%	0.002%
31	5.449	1276	1278	1280	rVV2	266	131	0.01%	0.002%
32	5.475	1284	1286	1288	rVB	249	124	0.01%	0.002%
33	5.517	1297	1299	1302	rBV	204	135	0.01%	0.002%
34	5.539	1302	1306	1307	rBV	210	150	0.02%	0.002%
35	5.575	1313	1317	1319	rBV3	270	191	0.02%	0.003%
36	5.726	1343	1364	1391	rBV2	329488	903517	100.00%	11.956%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049307.D
 Acq On : 20 Jun 2022 15:48
 Operator : SY/MD
 Sample : N3395-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.957	1433	1436	1438	rBV	299	138	0.02%	0.002%
38	5.983	1441	1444	1447	rVB2	263	168	0.02%	0.002%
39	5.999	1447	1449	1452	rBV	236	151	0.02%	0.002%
40	6.015	1452	1454	1457	rBV2	173	137	0.02%	0.002%
41	6.070	1469	1471	1477	rVB2	302	208	0.02%	0.003%
42	6.102	1477	1481	1485	rVB2	326	262	0.03%	0.003%
43	6.128	1485	1489	1495	rBV2	431	452	0.05%	0.006%
44	6.250	1513	1527	1550	rBV	317016	599691	66.37%	7.936%
45	6.449	1585	1589	1591	rVB	249	162	0.02%	0.002%
46	6.478	1595	1598	1601	rBV2	339	285	0.03%	0.004%
47	6.526	1606	1613	1622	rBV4	1739	3110	0.34%	0.041%
48	6.581	1627	1630	1634	rVB3	262	218	0.02%	0.003%
49	6.639	1645	1648	1650	rBV	308	171	0.02%	0.002%
50	6.690	1650	1664	1687	rBV	226922	439343	48.63%	5.814%
51	6.803	1693	1699	1700	rBV3	472	444	0.05%	0.006%
52	6.880	1717	1723	1727	rBV2	329	352	0.04%	0.005%
53	6.980	1749	1754	1756	rBV2	159	169	0.02%	0.002%
54	6.999	1756	1760	1762	rVV2	226	151	0.02%	0.002%
55	7.185	1811	1818	1828	rBV4	1355	2055	0.23%	0.027%
56	7.263	1837	1842	1845	rBV	190	156	0.02%	0.002%
57	7.301	1851	1854	1857	rVB	299	166	0.02%	0.002%
58	7.320	1857	1860	1863	rVB	356	218	0.02%	0.003%
59	7.340	1863	1866	1868	rBV	217	159	0.02%	0.002%
60	7.407	1884	1887	1891	rVB2	330	219	0.02%	0.003%
61	7.565	1923	1936	1953	rBV	124741	218485	24.18%	2.891%
62	7.687	1971	1974	1983	rVB5	999	1361	0.15%	0.018%
63	7.726	1983	1986	1987	rBV2	299	175	0.02%	0.002%
64	7.896	2026	2039	2069	rBV	405726	707362	78.29%	9.361%
65	8.121	2106	2109	2113	rBV2	198	171	0.02%	0.002%
66	8.179	2115	2127	2146	rVV	87247	146955	16.26%	1.945%
67	8.343	2175	2178	2179	rBV2	298	170	0.02%	0.002%
68	8.449	2207	2211	2213	rBV	361	306	0.03%	0.004%
69	8.632	2255	2268	2297	rBV2	335824	650088	71.95%	8.603%
70	8.864	2335	2340	2346	rBV2	440	605	0.07%	0.008%
71	9.054	2397	2399	2402	rBV2	223	141	0.02%	0.002%
72	9.108	2410	2416	2420	rBV2	360	409	0.05%	0.005%
73	9.140	2424	2426	2431	rVV2	217	153	0.02%	0.002%
74	9.176	2434	2437	2440	rVB2	352	226	0.03%	0.003%
75	9.195	2440	2443	2446	rBV2	297	219	0.02%	0.003%
76	9.240	2455	2457	2460	rBV	214	134	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049307.D
 Acq On : 20 Jun 2022 15:48
 Operator : SY/MD
 Sample : N3395-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0163

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.346	2487	2490	2493	rVB2	346	215	0.02%	0.003%
78	9.417	2499	2512	2538	rBV	447477	746411	82.61%	9.877%
79	9.571	2557	2560	2563	rBV2	348	248	0.03%	0.003%
80	9.690	2593	2597	2602	rBV2	668	605	0.07%	0.008%
81	9.754	2614	2617	2622	rVB2	214	214	0.02%	0.003%
82	9.787	2622	2627	2629	rBV3	391	284	0.03%	0.004%
83	9.803	2629	2632	2634	rVV	239	155	0.02%	0.002%
84	9.832	2638	2641	2642	rBV	207	124	0.01%	0.002%
85	9.915	2663	2667	2670	rBV2	317	280	0.03%	0.004%
86	10.089	2715	2721	2724	rBV2	367	394	0.04%	0.005%
87	10.246	2765	2770	2772	rBV2	371	372	0.04%	0.005%
88	10.317	2788	2792	2794	rBV	204	139	0.02%	0.002%
89	10.346	2798	2801	2806	rBV2	302	309	0.03%	0.004%
90	10.529	2854	2858	2861	rBV3	306	225	0.02%	0.003%
91	10.754	2916	2928	2944	rBV	337312	537731	59.52%	7.116%
92	11.246	3078	3081	3083	rBV	271	209	0.02%	0.003%
93	11.349	3110	3113	3122	rBV3	372	435	0.05%	0.006%
94	11.510	3158	3163	3164	rBV2	244	212	0.02%	0.003%
95	11.742	3232	3235	3237	rBV2	354	246	0.03%	0.003%
96	11.812	3243	3257	3280	rBV	471805	752472	83.28%	9.958%
97	11.976	3305	3308	3310	rBV	315	185	0.02%	0.002%
98	12.192	3363	3375	3395	rBV	422949	691681	76.55%	9.153%
99	12.455	3455	3457	3460	rBV	219	130	0.01%	0.002%
100	13.176	3677	3681	3682	rBV2	263	190	0.02%	0.003%




Sum of corrected areas: 7556767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049307.D
Acq On : 20 Jun 2022 15:48
Operator : SY/MD
Sample : N3395-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

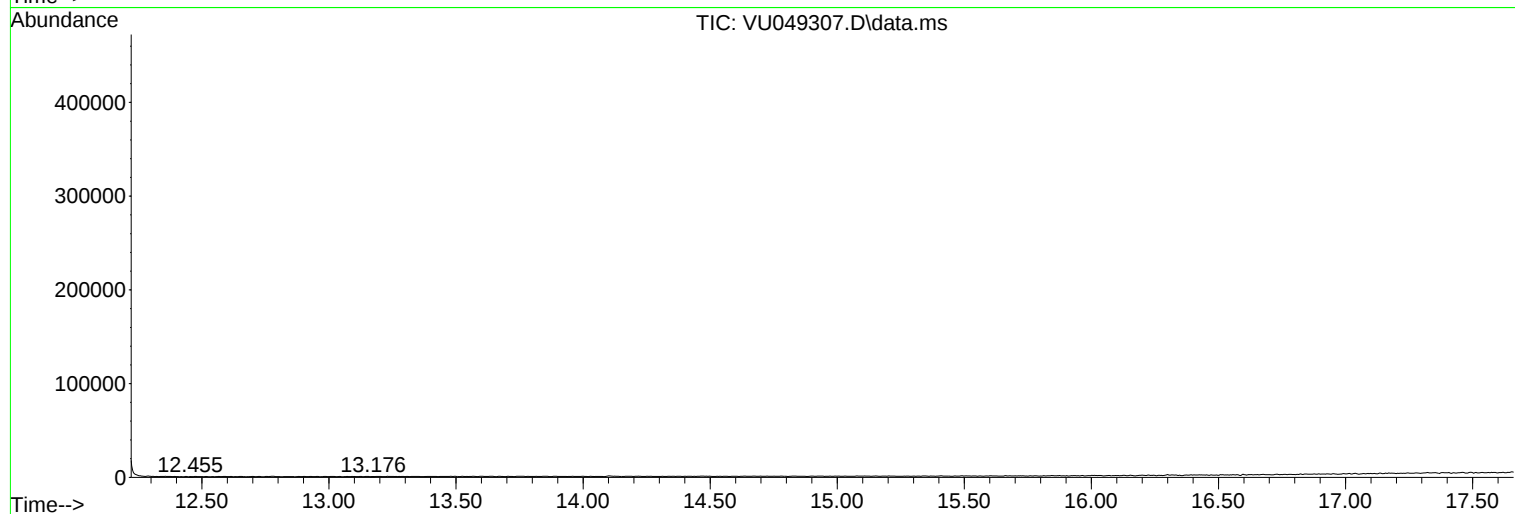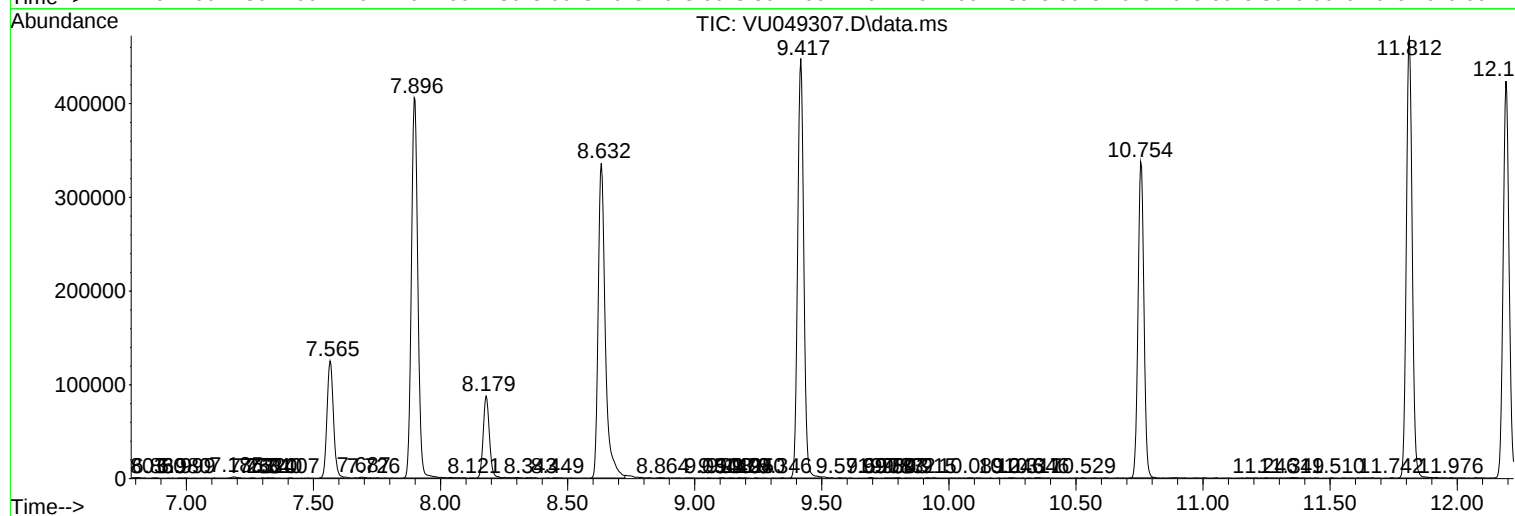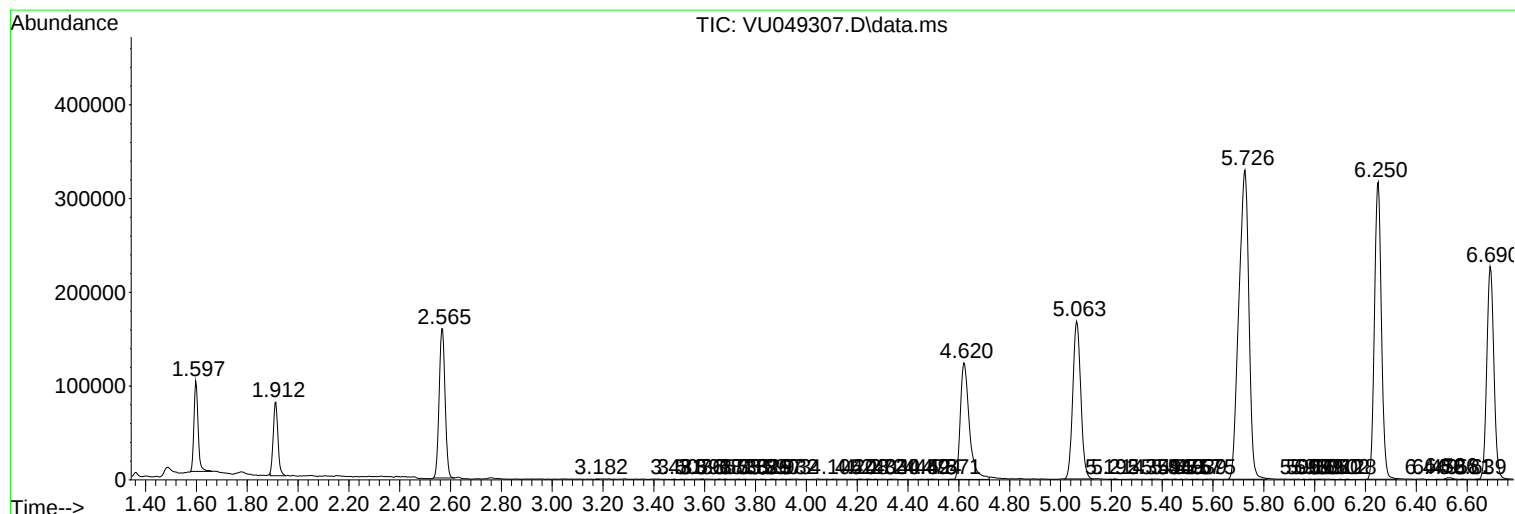

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049307.D
Acq On : 20 Jun 2022 15:48
Operator : SY/MD
Sample : N3395-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049307.D
Acq On : 20 Jun 2022 15:48
Operator : SY/MD
Sample : N3395-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0163

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------