

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049309.D
 Acq On : 20 Jun 2022 16:35
 Operator : SY/MD
 Sample : N3395-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	104	rVB	88513	102944	11.58%	1.408%
2	1.912	170	178	190	rBV	76611	97341	10.95%	1.331%
3	2.565	369	381	394	rBV	146697	236252	26.58%	3.231%
4	2.977	507	509	511	rBV2	321	143	0.02%	0.002%
5	3.067	534	537	546	rVB2	470	554	0.06%	0.008%
6	3.112	547	551	555	rBV2	379	406	0.05%	0.006%
7	3.186	568	574	581	rBV3	788	923	0.10%	0.013%
8	3.215	581	583	586	rBV2	293	157	0.02%	0.002%
9	3.427	647	649	653	rVB2	272	188	0.02%	0.003%
10	3.449	653	656	661	rBV2	355	374	0.04%	0.005%
11	3.475	661	664	670	rVB2	400	376	0.04%	0.005%
12	3.504	670	673	678	rBV3	466	443	0.05%	0.006%
13	3.549	684	687	688	rBV2	232	141	0.02%	0.002%
14	3.623	705	710	713	rBV2	272	212	0.02%	0.003%
15	3.674	719	726	728	rBV2	234	252	0.03%	0.003%
16	3.761	749	753	757	rBV	239	258	0.03%	0.004%
17	3.806	764	767	770	rBV	224	148	0.02%	0.002%
18	3.928	802	805	806	rBV	292	165	0.02%	0.002%
19	4.051	840	843	845	rBV2	337	263	0.03%	0.004%
20	4.096	853	857	859	rBV2	289	231	0.03%	0.003%
21	4.134	863	869	873	rBV2	397	440	0.05%	0.006%
22	4.240	899	902	906	rBV3	306	263	0.03%	0.004%
23	4.305	919	922	926	rVB2	311	227	0.03%	0.003%
24	4.350	934	936	941	rVB2	330	221	0.02%	0.003%
25	4.372	941	943	946	rBV	230	161	0.02%	0.002%
26	4.565	1000	1003	1007	rBV2	212	175	0.02%	0.002%
27	4.616	1007	1019	1052	rBV	120126	292351	32.89%	3.998%
28	5.063	1142	1158	1183	rBV	168108	366282	41.21%	5.010%
29	5.247	1212	1215	1222	rVB3	429	434	0.05%	0.006%
30	5.391	1258	1260	1262	rBV	210	126	0.01%	0.002%
31	5.481	1286	1288	1292	rVB2	307	208	0.02%	0.003%
32	5.517	1296	1299	1302	rBV	277	189	0.02%	0.003%
33	5.571	1313	1316	1318	rBV	205	127	0.01%	0.002%
34	5.584	1318	1320	1323	rVV2	288	178	0.02%	0.002%
35	5.726	1342	1364	1391	rBV2	323782	888869	100.00%	12.157%
36	5.999	1446	1449	1453	rBV2	167	133	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049309.D
 Acq On : 20 Jun 2022 16:35
 Operator : SY/MD
 Sample : N3395-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.057	1464	1467	1473	rVB2	301	263	0.03%	0.004%
38	6.086	1473	1476	1478	rBV2	198	142	0.02%	0.002%
39	6.134	1488	1491	1495	rVB3	280	184	0.02%	0.003%
40	6.198	1507	1511	1513	rBV2	273	212	0.02%	0.003%
41	6.250	1513	1527	1548	rVV	291682	556511	62.61%	7.611%
42	6.468	1592	1595	1598	rVB	237	165	0.02%	0.002%
43	6.526	1606	1613	1621	rBV4	1782	2715	0.31%	0.037%
44	6.558	1621	1623	1626	rVB2	337	183	0.02%	0.003%
45	6.600	1633	1636	1637	rBV2	324	168	0.02%	0.002%
46	6.690	1650	1664	1684	rBV	223738	437375	49.21%	5.982%
47	6.803	1695	1699	1703	rBV3	630	681	0.08%	0.009%
48	6.893	1723	1727	1729	rBV	289	223	0.03%	0.003%
49	6.922	1733	1736	1741	rVV2	157	134	0.02%	0.002%
50	7.002	1759	1761	1764	rBV2	271	187	0.02%	0.003%
51	7.095	1788	1790	1794	rVB	356	229	0.03%	0.003%
52	7.118	1794	1797	1801	rBV2	433	299	0.03%	0.004%
53	7.185	1811	1818	1825	rVB4	1095	1817	0.20%	0.025%
54	7.243	1833	1836	1838	rBV2	285	206	0.02%	0.003%
55	7.298	1849	1853	1855	rBV3	246	207	0.02%	0.003%
56	7.391	1876	1882	1887	rVB3	310	377	0.04%	0.005%
57	7.417	1887	1890	1891	rBV	228	131	0.01%	0.002%
58	7.430	1891	1894	1897	rBV2	275	200	0.02%	0.003%
59	7.478	1906	1909	1914	rBV2	268	228	0.03%	0.003%
60	7.565	1923	1936	1953	rBV	122005	214951	24.18%	2.940%
61	7.687	1967	1974	1975	rBV4	721	713	0.08%	0.010%
62	7.809	2007	2012	2014	rBV3	334	277	0.03%	0.004%
63	7.899	2026	2040	2058	rBV	389370	681722	76.70%	9.324%
64	8.118	2104	2108	2111	rBV2	300	275	0.03%	0.004%
65	8.179	2115	2127	2148	rBV	85641	144868	16.30%	1.981%
66	8.533	2229	2237	2242	rBV3	417	569	0.06%	0.008%
67	8.632	2255	2268	2302	rBV2	324959	648979	73.01%	8.876%
68	8.832	2328	2330	2333	rBV2	320	186	0.02%	0.003%
69	8.873	2337	2343	2344	rBV2	243	233	0.03%	0.003%
70	9.134	2421	2424	2428	rVB2	189	127	0.01%	0.002%
71	9.166	2428	2434	2436	rBV3	321	333	0.04%	0.005%
72	9.259	2458	2463	2465	rBV2	344	332	0.04%	0.005%
73	9.304	2474	2477	2480	rVV	381	317	0.04%	0.004%
74	9.333	2484	2486	2489	rBV	242	167	0.02%	0.002%
75	9.417	2499	2512	2530	rBV	420615	701026	78.87%	9.588%
76	9.574	2553	2561	2566	rVB4	420	609	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049309.D
 Acq On : 20 Jun 2022 16:35
 Operator : SY/MD
 Sample : N3395-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0165

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.623	2573	2576	2580	rVB2	323	234	0.03%	0.003%
78	9.738	2609	2612	2615	rVB2	387	214	0.02%	0.003%
79	9.767	2618	2621	2626	rBV3	301	252	0.03%	0.003%
80	9.825	2635	2639	2641	rBV2	403	317	0.04%	0.004%
81	9.915	2664	2667	2670	rBV2	269	219	0.02%	0.003%
82	9.935	2670	2673	2676	rVB2	268	177	0.02%	0.002%
83	9.957	2676	2680	2685	rBV2	331	358	0.04%	0.005%
84	10.041	2703	2706	2710	rBV2	287	237	0.03%	0.003%
85	10.230	2763	2765	2769	rBV	342	228	0.03%	0.003%
86	10.391	2809	2815	2821	rBV3	319	457	0.05%	0.006%
87	10.433	2825	2828	2833	rVV	280	210	0.02%	0.003%
88	10.523	2850	2856	2859	rBV2	271	325	0.04%	0.004%
89	10.542	2859	2862	2863	rBV	217	136	0.02%	0.002%
90	10.629	2885	2889	2891	rBV3	286	219	0.02%	0.003%
91	10.706	2908	2913	2915	rBV	257	247	0.03%	0.003%
92	10.754	2915	2928	2948	rVV	334151	539885	60.74%	7.384%
93	11.089	3027	3032	3033	rBV2	369	268	0.03%	0.004%
94	11.475	3150	3152	3155	rBV	230	128	0.01%	0.002%
95	11.520	3162	3166	3170	rBV2	299	293	0.03%	0.004%
96	11.542	3170	3173	3180	rVB3	325	351	0.04%	0.005%
97	11.571	3180	3182	3185	rBV	280	163	0.02%	0.002%
98	11.812	3245	3257	3285	rBV	434927	700683	78.83%	9.583%
99	12.192	3363	3375	3393	rBV	420775	674976	75.94%	9.232%
100	12.314	3410	3413	3417	rBV3	362	290	0.03%	0.004%




Sum of corrected areas: 7311543

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049309.D
Acq On : 20 Jun 2022 16:35
Operator : SY/MD
Sample : N3395-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

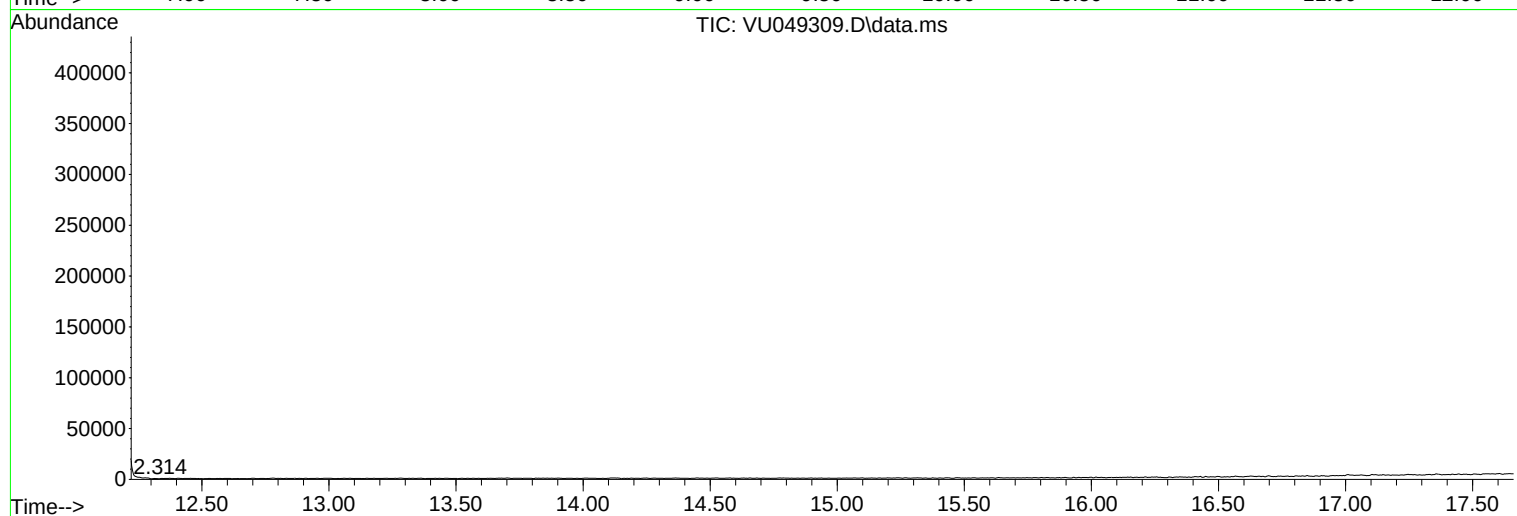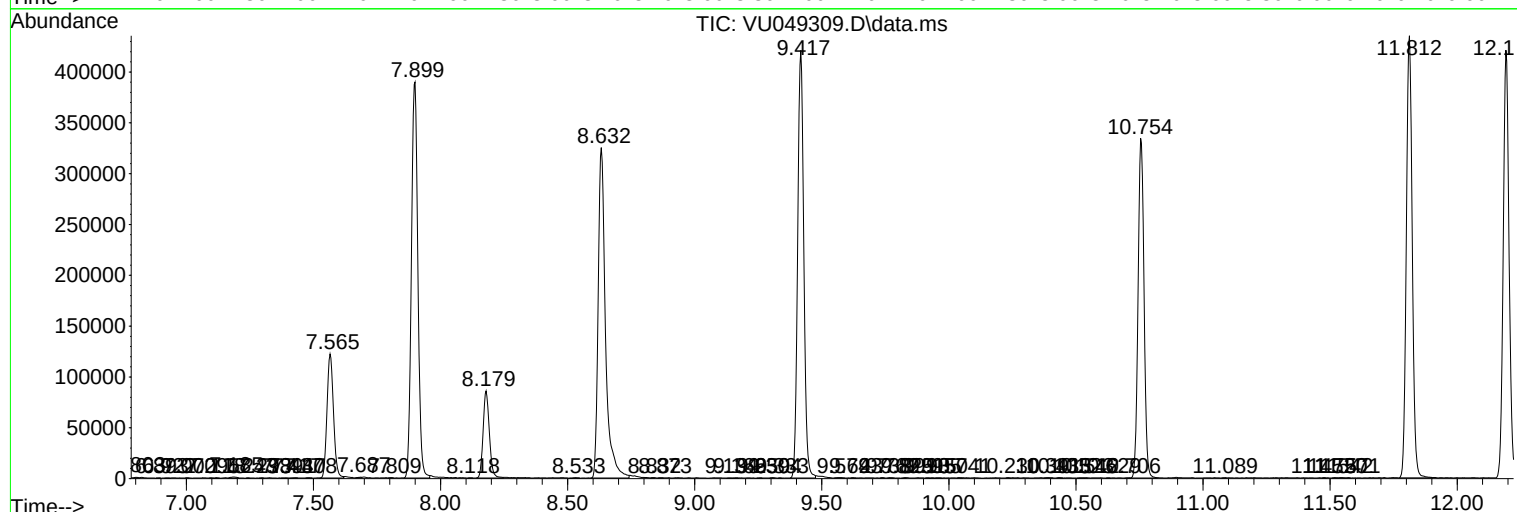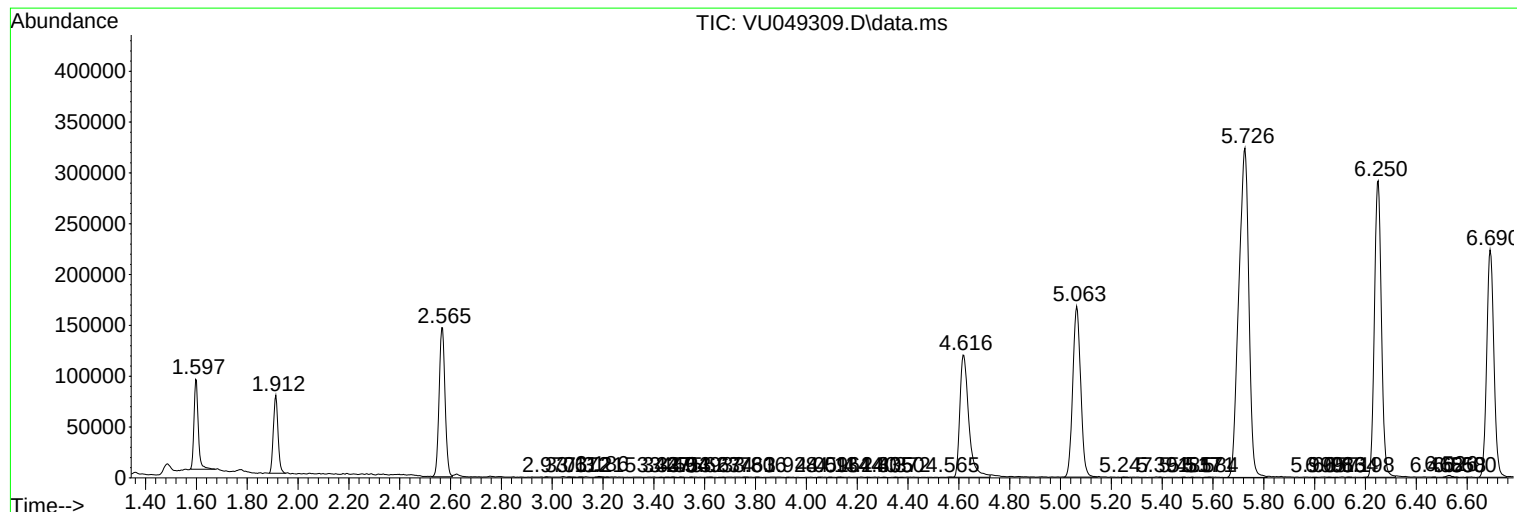

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049309.D
Acq On : 20 Jun 2022 16:35
Operator : SY/MD
Sample : N3395-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049309.D
Acq On : 20 Jun 2022 16:35
Operator : SY/MD
Sample : N3395-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0165

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------