

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049312.D
 Acq On : 20 Jun 2022 17:46
 Operator : SY/MD
 Sample : N3395-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	99	rVB	96812	110536	12.36%	1.474%
2	1.912	171	178	192	rVB	77349	100455	11.23%	1.339%
3	2.565	370	381	392	rBV	157382	253876	28.39%	3.385%
4	2.742	433	436	437	rBV	733	486	0.05%	0.006%
5	2.842	463	467	471	rVB2	340	262	0.03%	0.003%
6	3.015	520	521	526	rVB	366	223	0.02%	0.003%
7	3.041	526	529	530	rBV	384	203	0.02%	0.003%
8	3.089	541	544	547	rBV2	237	174	0.02%	0.002%
9	3.131	555	557	560	rBV	269	174	0.02%	0.002%
10	3.501	669	672	673	rBV	231	145	0.02%	0.002%
11	3.526	677	680	684	rVB2	216	157	0.02%	0.002%
12	3.555	686	689	693	rVV3	202	159	0.02%	0.002%
13	3.597	700	702	707	rVB3	391	263	0.03%	0.004%
14	3.690	729	731	734	rVV	171	110	0.01%	0.001%
15	3.735	742	745	747	rBV	176	138	0.02%	0.002%
16	3.835	773	776	779	rBV3	267	214	0.02%	0.003%
17	3.922	800	803	806	rBV2	272	173	0.02%	0.002%
18	3.951	810	812	816	rVV2	396	246	0.03%	0.003%
19	3.980	816	821	825	rVB2	421	438	0.05%	0.006%
20	4.002	825	828	831	rBV2	204	135	0.02%	0.002%
21	4.160	875	877	883	rVB2	344	236	0.03%	0.003%
22	4.195	883	888	893	rBV2	375	340	0.04%	0.005%
23	4.285	913	916	918	rBV2	196	138	0.02%	0.002%
24	4.372	939	943	944	rBV	237	194	0.02%	0.003%
25	4.520	987	989	993	rBV2	277	164	0.02%	0.002%
26	4.549	993	998	1001	rBV3	389	378	0.04%	0.005%
27	4.620	1007	1020	1042	rBV	121898	292686	32.73%	3.902%
28	4.976	1127	1131	1134	rBV2	472	403	0.05%	0.005%
29	5.063	1142	1158	1179	rBV	167607	371696	41.56%	4.955%
30	5.211	1202	1204	1206	rBV	361	205	0.02%	0.003%
31	5.282	1220	1226	1228	rBV3	375	345	0.04%	0.005%
32	5.385	1254	1258	1263	rVB3	269	295	0.03%	0.004%
33	5.449	1274	1278	1279	rBV	192	136	0.02%	0.002%
34	5.558	1309	1312	1318	rBV	123	145	0.02%	0.002%
35	5.726	1339	1364	1385	rBV2	330609	894347	100.00%	11.923%
36	5.970	1433	1440	1447	rBV3	633	705	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049312.D
 Acq On : 20 Jun 2022 17:46
 Operator : SY/MD
 Sample : N3395-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.005	1447	1451	1454	rVB3	374	277	0.03%	0.004%
38	6.025	1454	1457	1458	rBV	276	151	0.02%	0.002%
39	6.041	1458	1462	1463	rBV2	314	194	0.02%	0.003%
40	6.073	1470	1472	1474	rBV2	189	116	0.01%	0.002%
41	6.153	1495	1497	1504	rVB2	307	354	0.04%	0.005%
42	6.250	1512	1527	1553	rBV	308799	594678	66.49%	7.928%
43	6.533	1604	1615	1625	rVB7	2021	4346	0.49%	0.058%
44	6.578	1625	1629	1630	rBV	468	299	0.03%	0.004%
45	6.690	1650	1664	1683	rBV	223690	438168	48.99%	5.842%
46	6.870	1717	1720	1722	rBV2	359	262	0.03%	0.003%
47	6.886	1722	1725	1733	rVB3	1023	870	0.10%	0.012%
48	7.057	1774	1778	1780	rBV3	394	289	0.03%	0.004%
49	7.118	1795	1797	1799	rBV3	247	117	0.01%	0.002%
50	7.160	1807	1810	1812	rBV3	307	224	0.03%	0.003%
51	7.185	1812	1818	1826	rVB5	1533	2276	0.25%	0.030%
52	7.221	1826	1829	1831	rBV	230	145	0.02%	0.002%
53	7.298	1849	1853	1856	rBV3	324	282	0.03%	0.004%
54	7.356	1866	1871	1872	rBV3	405	336	0.04%	0.004%
55	7.420	1888	1891	1893	rBV	358	226	0.03%	0.003%
56	7.468	1903	1906	1908	rBV2	236	155	0.02%	0.002%
57	7.507	1916	1918	1920	rBV2	190	135	0.02%	0.002%
58	7.565	1924	1936	1954	rBV	121596	215428	24.09%	2.872%
59	7.687	1969	1974	1983	rBV5	1130	1701	0.19%	0.023%
60	7.899	2026	2040	2057	rBV	400121	696397	77.87%	9.284%
61	8.115	2102	2107	2111	rBV3	342	386	0.04%	0.005%
62	8.179	2116	2127	2148	rVV	86284	144149	16.12%	1.922%
63	8.320	2167	2171	2173	rBV3	340	313	0.03%	0.004%
64	8.375	2184	2188	2191	rVB3	484	307	0.03%	0.004%
65	8.420	2196	2202	2205	rBV3	216	259	0.03%	0.003%
66	8.449	2205	2211	2214	rBV	473	517	0.06%	0.007%
67	8.632	2256	2268	2301	rBV2	337227	649717	72.65%	8.662%
68	8.922	2355	2358	2363	rVB3	590	402	0.04%	0.005%
69	9.066	2400	2403	2405	rBV	284	158	0.02%	0.002%
70	9.092	2408	2411	2416	rVB3	268	202	0.02%	0.003%
71	9.124	2416	2421	2426	rBV2	342	409	0.05%	0.005%
72	9.185	2435	2440	2444	rVB3	316	320	0.04%	0.004%
73	9.211	2446	2448	2451	rBV2	205	135	0.02%	0.002%
74	9.417	2499	2512	2543	rBV	442619	735297	82.22%	9.803%
75	9.571	2557	2560	2563	rBV2	343	241	0.03%	0.003%
76	9.639	2578	2581	2586	rBV3	266	260	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049312.D
 Acq On : 20 Jun 2022 17:46
 Operator : SY/MD
 Sample : N3395-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0170

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.697	2594	2599	2603	rBV4	478	499	0.06%	0.007%
78	9.748	2613	2615	2620	rBV2	249	180	0.02%	0.002%
79	9.803	2629	2632	2634	rBV	315	169	0.02%	0.002%
80	9.976	2682	2686	2689	rBV3	357	357	0.04%	0.005%
81	10.034	2701	2704	2707	rBV	196	129	0.01%	0.002%
82	10.092	2718	2722	2724	rBV	264	211	0.02%	0.003%
83	10.275	2777	2779	2781	rBV	315	142	0.02%	0.002%
84	10.346	2791	2801	2806	rBV5	1406	1726	0.19%	0.023%
85	10.369	2806	2808	2811	rVB2	226	119	0.01%	0.002%
86	10.452	2831	2834	2837	rBV	319	258	0.03%	0.003%
87	10.571	2861	2871	2882	rVB5	3140	5542	0.62%	0.074%
88	10.706	2910	2913	2916	rVV	325	231	0.03%	0.003%
89	10.754	2916	2928	2947	rVV	332850	534647	59.78%	7.128%
90	10.841	2951	2955	2961	rBV4	392	493	0.06%	0.007%
91	10.873	2961	2965	2966	rBV	215	141	0.02%	0.002%
92	11.224	3071	3074	3076	rBV2	213	155	0.02%	0.002%
93	11.314	3101	3102	3106	rBV2	201	155	0.02%	0.002%
94	11.475	3145	3152	3161	rBV5	2607	4605	0.51%	0.061%
95	11.812	3244	3257	3275	rBV	458234	729903	81.61%	9.731%
96	12.018	3319	3321	3324	rBV2	204	125	0.01%	0.002%
97	12.073	3331	3338	3351	rVB7	2243	4075	0.46%	0.054%
98	12.192	3363	3375	3403	rBV	417728	688761	77.01%	9.182%
99	12.378	3423	3433	3447	rBV8	3561	6366	0.71%	0.085%
100	13.005	3624	3628	3633	rBV3	414	401	0.04%	0.005%




Sum of corrected areas: 7500868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049312.D
Acq On : 20 Jun 2022 17:46
Operator : SY/MD
Sample : N3395-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

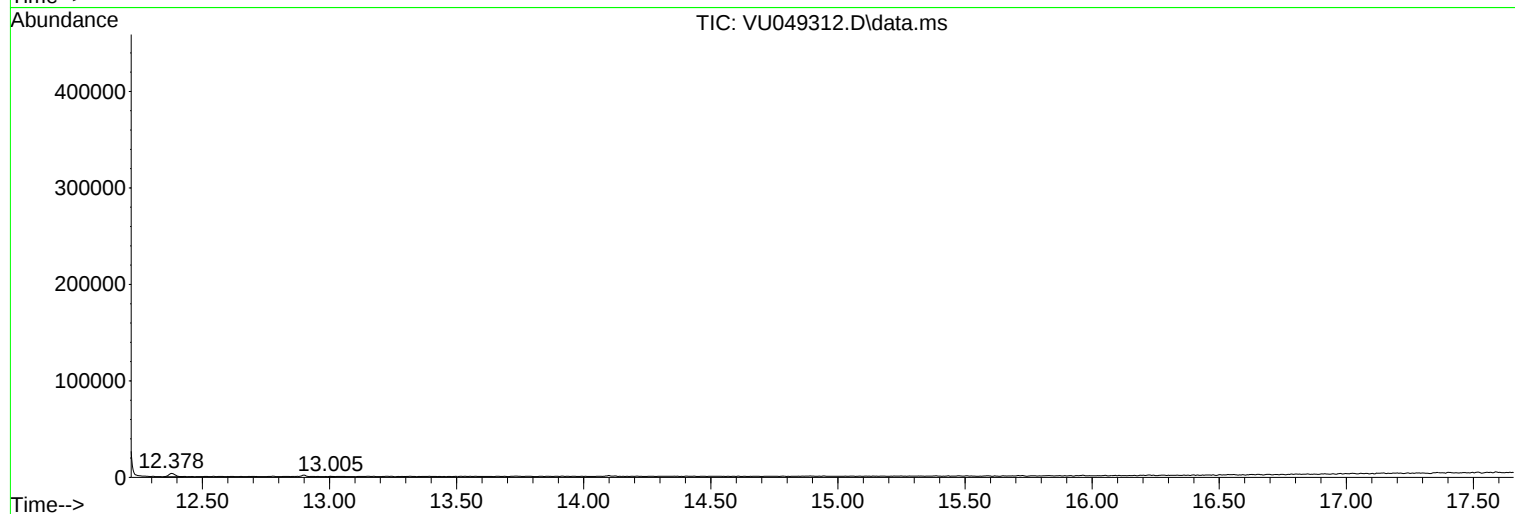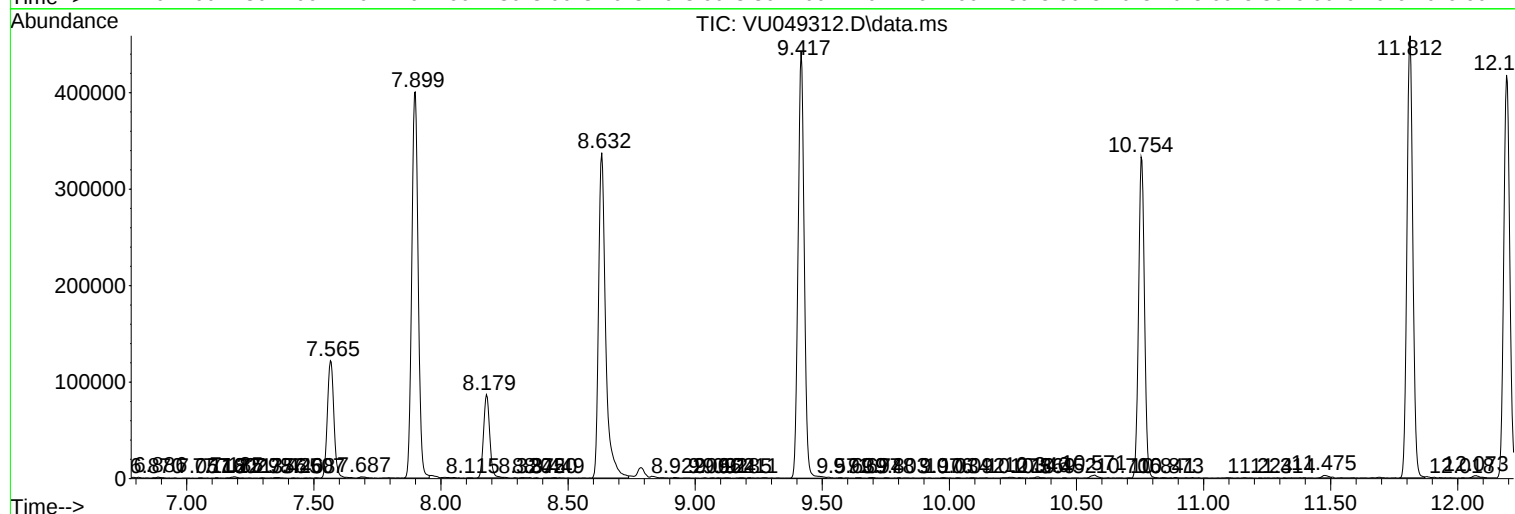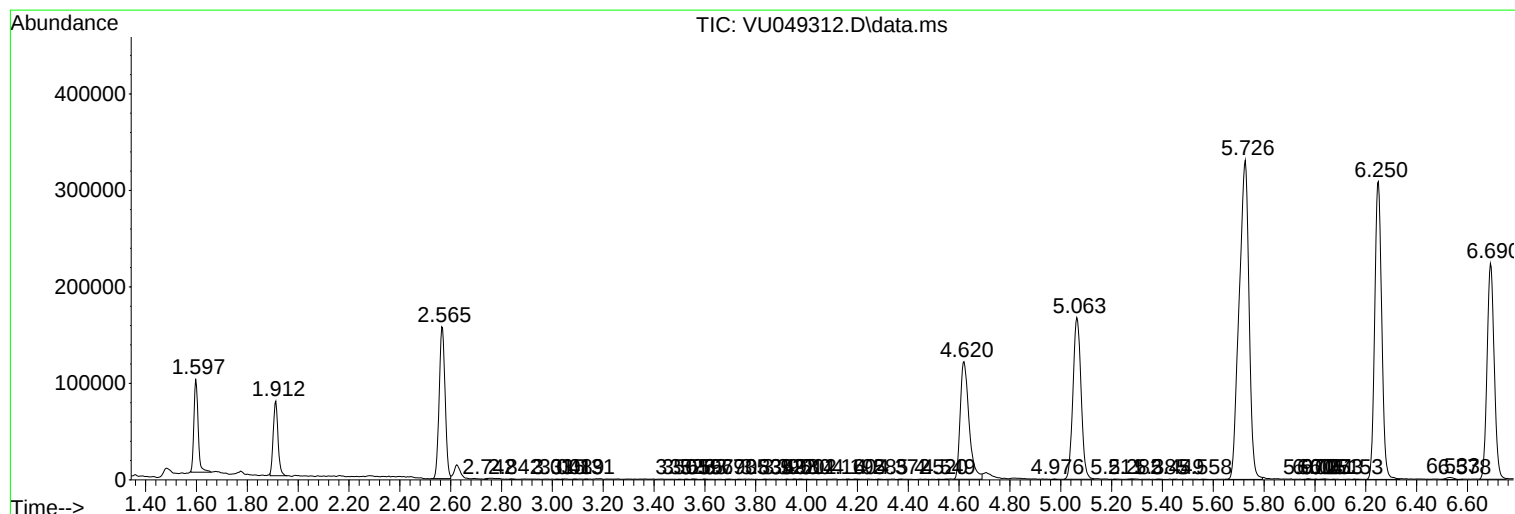

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049312.D
Acq On : 20 Jun 2022 17:46
Operator : SY/MD
Sample : N3395-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049312.D
Acq On : 20 Jun 2022 17:46
Operator : SY/MD
Sample : N3395-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0170

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc