

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049314.D
 Acq On : 20 Jun 2022 18:33
 Operator : SY/MD
 Sample : N3396-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	89	rBV	85480	92481	10.53%	1.264%
2	1.909	170	177	191	rVB	75178	96971	11.05%	1.325%
3	2.565	369	381	393	rBV	145541	233791	26.63%	3.196%
4	3.128	548	556	566	rBV6	1140	2200	0.25%	0.030%
5	3.308	609	612	614	rBV2	295	201	0.02%	0.003%
6	3.337	618	621	624	rVV2	542	370	0.04%	0.005%
7	3.359	625	628	636	rVV4	597	634	0.07%	0.009%
8	3.472	660	663	665	rBV2	190	130	0.01%	0.002%
9	3.488	665	668	674	rVV2	358	334	0.04%	0.005%
10	3.620	705	709	710	rBV2	234	147	0.02%	0.002%
11	3.732	740	744	746	rBV2	260	255	0.03%	0.003%
12	3.874	783	788	792	rBV3	300	333	0.04%	0.005%
13	3.925	801	804	808	rVB2	221	181	0.02%	0.002%
14	3.999	824	827	831	rVV2	261	209	0.02%	0.003%
15	4.028	833	836	840	rVV3	322	270	0.03%	0.004%
16	4.198	887	889	897	rVB3	316	269	0.03%	0.004%
17	4.276	911	913	919	rVB2	276	192	0.02%	0.003%
18	4.372	938	943	949	rBV2	250	271	0.03%	0.004%
19	4.404	949	953	955	rBV2	345	233	0.03%	0.003%
20	4.562	997	1002	1004	rBV3	257	229	0.03%	0.003%
21	4.620	1007	1020	1043	rBV	123376	295189	33.63%	4.035%
22	4.967	1125	1128	1130	rBV3	279	198	0.02%	0.003%
23	5.063	1141	1158	1189	rVV	165774	366558	41.76%	5.010%
24	5.211	1201	1204	1208	rBV3	429	395	0.04%	0.005%
25	5.288	1222	1228	1231	rBV3	361	419	0.05%	0.006%
26	5.353	1246	1248	1251	rBV2	168	129	0.01%	0.002%
27	5.452	1274	1279	1282	rVV	330	317	0.04%	0.004%
28	5.555	1307	1311	1314	rBV2	234	175	0.02%	0.002%
29	5.594	1319	1323	1326	rBV2	353	307	0.03%	0.004%
30	5.726	1343	1364	1389	rVV2	320318	877853	100.00%	11.999%
31	5.967	1434	1439	1441	rBV2	286	274	0.03%	0.004%
32	6.022	1452	1456	1458	rBV2	317	283	0.03%	0.004%
33	6.070	1465	1471	1473	rBV	238	225	0.03%	0.003%
34	6.083	1473	1475	1481	rVB2	207	130	0.01%	0.002%
35	6.247	1513	1526	1553	rVV	297866	566263	64.51%	7.740%
36	6.452	1587	1590	1597	rBV3	340	333	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049314.D
 Acq On : 20 Jun 2022 18:33
 Operator : SY/MD
 Sample : N3396-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.530	1607	1614	1621	rBV6	1758	3056	0.35%	0.042%
38	6.584	1628	1631	1633	rBV2	347	186	0.02%	0.003%
39	6.690	1650	1664	1684	rBV	221576	431567	49.16%	5.899%
40	6.848	1712	1713	1716	rVB2	333	129	0.01%	0.002%
41	6.880	1716	1723	1730	rBV5	1225	1895	0.22%	0.026%
42	6.932	1736	1739	1742	rVB2	307	199	0.02%	0.003%
43	6.954	1743	1746	1750	rVV2	285	255	0.03%	0.003%
44	7.108	1786	1794	1803	rVB4	481	738	0.08%	0.010%
45	7.179	1810	1816	1817	rBV2	1016	768	0.09%	0.010%
46	7.243	1832	1836	1842	rBV	240	270	0.03%	0.004%
47	7.288	1844	1850	1854	rBV2	344	399	0.05%	0.005%
48	7.337	1861	1865	1868	rVB	382	278	0.03%	0.004%
49	7.359	1868	1872	1873	rBV2	593	394	0.04%	0.005%
50	7.430	1891	1894	1896	rBV	209	148	0.02%	0.002%
51	7.504	1912	1917	1919	rBV2	228	227	0.03%	0.003%
52	7.565	1923	1936	1960	rVV	120621	213620	24.33%	2.920%
53	7.732	1986	1988	1992	rVB2	304	173	0.02%	0.002%
54	7.780	1999	2003	2005	rBV3	345	268	0.03%	0.004%
55	7.896	2026	2039	2056	rBV	390039	671334	76.47%	9.176%
56	8.179	2112	2127	2144	rBV	84143	140628	16.02%	1.922%
57	8.404	2194	2197	2199	rVB2	352	203	0.02%	0.003%
58	8.430	2199	2205	2206	rBV2	177	140	0.02%	0.002%
59	8.459	2210	2214	2215	rBV	253	221	0.03%	0.003%
60	8.546	2235	2241	2244	rBV3	283	389	0.04%	0.005%
61	8.632	2256	2268	2306	rBV2	337360	654424	74.55%	8.945%
62	8.951	2365	2367	2373	rVB2	298	270	0.03%	0.004%
63	8.983	2373	2377	2381	rBV2	243	307	0.03%	0.004%
64	9.102	2409	2414	2417	rBV3	215	208	0.02%	0.003%
65	9.137	2421	2425	2430	rBV3	387	391	0.04%	0.005%
66	9.250	2457	2460	2465	rBV3	237	220	0.03%	0.003%
67	9.362	2493	2495	2499	rBV2	231	127	0.01%	0.002%
68	9.417	2499	2512	2534	rBV	427745	710789	80.97%	9.716%
69	9.578	2560	2562	2566	rVB2	466	248	0.03%	0.003%
70	9.603	2567	2570	2573	rVV3	254	165	0.02%	0.002%
71	9.697	2592	2599	2606	rBV3	912	1007	0.11%	0.014%
72	9.742	2611	2613	2618	rBV	383	260	0.03%	0.004%
73	9.832	2635	2641	2652	rVB3	390	768	0.09%	0.010%
74	9.880	2652	2656	2660	rBV3	399	426	0.05%	0.006%
75	9.992	2684	2691	2694	rVB2	365	399	0.05%	0.005%
76	10.246	2760	2770	2775	rBV3	1149	1965	0.22%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049314.D
 Acq On : 20 Jun 2022 18:33
 Operator : SY/MD
 Sample : N3396-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0167

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	10.285	2779	2782	2783	rBV	250	144	0.02%	0.002%
78	10.320	2790	2793	2794	rBV	188	124	0.01%	0.002%
79	10.533	2857	2859	2862	rBV2	220	150	0.02%	0.002%
80	10.562	2862	2868	2881	rVV5	2111	3898	0.44%	0.053%
81	10.639	2889	2892	2895	rBV3	282	210	0.02%	0.003%
82	10.754	2916	2928	2949	rVV	332129	535952	61.05%	7.326%
83	10.841	2952	2955	2961	rBV2	268	271	0.03%	0.004%
84	11.102	3032	3036	3039	rBV	383	269	0.03%	0.004%
85	11.127	3042	3044	3046	rVB2	314	130	0.01%	0.002%
86	11.246	3078	3081	3084	rBV2	250	189	0.02%	0.003%
87	11.324	3101	3105	3109	rBV2	389	433	0.05%	0.006%
88	11.449	3141	3144	3146	rBV2	313	177	0.02%	0.002%
89	11.481	3146	3154	3165	rVV3	2094	3963	0.45%	0.054%
90	11.690	3215	3219	3222	rBV4	579	482	0.05%	0.007%
91	11.751	3229	3238	3244	rVB5	1658	2581	0.29%	0.035%
92	11.812	3244	3257	3275	rBV	439125	706045	80.43%	9.651%
93	12.070	3325	3337	3345	rBV6	2672	4919	0.56%	0.067%
94	12.192	3362	3375	3398	rBV	401587	668222	76.12%	9.134%
95	12.378	3427	3433	3435	rBV4	2236	2466	0.28%	0.034%
96	12.893	3589	3593	3602	rBV4	1254	1761	0.20%	0.024%
97	13.086	3649	3653	3657	rBV2	411	359	0.04%	0.005%
98	13.295	3714	3718	3721	rBV2	452	486	0.06%	0.007%
99	13.500	3779	3782	3786	rBV2	358	375	0.04%	0.005%
100	13.848	3882	3890	3904	rVB4	2597	4164	0.47%	0.057%




Sum of corrected areas: 7315978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049314.D
Acq On : 20 Jun 2022 18:33
Operator : SY/MD
Sample : N3396-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

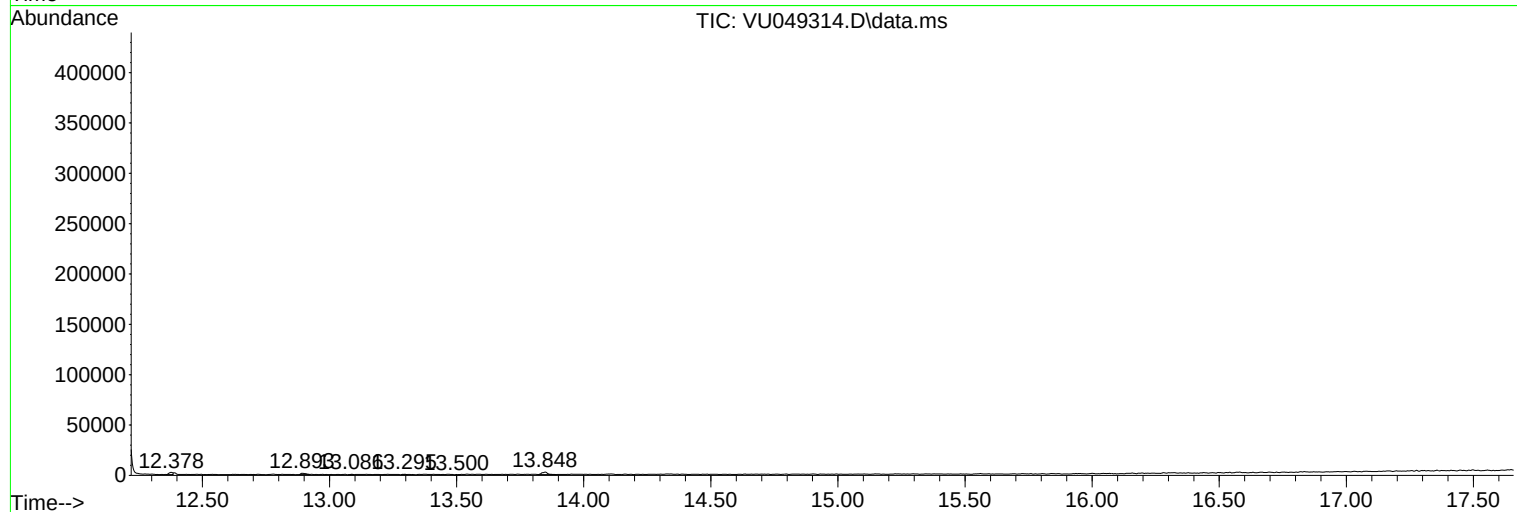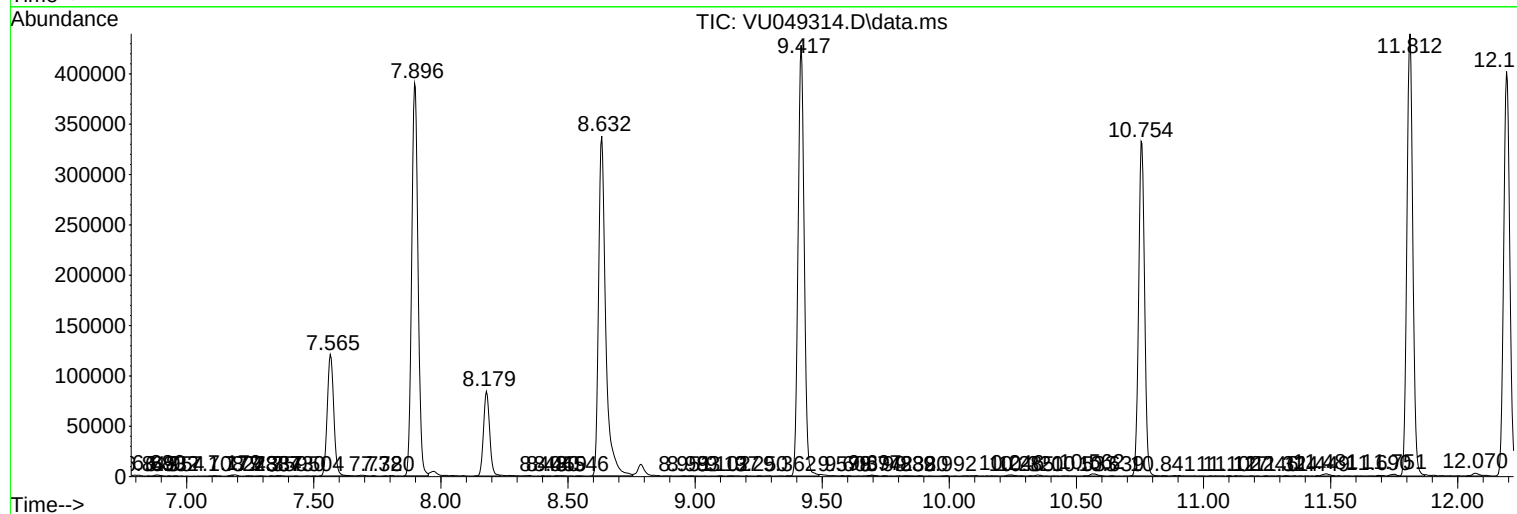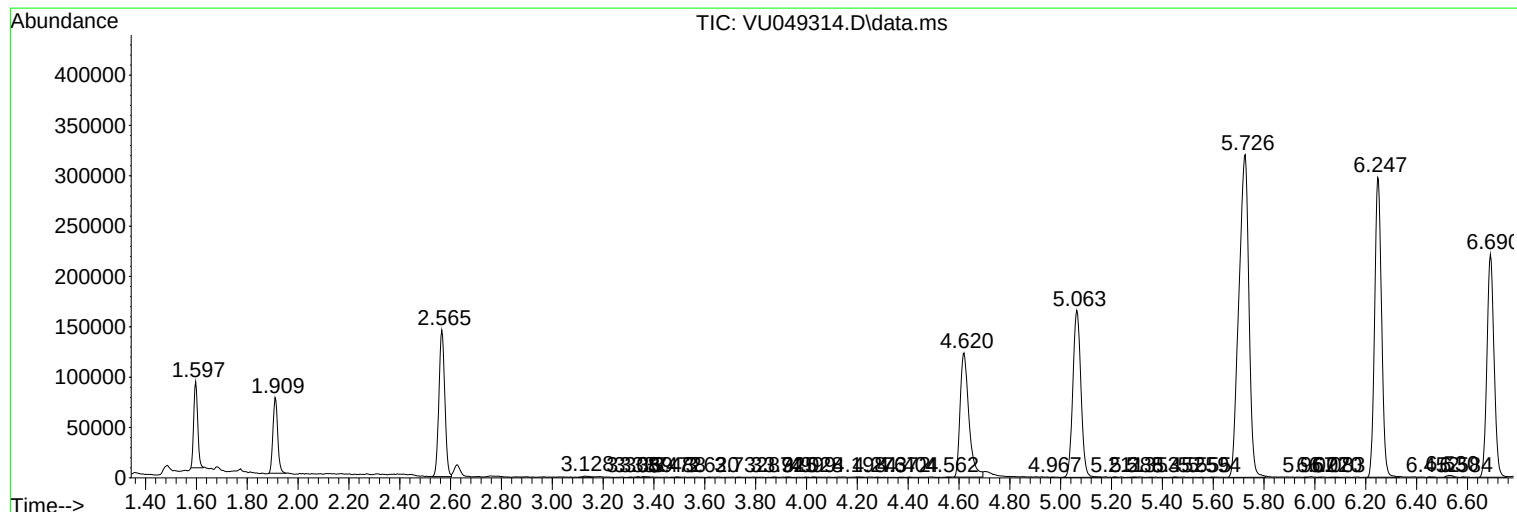

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049314.D
Acq On : 20 Jun 2022 18:33
Operator : SY/MD
Sample : N3396-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049314.D
Acq On : 20 Jun 2022 18:33
Operator : SY/MD
Sample : N3396-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0167

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc