

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049315.D
 Acq On : 20 Jun 2022 18:57
 Operator : SY/MD
 Sample : N3396-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	99	rBV	86658	96321	11.13%	1.334%
2	1.909	170	177	189	rVB	72487	93644	10.82%	1.297%
3	2.565	369	381	393	rBV	142683	230354	26.61%	3.190%
4	2.893	481	483	487	rVB2	369	248	0.03%	0.003%
5	3.041	525	529	530	rBV2	601	375	0.04%	0.005%
6	3.121	552	554	559	rBV3	203	190	0.02%	0.003%
7	3.363	625	629	634	rBV3	491	634	0.07%	0.009%
8	3.408	639	643	647	rBV3	288	241	0.03%	0.003%
9	3.430	647	650	654	rVB2	460	352	0.04%	0.005%
10	3.456	654	658	660	rBV2	332	230	0.03%	0.003%
11	3.588	696	699	705	rVB3	366	338	0.04%	0.005%
12	3.620	705	709	712	rBV2	362	330	0.04%	0.005%
13	3.687	727	730	734	rBV3	413	399	0.05%	0.006%
14	3.719	738	740	743	rVV2	233	150	0.02%	0.002%
15	3.790	758	762	764	rBV3	255	222	0.03%	0.003%
16	3.877	785	789	794	rBV2	401	403	0.05%	0.006%
17	3.948	808	811	813	rVV2	271	128	0.01%	0.002%
18	4.070	846	849	852	rVB2	375	210	0.02%	0.003%
19	4.092	853	856	860	rBV2	236	191	0.02%	0.003%
20	4.346	932	935	938	rVB	316	238	0.03%	0.003%
21	4.382	944	946	948	rBV2	240	138	0.02%	0.002%
22	4.620	1004	1020	1041	rBV	121140	290197	33.52%	4.019%
23	5.063	1140	1158	1179	rBV	164240	359323	41.51%	4.976%
24	5.186	1193	1196	1197	rBV	311	176	0.02%	0.002%
25	5.247	1210	1215	1219	rBV2	420	358	0.04%	0.005%
26	5.279	1219	1225	1227	rBV3	513	571	0.07%	0.008%
27	5.369	1251	1253	1257	rBV2	212	139	0.02%	0.002%
28	5.430	1269	1272	1275	rVB2	211	138	0.02%	0.002%
29	5.449	1275	1278	1280	rBV3	208	114	0.01%	0.002%
30	5.465	1280	1283	1285	rBV3	197	110	0.01%	0.002%
31	5.726	1341	1364	1390	rBV2	316411	865682	100.00%	11.989%
32	6.038	1459	1461	1465	rBV2	356	272	0.03%	0.004%
33	6.083	1470	1475	1477	rBV2	205	176	0.02%	0.002%
34	6.176	1497	1504	1508	rVB4	424	533	0.06%	0.007%
35	6.250	1512	1527	1555	rBV	295941	562392	64.97%	7.789%
36	6.469	1592	1595	1597	rBV2	381	302	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049315.D
 Acq On : 20 Jun 2022 18:57
 Operator : SY/MD
 Sample : N3396-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	6.526	1606	1613	1614	rBV3	1685	1621	0.19%	0.022%
38	6.594	1631	1634	1639	rVB2	530	381	0.04%	0.005%
39	6.636	1644	1647	1650	rBV	311	282	0.03%	0.004%
40	6.690	1650	1664	1693	rVV	222783	427883	49.43%	5.926%
41	6.803	1697	1699	1702	rBV2	562	313	0.04%	0.004%
42	6.861	1714	1717	1718	rBV	255	121	0.01%	0.002%
43	6.877	1720	1722	1725	rVV2	560	346	0.04%	0.005%
44	6.925	1732	1737	1739	rBV	252	247	0.03%	0.003%
45	6.967	1746	1750	1752	rBV2	316	198	0.02%	0.003%
46	7.073	1778	1783	1790	rBV3	497	657	0.08%	0.009%
47	7.186	1810	1818	1826	rBV5	1312	2101	0.24%	0.029%
48	7.234	1830	1833	1839	rVB3	350	349	0.04%	0.005%
49	7.288	1848	1850	1853	rVB	339	138	0.02%	0.002%
50	7.324	1853	1861	1865	rVB3	290	385	0.04%	0.005%
51	7.359	1868	1872	1874	rBV3	624	500	0.06%	0.007%
52	7.395	1881	1883	1886	rVB2	222	136	0.02%	0.002%
53	7.417	1886	1890	1893	rBV3	273	251	0.03%	0.003%
54	7.565	1924	1936	1955	rBV	118788	210845	24.36%	2.920%
55	7.687	1969	1974	1978	rBB4	738	712	0.08%	0.010%
56	7.745	1988	1992	1995	rBV2	446	338	0.04%	0.005%
57	7.784	1998	2004	2007	rBV2	501	589	0.07%	0.008%
58	7.896	2026	2039	2057	rBV	379811	661946	76.47%	9.168%
59	8.179	2116	2127	2144	rVV	82422	137926	15.93%	1.910%
60	8.369	2184	2186	2188	rBV	332	191	0.02%	0.003%
61	8.468	2211	2217	2221	rBV2	461	554	0.06%	0.008%
62	8.507	2227	2229	2232	rVB3	363	208	0.02%	0.003%
63	8.571	2244	2249	2250	rBV2	308	232	0.03%	0.003%
64	8.632	2256	2268	2303	rBV2	322875	642814	74.26%	8.903%
65	8.896	2345	2350	2354	rBV3	336	338	0.04%	0.005%
66	8.941	2362	2364	2369	rVB	266	195	0.02%	0.003%
67	9.070	2400	2404	2405	rBV	173	118	0.01%	0.002%
68	9.102	2411	2414	2419	rVB3	323	274	0.03%	0.004%
69	9.189	2438	2441	2444	rBV2	275	165	0.02%	0.002%
70	9.234	2453	2455	2459	rBV2	261	192	0.02%	0.003%
71	9.311	2477	2479	2485	rVB2	239	219	0.03%	0.003%
72	9.417	2499	2512	2530	rBV	426594	710036	82.02%	9.834%
73	9.722	2605	2607	2610	rBV2	205	132	0.02%	0.002%
74	9.803	2630	2632	2637	rVB2	378	261	0.03%	0.004%
75	9.857	2645	2649	2654	rVB3	253	248	0.03%	0.003%
76	9.909	2663	2665	2670	rVB	297	231	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049315.D
 Acq On : 20 Jun 2022 18:57
 Operator : SY/MD
 Sample : N3396-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0168

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.944	2673	2676	2678	rBV2	282	209	0.02%	0.003%
78	9.983	2684	2688	2692	rBV3	396	302	0.03%	0.004%
79	10.021	2696	2700	2703	rVV3	285	226	0.03%	0.003%
80	10.073	2713	2716	2718	rBV	268	198	0.02%	0.003%
81	10.240	2762	2768	2773	rBV4	672	952	0.11%	0.013%
82	10.320	2789	2793	2794	rBV	289	216	0.02%	0.003%
83	10.346	2798	2801	2807	rVB2	1040	915	0.11%	0.013%
84	10.436	2823	2829	2832	rBV2	464	445	0.05%	0.006%
85	10.568	2862	2870	2880	rBV6	3125	5916	0.68%	0.082%
86	10.703	2909	2912	2916	rBV3	325	314	0.04%	0.004%
87	10.755	2916	2928	2951	rVB	323899	528329	61.03%	7.317%
88	10.902	2965	2974	2978	rBV3	890	1174	0.14%	0.016%
89	10.928	2979	2982	2989	rVB3	366	336	0.04%	0.005%
90	11.189	3060	3063	3065	rBV	191	112	0.01%	0.002%
91	11.259	3081	3085	3087	rBV2	223	193	0.02%	0.003%
92	11.552	3170	3176	3180	rBV3	465	528	0.06%	0.007%
93	11.578	3181	3184	3185	rBV	233	124	0.01%	0.002%
94	11.812	3244	3257	3275	rBV	438411	704084	81.33%	9.751%
95	12.028	3321	3324	3326	rBV2	273	153	0.02%	0.002%
96	12.070	3331	3337	3349	rVB6	2482	4786	0.55%	0.066%
97	12.192	3362	3375	3397	rBV	401738	654676	75.63%	9.067%
98	12.378	3426	3433	3441	rVB6	3463	5175	0.60%	0.072%
99	13.285	3712	3715	3717	rBV2	405	288	0.03%	0.004%
100	13.848	3887	3890	3892	rBV2	653	363	0.04%	0.005%




Sum of corrected areas: 7220506

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049315.D
Acq On : 20 Jun 2022 18:57
Operator : SY/MD
Sample : N3396-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0168

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

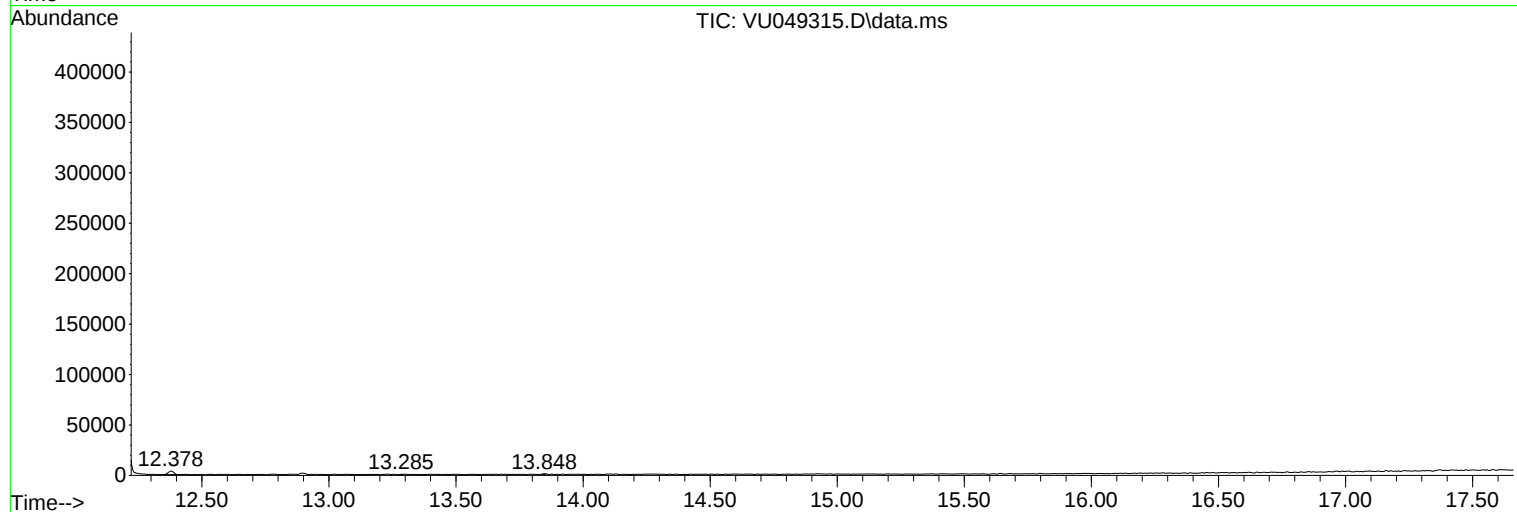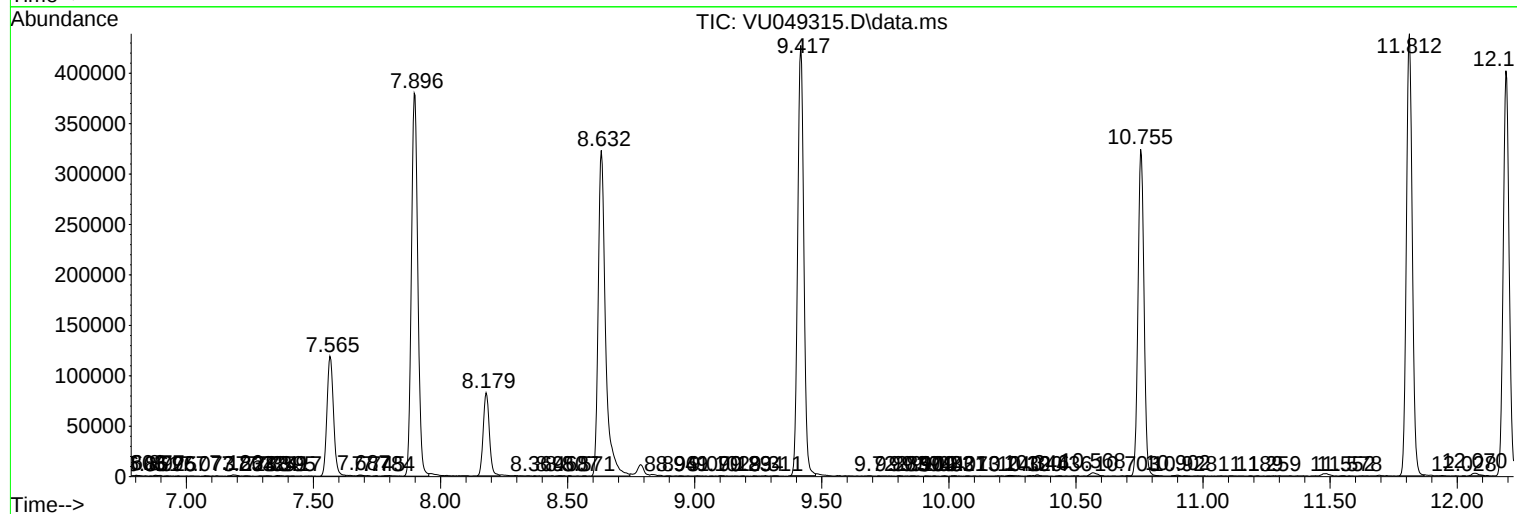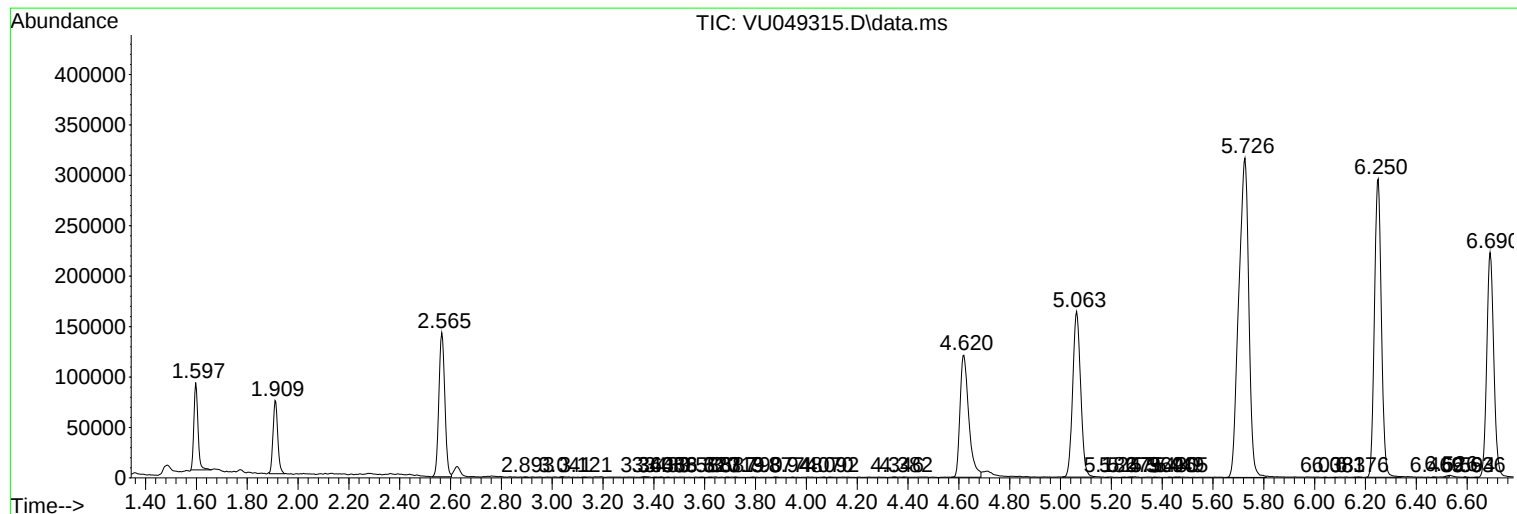

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049315.D
Acq On : 20 Jun 2022 18:57
Operator : SY/MD
Sample : N3396-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0168

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049315.D
Acq On : 20 Jun 2022 18:57
Operator : SY/MD
Sample : N3396-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0168

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------