

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049316.D
 Acq On : 20 Jun 2022 19:20
 Operator : SY/MD
 Sample : N3396-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	90	rBV	95737	103240	11.37%	1.366%
2	1.913	170	178	190	rVB	79489	103780	11.43%	1.373%
3	2.565	370	381	397	rBV	157216	255829	28.17%	3.385%
4	2.912	486	489	491	rBV3	246	158	0.02%	0.002%
5	3.044	524	530	544	rVB4	1899	3327	0.37%	0.044%
6	3.189	562	575	589	rVB	3293	7490	0.82%	0.099%
7	3.298	607	609	613	rBV	193	127	0.01%	0.002%
8	3.388	634	637	640	rBV	243	190	0.02%	0.003%
9	3.411	641	644	647	rVV2	229	157	0.02%	0.002%
10	3.549	684	687	691	rBV2	239	210	0.02%	0.003%
11	3.620	706	709	712	rVB2	392	254	0.03%	0.003%
12	3.649	716	718	721	rBV	193	136	0.01%	0.002%
13	3.723	736	741	745	rBV3	271	244	0.03%	0.003%
14	3.810	766	768	770	rBV	188	113	0.01%	0.001%
15	3.822	770	772	775	rVV	425	269	0.03%	0.004%
16	3.858	779	783	787	rBV3	252	218	0.02%	0.003%
17	3.900	791	796	799	rBV2	298	314	0.03%	0.004%
18	3.986	820	823	826	rBV2	291	199	0.02%	0.003%
19	4.186	880	885	887	rBV2	364	434	0.05%	0.006%
20	4.244	897	903	907	rBV3	278	307	0.03%	0.004%
21	4.337	930	932	935	rBV2	241	196	0.02%	0.003%
22	4.398	947	951	955	rBV2	188	214	0.02%	0.003%
23	4.417	955	957	958	rBV	181	98	0.01%	0.001%
24	4.443	963	965	968	rVV2	255	162	0.02%	0.002%
25	4.488	973	979	982	rVB	306	244	0.03%	0.003%
26	4.620	1004	1020	1048	rBV	127662	309708	34.10%	4.098%
27	4.961	1123	1126	1129	rBV2	315	197	0.02%	0.003%
28	5.064	1140	1158	1186	rBV	175125	380482	41.89%	5.035%
29	5.192	1194	1198	1201	rBV2	425	312	0.03%	0.004%
30	5.424	1263	1270	1274	rBV2	363	314	0.03%	0.004%
31	5.469	1281	1284	1286	rBV	300	173	0.02%	0.002%
32	5.498	1289	1293	1295	rBV	191	164	0.02%	0.002%
33	5.562	1311	1313	1317	rVB	271	165	0.02%	0.002%
34	5.610	1324	1328	1331	rVB2	299	196	0.02%	0.003%
35	5.633	1331	1335	1337	rBV2	329	179	0.02%	0.002%
36	5.652	1337	1341	1342	rBV	207	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049316.D
 Acq On : 20 Jun 2022 19:20
 Operator : SY/MD
 Sample : N3396-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1401	rVV2	330684	908315	100.00%	12.019%
38	5.932	1426	1428	1431	rVB2	257	145	0.02%	0.002%
39	6.012	1450	1453	1455	rBV2	357	258	0.03%	0.003%
40	6.076	1470	1473	1476	rBV2	265	202	0.02%	0.003%
41	6.092	1476	1478	1481	rBV2	237	135	0.01%	0.002%
42	6.112	1481	1484	1486	rBV2	364	211	0.02%	0.003%
43	6.157	1495	1498	1504	rBV2	137	170	0.02%	0.002%
44	6.189	1504	1508	1511	rBV2	280	261	0.03%	0.003%
45	6.250	1513	1527	1552	rVV	309436	585929	64.51%	7.753%
46	6.411	1573	1577	1580	rBV2	327	359	0.04%	0.005%
47	6.526	1607	1613	1624	rVB7	1807	3234	0.36%	0.043%
48	6.597	1631	1635	1640	rBV	393	351	0.04%	0.005%
49	6.626	1640	1644	1645	rBV	243	198	0.02%	0.003%
50	6.690	1650	1664	1682	rBV	230303	445578	49.06%	5.896%
51	6.809	1697	1701	1706	rBV	668	461	0.05%	0.006%
52	7.044	1771	1774	1776	rVB	185	103	0.01%	0.001%
53	7.089	1784	1788	1791	rBV3	260	224	0.02%	0.003%
54	7.105	1791	1793	1795	rVV	274	146	0.02%	0.002%
55	7.128	1795	1800	1803	rVB2	304	294	0.03%	0.004%
56	7.182	1812	1817	1819	rBV3	907	881	0.10%	0.012%
57	7.224	1826	1830	1834	rBV2	519	426	0.05%	0.006%
58	7.327	1860	1862	1865	rBV2	367	254	0.03%	0.003%
59	7.359	1869	1872	1876	rVB	157	102	0.01%	0.001%
60	7.379	1876	1878	1880	rBV2	211	118	0.01%	0.002%
61	7.404	1884	1886	1887	rBV	256	132	0.01%	0.002%
62	7.491	1911	1913	1916	rVB2	240	91	0.01%	0.001%
63	7.517	1918	1921	1923	rBV	223	115	0.01%	0.002%
64	7.565	1924	1936	1957	rVV	122254	214808	23.65%	2.842%
65	7.793	2005	2007	2011	rBV3	314	230	0.03%	0.003%
66	7.896	2025	2039	2065	rBV	410947	709538	78.12%	9.389%
67	8.128	2105	2111	2114	rBV	265	302	0.03%	0.004%
68	8.179	2115	2127	2149	rVV	83914	143220	15.77%	1.895%
69	8.369	2184	2186	2188	rBV2	167	104	0.01%	0.001%
70	8.440	2206	2208	2211	rVB2	263	104	0.01%	0.001%
71	8.581	2250	2252	2255	rVB2	312	176	0.02%	0.002%
72	8.633	2255	2268	2300	rBV2	333727	659123	72.57%	8.721%
73	9.044	2393	2396	2399	rBV	229	207	0.02%	0.003%
74	9.134	2422	2424	2428	rVB2	292	127	0.01%	0.002%
75	9.227	2451	2453	2456	rVB2	219	117	0.01%	0.002%
76	9.298	2472	2475	2479	rBV3	240	238	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049316.D
 Acq On : 20 Jun 2022 19:20
 Operator : SY/MD
 Sample : N3396-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.417	2499	2512	2533	rBV	436425	737802	81.23%	9.763%
78	9.867	2650	2652	2654	rBV2	276	166	0.02%	0.002%
79	9.935	2670	2673	2679	rVB2	307	270	0.03%	0.004%
80	10.089	2719	2721	2725	rVB	217	104	0.01%	0.001%
81	10.112	2725	2728	2731	rVB2	318	212	0.02%	0.003%
82	10.192	2751	2753	2755	rBV	203	92	0.01%	0.001%
83	10.359	2804	2805	2808	rBV2	182	121	0.01%	0.002%
84	10.497	2844	2848	2851	rBV	218	211	0.02%	0.003%
85	10.710	2912	2914	2916	rBV2	362	198	0.02%	0.003%
86	10.755	2916	2928	2946	rVV	336566	546362	60.15%	7.229%
87	10.935	2982	2984	2985	rBV	229	100	0.01%	0.001%
88	11.070	3023	3026	3027	rBV	231	142	0.02%	0.002%
89	11.253	3080	3083	3084	rBV	251	163	0.02%	0.002%
90	11.317	3100	3103	3109	rVB2	361	325	0.04%	0.004%
91	11.394	3125	3127	3130	rBV	210	146	0.02%	0.002%
92	11.491	3154	3157	3158	rBV2	219	116	0.01%	0.002%
93	11.677	3213	3215	3217	rBV	228	114	0.01%	0.002%
94	11.706	3222	3224	3226	rBV2	328	197	0.02%	0.003%
95	11.755	3236	3239	3240	rBV2	244	162	0.02%	0.002%
96	11.812	3244	3257	3275	rVV	458649	731641	80.55%	9.681%
97	11.944	3296	3298	3301	rBV	517	293	0.03%	0.004%
98	12.192	3362	3375	3400	rBV	424275	691237	76.10%	9.146%
99	12.629	3508	3511	3513	rBV2	283	250	0.03%	0.003%
100	13.626	3819	3821	3823	rBV	235	125	0.01%	0.002%




Sum of corrected areas: 7557473

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049316.D
Acq On : 20 Jun 2022 19:20
Operator : SY/MD
Sample : N3396-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

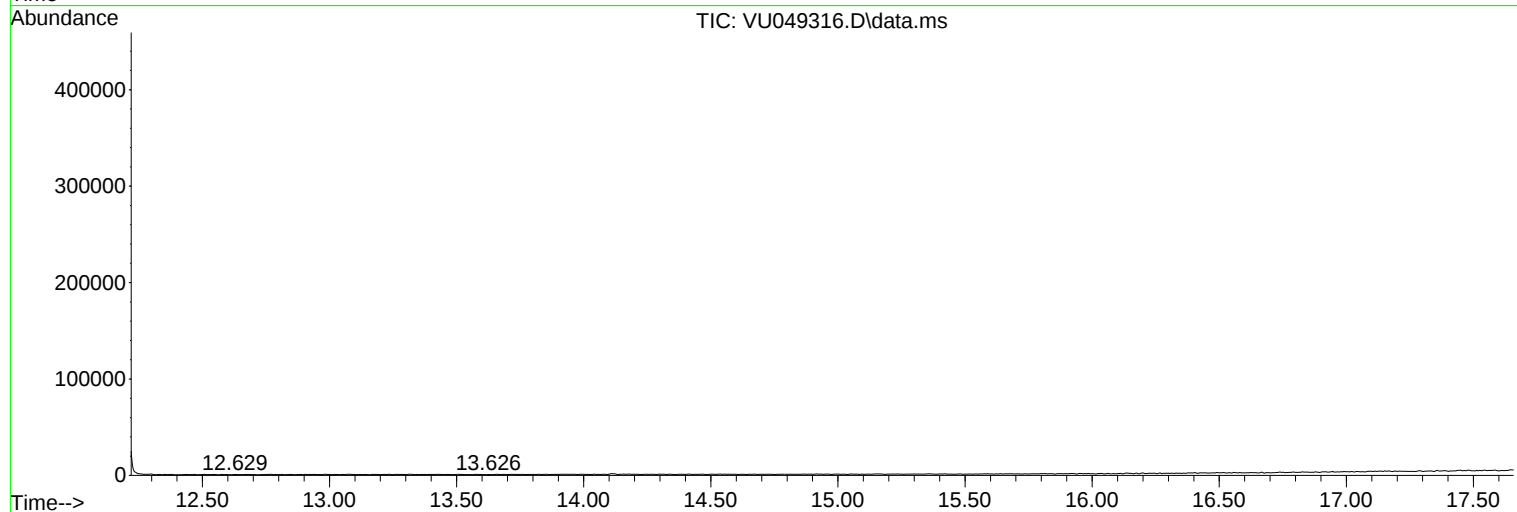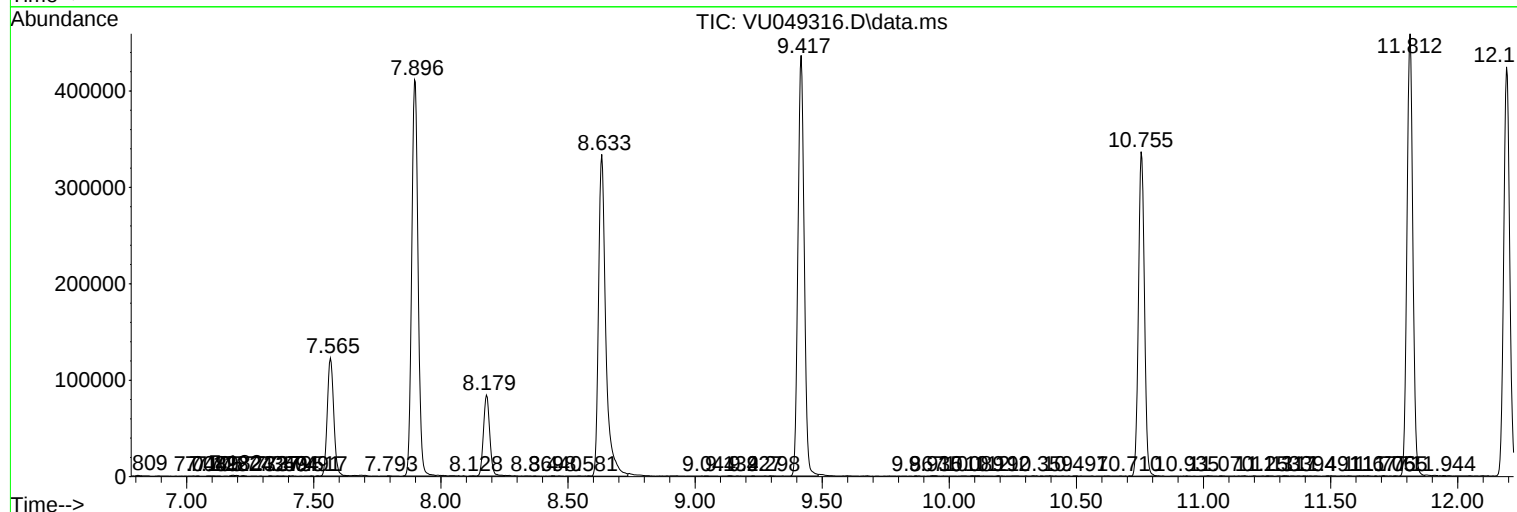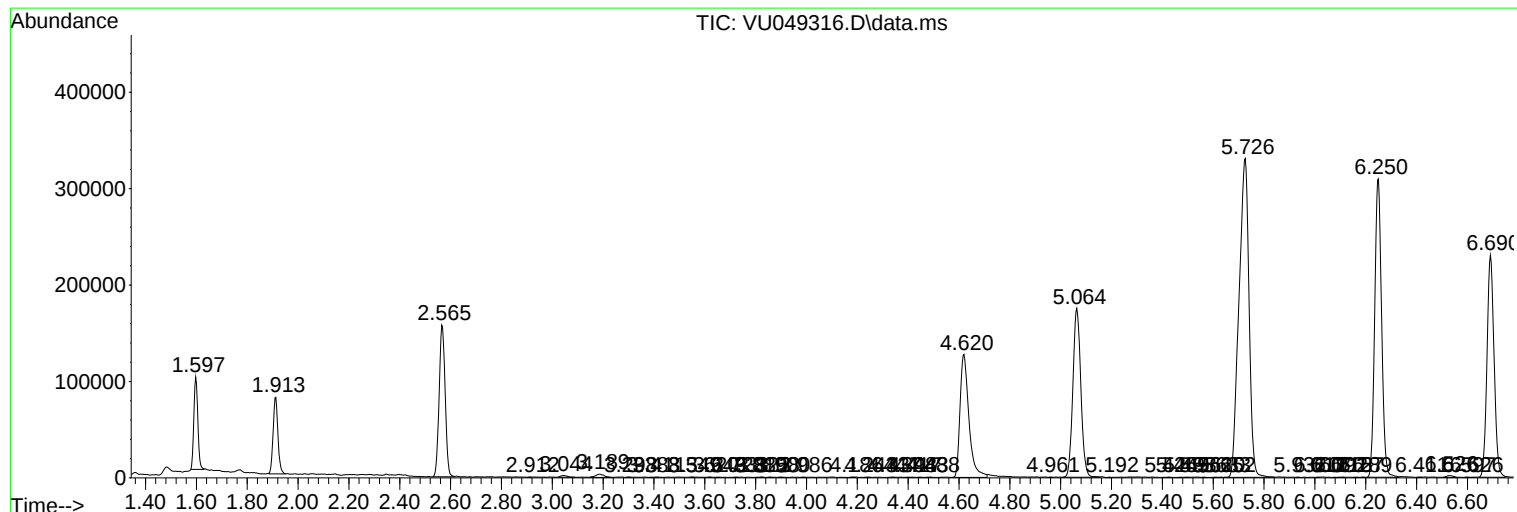

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049316.D
Acq On : 20 Jun 2022 19:20
Operator : SY/MD
Sample : N3396-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049316.D
Acq On : 20 Jun 2022 19:20
Operator : SY/MD
Sample : N3396-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------