

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049317.D
 Acq On : 20 Jun 2022 19:44
 Operator : SY/MD
 Sample : N3395-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

Signal : TIC: VU049317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	92	rBV	95885	103311	11.53%	1.388%
2	1.909	170	177	192	rVB	77965	101819	11.36%	1.368%
3	2.565	370	381	397	rVB	156805	252185	28.14%	3.389%
4	3.025	522	524	525	rBV2	371	142	0.02%	0.002%
5	3.137	556	559	561	rBV2	368	250	0.03%	0.003%
6	3.227	585	587	590	rBV	235	142	0.02%	0.002%
7	3.559	688	690	692	rBV2	209	138	0.02%	0.002%
8	3.610	702	706	711	rVB2	301	249	0.03%	0.003%
9	3.649	715	718	722	rBV3	275	208	0.02%	0.003%
10	3.774	754	757	760	rBV3	391	248	0.03%	0.003%
11	3.790	760	762	764	rBV	213	109	0.01%	0.001%
12	3.919	797	802	804	rVV3	348	295	0.03%	0.004%
13	3.951	809	812	813	rBV2	220	125	0.01%	0.002%
14	4.044	839	841	844	rVB2	229	135	0.02%	0.002%
15	4.067	844	848	850	rBV2	303	232	0.03%	0.003%
16	4.099	855	858	859	rBV	329	174	0.02%	0.002%
17	4.153	870	875	878	rVB2	300	180	0.02%	0.002%
18	4.182	878	884	885	rBV2	316	273	0.03%	0.004%
19	4.237	898	901	903	rBV2	185	108	0.01%	0.001%
20	4.266	907	910	915	rVB3	260	203	0.02%	0.003%
21	4.375	939	944	946	rBV2	240	238	0.03%	0.003%
22	4.411	952	955	958	rBV2	172	144	0.02%	0.002%
23	4.485	976	978	981	rBV2	172	110	0.01%	0.001%
24	4.549	995	998	1000	rBV2	250	128	0.01%	0.002%
25	4.623	1007	1021	1058	rBV	123959	312783	34.90%	4.204%
26	5.063	1140	1158	1176	rBV	167108	368034	41.06%	4.946%
27	5.240	1211	1213	1216	rVB2	318	161	0.02%	0.002%
28	5.256	1216	1218	1223	rVB2	290	176	0.02%	0.002%
29	5.292	1224	1229	1236	rBV4	444	520	0.06%	0.007%
30	5.369	1250	1253	1254	rBV	358	202	0.02%	0.003%
31	5.404	1259	1264	1268	rBV3	278	370	0.04%	0.005%
32	5.542	1304	1307	1311	rBV2	276	202	0.02%	0.003%
33	5.562	1311	1313	1316	rVB	192	119	0.01%	0.002%
34	5.584	1316	1320	1323	rBV3	225	190	0.02%	0.003%
35	5.603	1323	1326	1329	rVB3	267	186	0.02%	0.002%
36	5.623	1329	1332	1333	rBV	181	112	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049317.D
 Acq On : 20 Jun 2022 19:44
 Operator : SY/MD
 Sample : N3395-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1390	rBV2	327370	896325	100.00%	12.046%
38	5.861	1403	1406	1408	rBV2	383	247	0.03%	0.003%
39	5.964	1434	1438	1440	rBV3	325	260	0.03%	0.003%
40	6.112	1482	1484	1487	rBV2	292	183	0.02%	0.002%
41	6.153	1495	1497	1499	rVB	262	110	0.01%	0.001%
42	6.179	1503	1505	1509	rVB2	237	150	0.02%	0.002%
43	6.250	1513	1527	1545	rBV	300760	573492	63.98%	7.707%
44	6.436	1583	1585	1588	rBV2	259	161	0.02%	0.002%
45	6.504	1602	1606	1607	rVV2	344	211	0.02%	0.003%
46	6.533	1607	1615	1624	rVB4	1959	3588	0.40%	0.048%
47	6.568	1624	1626	1630	rVB	254	149	0.02%	0.002%
48	6.597	1630	1635	1640	rBV2	287	334	0.04%	0.004%
49	6.636	1640	1647	1650	rBV2	172	192	0.02%	0.003%
50	6.690	1650	1664	1691	rBV	225197	437831	48.85%	5.884%
51	6.784	1691	1693	1694	rBV	311	133	0.01%	0.002%
52	6.809	1696	1701	1710	rVB5	822	1240	0.14%	0.017%
53	6.845	1710	1712	1717	rBV2	280	253	0.03%	0.003%
54	6.951	1740	1745	1749	rVB3	190	192	0.02%	0.003%
55	7.012	1760	1764	1770	rBV3	338	343	0.04%	0.005%
56	7.054	1770	1777	1784	rVB3	389	653	0.07%	0.009%
57	7.105	1790	1793	1794	rBV	290	174	0.02%	0.002%
58	7.185	1812	1818	1830	rVB3	1305	1768	0.20%	0.024%
59	7.256	1837	1840	1843	rBV	252	152	0.02%	0.002%
60	7.282	1843	1848	1851	rBV2	320	333	0.04%	0.004%
61	7.353	1864	1870	1872	rBV3	290	295	0.03%	0.004%
62	7.414	1885	1889	1890	rBV	270	187	0.02%	0.003%
63	7.449	1897	1900	1904	rBV3	261	250	0.03%	0.003%
64	7.565	1922	1936	1956	rBV	123007	215017	23.99%	2.890%
65	7.684	1971	1973	1976	rBV2	561	320	0.04%	0.004%
66	7.812	2010	2013	2018	rBV	309	200	0.02%	0.003%
67	7.841	2019	2022	2025	rVB	288	183	0.02%	0.002%
68	7.896	2025	2039	2063	rBV	396848	693436	77.36%	9.319%
69	8.092	2096	2100	2102	rBV2	333	306	0.03%	0.004%
70	8.179	2114	2127	2149	rBV	85022	143731	16.04%	1.932%
71	8.382	2188	2190	2194	rVB2	305	191	0.02%	0.003%
72	8.439	2205	2208	2211	rBV2	249	172	0.02%	0.002%
73	8.632	2256	2268	2301	rBV2	341492	665502	74.25%	8.944%
74	8.912	2352	2355	2359	rVB2	320	213	0.02%	0.003%
75	9.089	2406	2410	2415	rVB2	352	334	0.04%	0.004%
76	9.121	2418	2420	2423	rBV3	207	156	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049317.D
 Acq On : 20 Jun 2022 19:44
 Operator : SY/MD
 Sample : N3395-23
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis

77	9.250	2457	2460	2462	rBV2	250	169	0.02%	0.002%
78	9.279	2466	2469	2473	rBV2	307	278	0.03%	0.004%
79	9.320	2479	2482	2485	rBV2	241	174	0.02%	0.002%
80	9.372	2495	2498	2500	rBV	217	149	0.02%	0.002%
81	9.417	2500	2512	2537	rVV	429190	715719	79.85%	9.619%
82	9.626	2575	2577	2579	rBV2	210	115	0.01%	0.002%
83	9.816	2634	2636	2641	rVB2	334	234	0.03%	0.003%
84	9.886	2654	2658	2662	rBV3	314	323	0.04%	0.004%
85	9.934	2670	2673	2676	rBV3	199	158	0.02%	0.002%
86	9.986	2686	2689	2692	rBV2	282	181	0.02%	0.002%
87	10.021	2692	2700	2702	rBV2	323	336	0.04%	0.005%
88	10.616	2882	2885	2887	rBV	272	161	0.02%	0.002%
89	10.754	2916	2928	2951	rBV	331787	538935	60.13%	7.243%
90	10.918	2975	2979	2982	rBV2	264	220	0.02%	0.003%
91	11.041	3014	3017	3025	rBV3	234	320	0.04%	0.004%
92	11.253	3077	3083	3085	rBV	408	382	0.04%	0.005%
93	11.481	3151	3154	3157	rVV2	308	202	0.02%	0.003%
94	11.520	3162	3166	3171	rBV3	378	439	0.05%	0.006%
95	11.700	3219	3222	3225	rBV	184	153	0.02%	0.002%
96	11.812	3244	3257	3273	rBV	451713	718656	80.18%	9.658%
97	11.986	3309	3311	3314	rVB2	348	196	0.02%	0.003%
98	12.047	3325	3330	3332	rBV2	268	310	0.03%	0.004%
99	12.192	3363	3375	3397	rBV	421573	678963	75.75%	9.125%
100	13.320	3719	3726	3735	rBV3	482	984	0.11%	0.013%




Sum of corrected areas: 7440925

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049317.D
Acq On : 20 Jun 2022 19:44
Operator : SY/MD
Sample : N3395-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

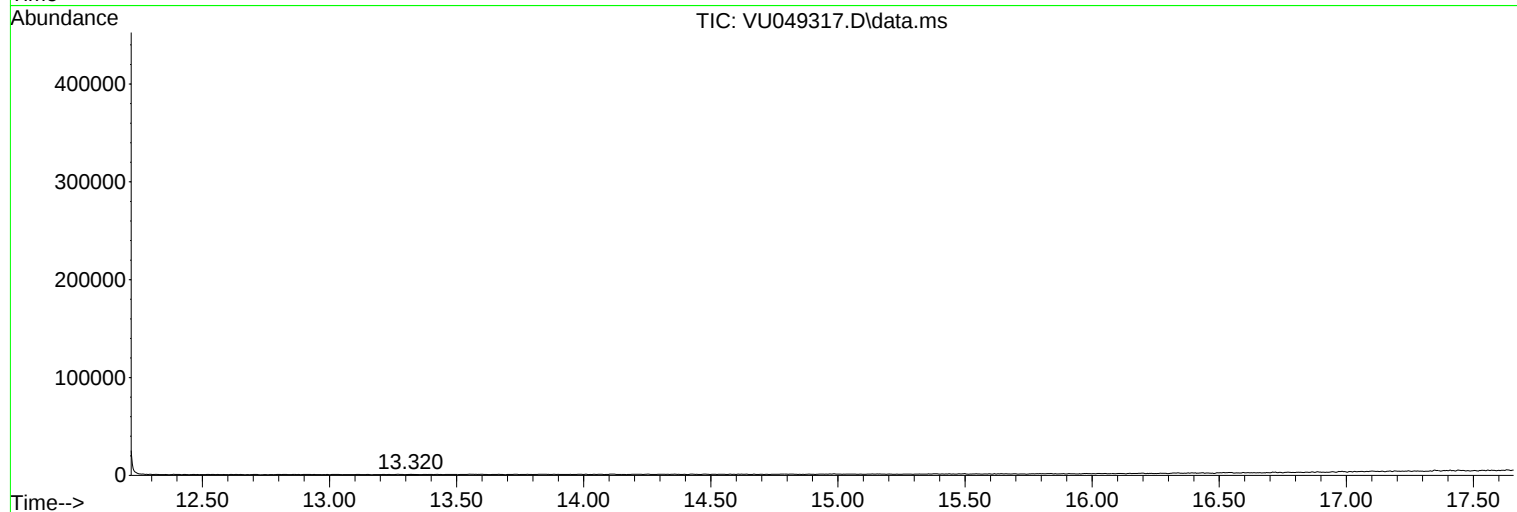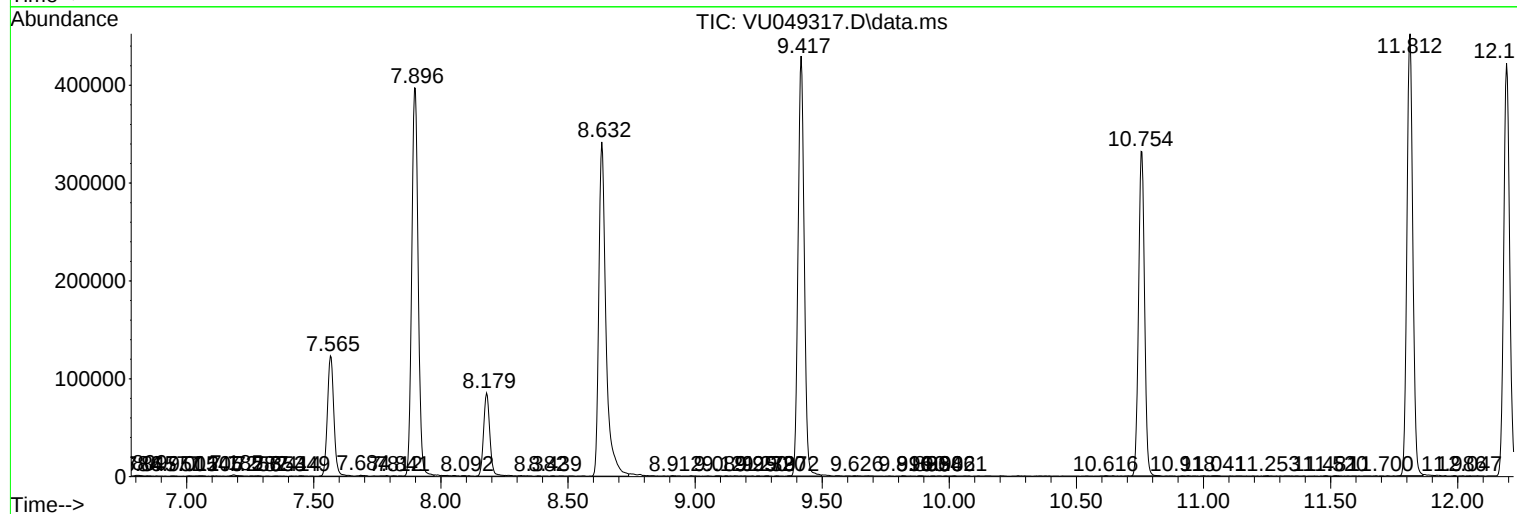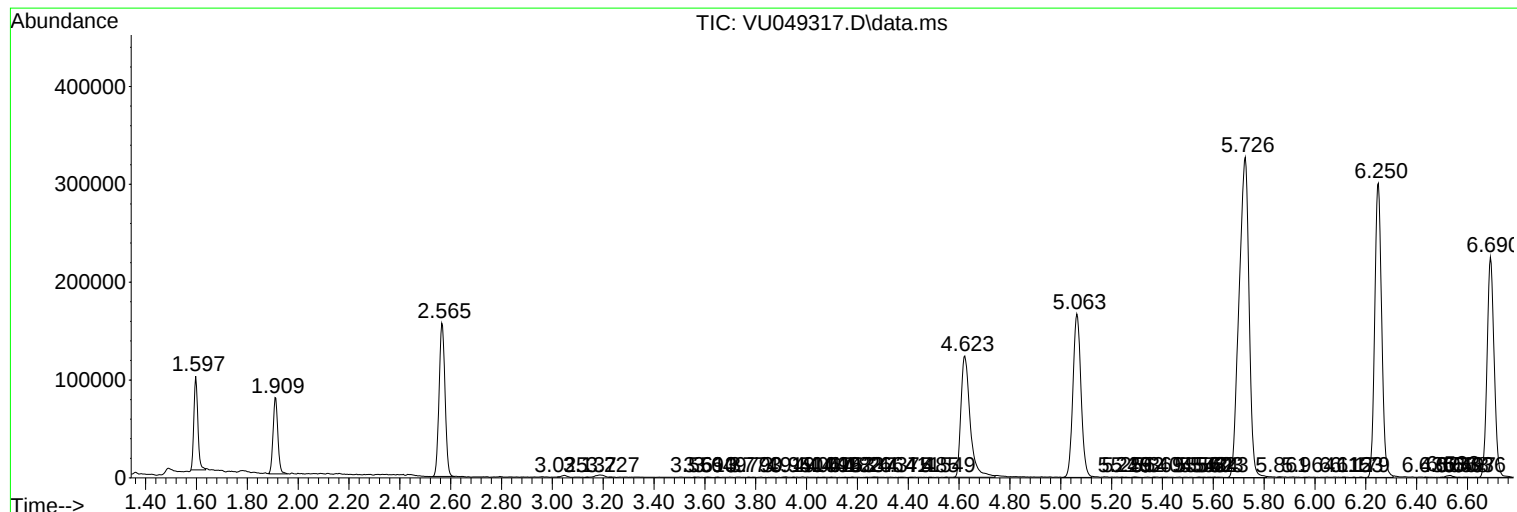

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049317.D
Acq On : 20 Jun 2022 19:44
Operator : SY/MD
Sample : N3395-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
Data File : VU049317.D
Acq On : 20 Jun 2022 19:44
Operator : SY/MD
Sample : N3395-23
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------