


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062022\
 Data File : VU049294.D
 Acq On : 20 Jun 2022 09:40
 Operator : SY/MD
 Sample : BFB098
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB098

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM061022WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 21 01:08:31 2022

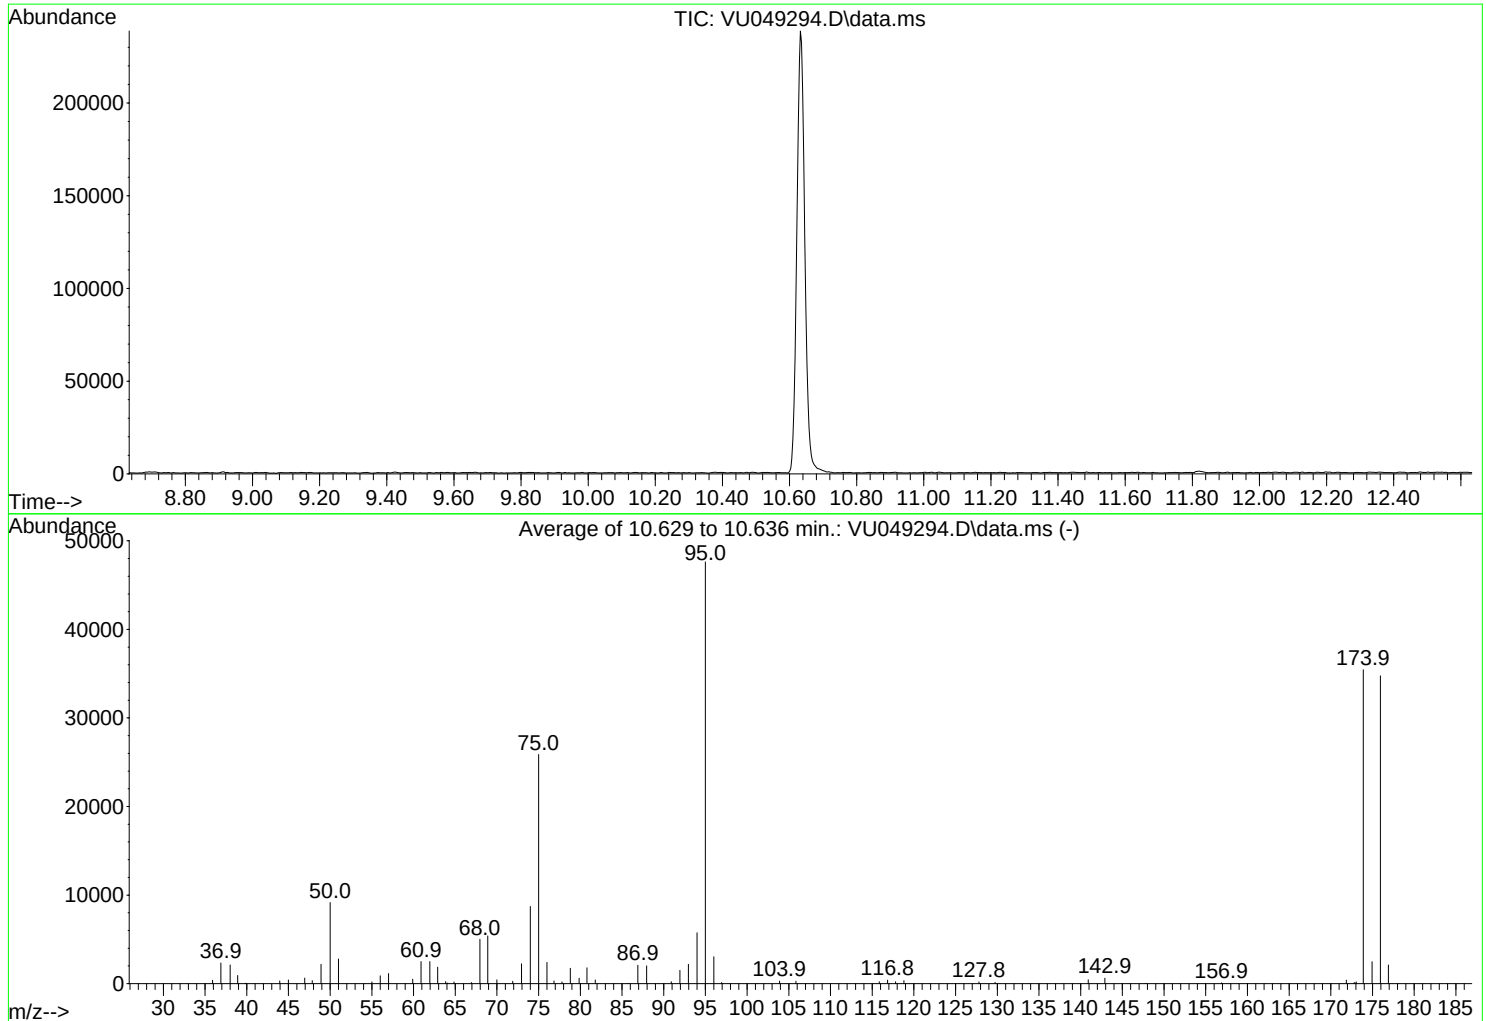

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	9159	PASS
75	95	30	80	54.3	25864	PASS
95	95	100	100	100.0	47627	PASS
96	95	5	9	6.4	3045	PASS
173	174	0.00	2	0.6	207	PASS
174	95	50	120	74.4	35453	PASS
175	174	5	9	7.0	2469	PASS
176	174	95	101	98.1	34768	PASS
177	176	5	9	6.1	2109	PASS

m/z	Abundance
39.90	182.0
43.90	393.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	371.0
36.90	2357.0
38.00	2020.0
38.90	936.0
39.80	257.0
44.00	616.0
45.00	395.0
46.90	624.0
47.80	401.0
48.90	2113.0
50.00	9188.0
51.00	2750.0
55.00	178.0
56.00	855.0
57.00	1089.0
59.90	470.0
60.90	2441.0
62.00	2418.0
62.90	1792.0
63.90	264.0
64.80	209.0
66.90	112.0
68.00	5053.0
68.90	5287.0
70.00	400.0
71.90	257.0
72.90	2271.0
74.00	8380.0
75.00	25416.0
76.00	2383.0
76.90	315.0
77.80	165.0
78.80	1685.0
79.80	545.0
80.80	1742.0
81.80	391.0
86.90	2068.0
87.90	1883.0
90.90	217.0
91.90	1434.0
93.00	2118.0
94.00	5507.0
95.00	46016.0
96.00	2784.0
97.00	109.0
103.90	304.0
105.80	237.0
115.90	195.0
116.80	330.0
117.80	236.0
118.80	313.0
127.80	181.0
129.70	154.0
140.90	401.0
142.90	572.0
147.80	103.0
171.80	393.0
173.10	307.0
173.90	33256.0
174.90	2286.0
175.90	32752.0
176.90	2019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	392.0
36.90	2400.0
38.00	2186.0
38.90	956.0
39.90	243.0
44.00	700.0
45.00	450.0
46.90	646.0
47.80	358.0
48.90	2290.0
50.00	9432.0
51.00	2871.0
55.00	206.0
56.00	975.0
57.00	1178.0
59.90	534.0
60.90	2542.0
61.90	2563.0
62.90	1902.0
63.80	248.0
64.90	219.0
67.00	128.0
68.00	5160.0
68.90	5574.0
70.00	462.0
71.90	274.0
73.00	2325.0
74.00	9026.0
75.00	26672.0
76.00	2511.0
76.90	300.0
77.80	207.0
78.80	1781.0
79.80	646.0
80.80	1857.0
81.80	429.0
86.90	2092.0
87.90	2018.0
90.90	222.0
92.00	1547.0
92.90	2227.0
94.00	5976.0
95.00	49232.0
96.00	3099.0
97.00	134.0
103.90	318.0
105.80	287.0
115.90	227.0
116.90	404.0
117.80	200.0
118.80	362.0
127.80	199.0
129.80	148.0
140.90	443.0
142.90	626.0
156.90	135.0
171.80	399.0
172.80	314.0
173.00	313.0
173.90	36576.0
174.90	2532.0
176.00	35936.0
176.90	2184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098

m/z	Abundance
35.90	370.0
36.90	2257.0
38.00	2112.0
38.90	883.0
39.90	234.0
44.00	769.0
45.00	401.0
47.00	606.0
47.90	297.0
48.90	2143.0
50.00	8857.0
51.00	2745.0
55.00	192.0
56.00	851.0
57.00	1170.0
59.90	506.0
60.90	2476.0
61.90	2500.0
62.90	1867.0
63.80	209.0
64.10	208.0
64.90	199.0
67.00	122.0
67.90	4796.0
68.90	5282.0
70.00	451.0
71.90	263.0
73.00	2126.0
74.00	8695.0
75.00	25504.0
76.00	2297.0
76.80	293.0
77.80	231.0
78.80	1716.0
79.90	630.0
80.80	1767.0
81.80	420.0
85.70	108.0
86.90	2068.0
88.00	2142.0
90.90	238.0
91.90	1534.0
92.90	2204.0
94.00	5771.0
95.00	47632.0
96.00	3252.0
96.90	127.0
103.90	266.0
105.90	278.0
115.80	253.0
116.90	453.0
117.80	198.0
118.80	374.0
127.80	204.0
129.80	151.0
140.90	470.0
142.90	641.0
156.90	124.0
171.90	401.0
172.90	344.0
173.90	36528.0
175.00	2588.0
176.00	35616.0
176.90	2124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB098