

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062023\
 Data File : VU054628.D
 Acq On : 20 Jun 2023 22:25
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK164

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	89	96	110	rVB	167855	193528	18.04%	1.928%
2	1.914	186	194	208	rBV	127275	171670	16.00%	1.711%
3	2.567	385	397	413	rVB	238709	390279	36.38%	3.889%
4	3.043	529	545	566	rBV	166733	329161	30.68%	3.280%
5	3.181	573	588	602	rBV	20700	45402	4.23%	0.452%
6	4.631	1020	1039	1075	rBV2	161694	530118	49.42%	5.282%
7	5.059	1156	1172	1199	rVB	192410	439844	41.00%	4.383%
8	5.721	1356	1378	1410	rBV2	398482	1048292	97.72%	10.445%
9	6.245	1527	1541	1569	rBV	423842	829834	77.36%	8.269%
10	6.686	1664	1678	1698	rBV	250630	498078	46.43%	4.963%
11	7.563	1934	1951	1974	rBV	119541	226003	21.07%	2.252%
12	7.792	2010	2022	2036	rBV2	16054	31574	2.94%	0.315%
13	7.895	2041	2054	2070	rBV	473956	829485	77.32%	8.265%
14	8.177	2129	2142	2159	rBV2	73604	133755	12.47%	1.333%
15	8.631	2271	2283	2325	rBV2	510797	1072760	100.00%	10.689%
16	9.412	2513	2526	2550	rBV	589623	1002474	93.45%	9.989%
17	9.570	2568	2575	2586	rVB4	7416	12176	1.14%	0.121%
18	9.695	2605	2614	2624	rVB4	7634	13674	1.27%	0.136%
19	10.110	2732	2743	2756	rVB5	8795	20496	1.91%	0.204%
20	10.480	2850	2858	2871	rVB3	8067	13271	1.24%	0.132%
21	10.750	2931	2942	2960	rBV	165380	273599	25.50%	2.726%
22	11.084	3040	3046	3058	rVB5	9047	13326	1.24%	0.133%
23	11.467	3156	3165	3173	rBV3	12379	18831	1.76%	0.188%
24	11.743	3242	3251	3259	rBV4	12290	19386	1.81%	0.193%
25	11.808	3259	3271	3292	rVB	580820	945509	88.14%	9.421%
26	12.187	3377	3389	3410	rBV	415571	702794	65.51%	7.003%
27	12.888	3597	3607	3615	rBV8	9380	17355	1.62%	0.173%
28	13.216	3699	3709	3720	rBV4	20764	35297	3.29%	0.352%
29	13.836	3893	3902	3914	rBV	32742	51068	4.76%	0.509%
30	14.084	3968	3979	3989	rBV	26854	46669	4.35%	0.465%
31	14.325	4044	4054	4063	rBV2	31089	51052	4.76%	0.509%
32	16.338	4672	4680	4689	rBV3	19731	29136	2.72%	0.290%




Sum of corrected areas: 10035896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062023\
Data File : VU054628.D
Acq On : 20 Jun 2023 22:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK164

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

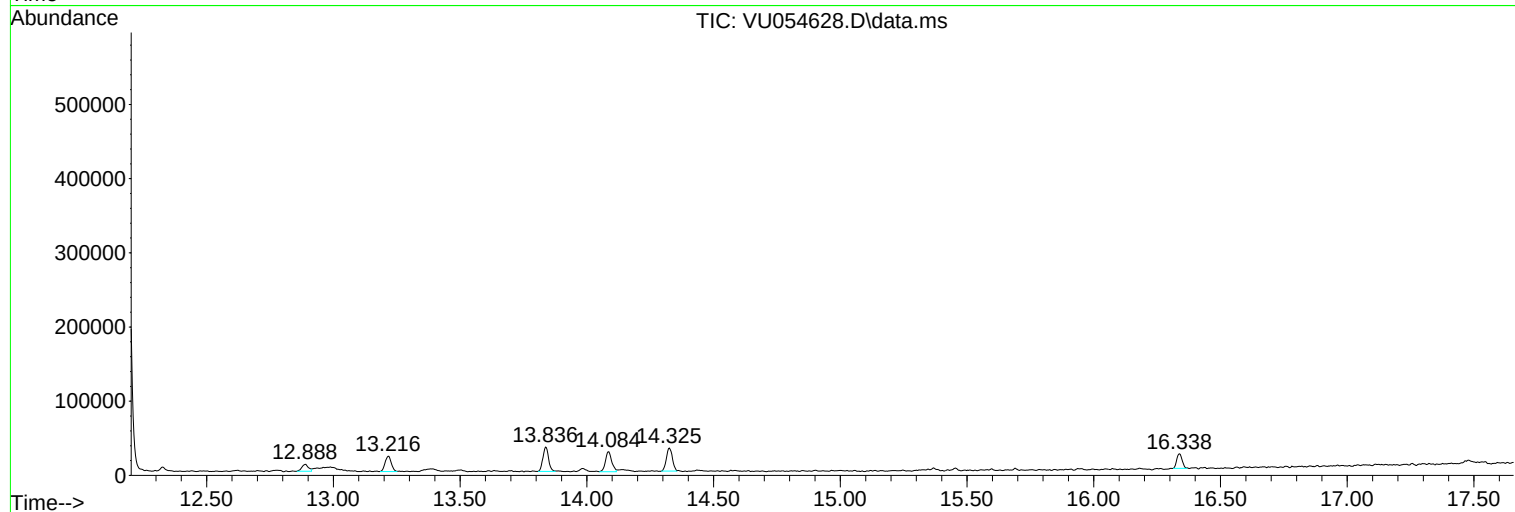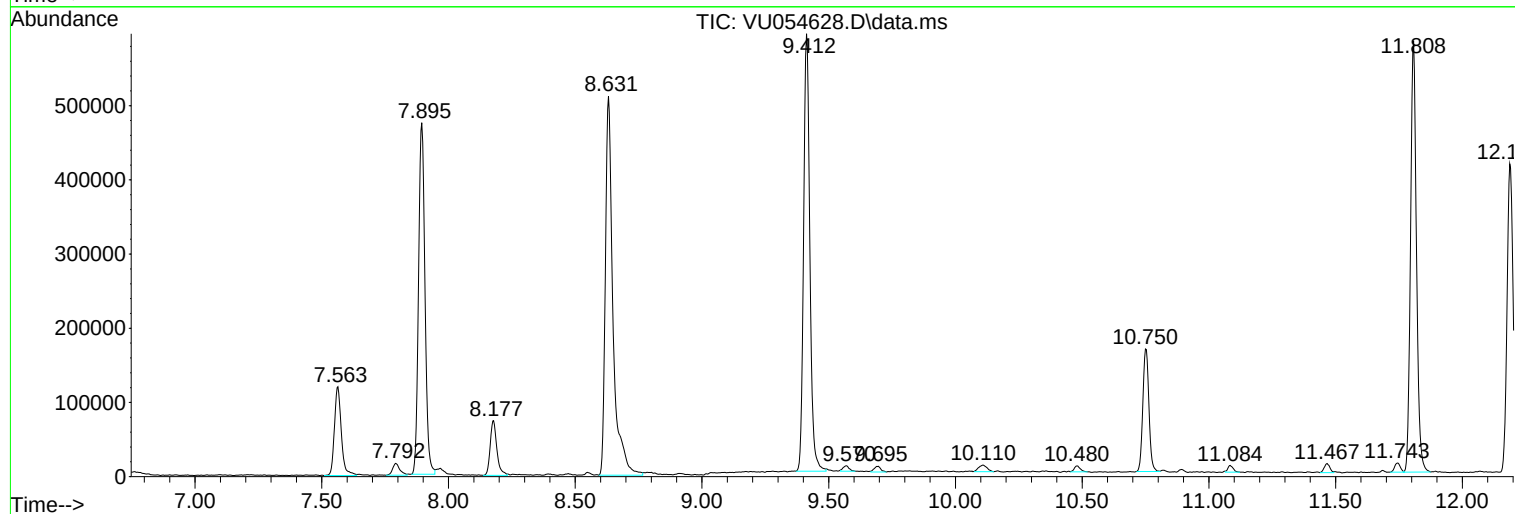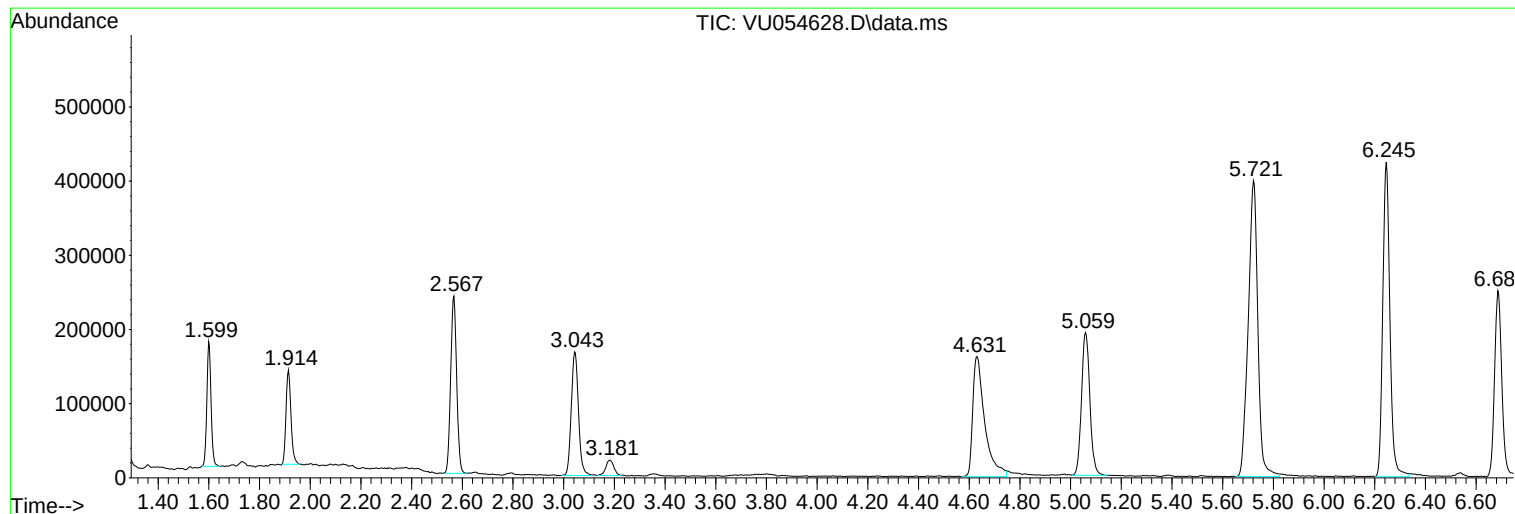

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062023\
Data File : VU054628.D
Acq On : 20 Jun 2023 22:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK164

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062023\
Data File : VU054628.D
Acq On : 20 Jun 2023 22:25
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK164

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------