


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062023\
Data File : VU054611.D
Acq On : 20 Jun 2023 13:06
Operator : MD/SY
Sample : BFB022
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB022

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 22 02:42:14 2023

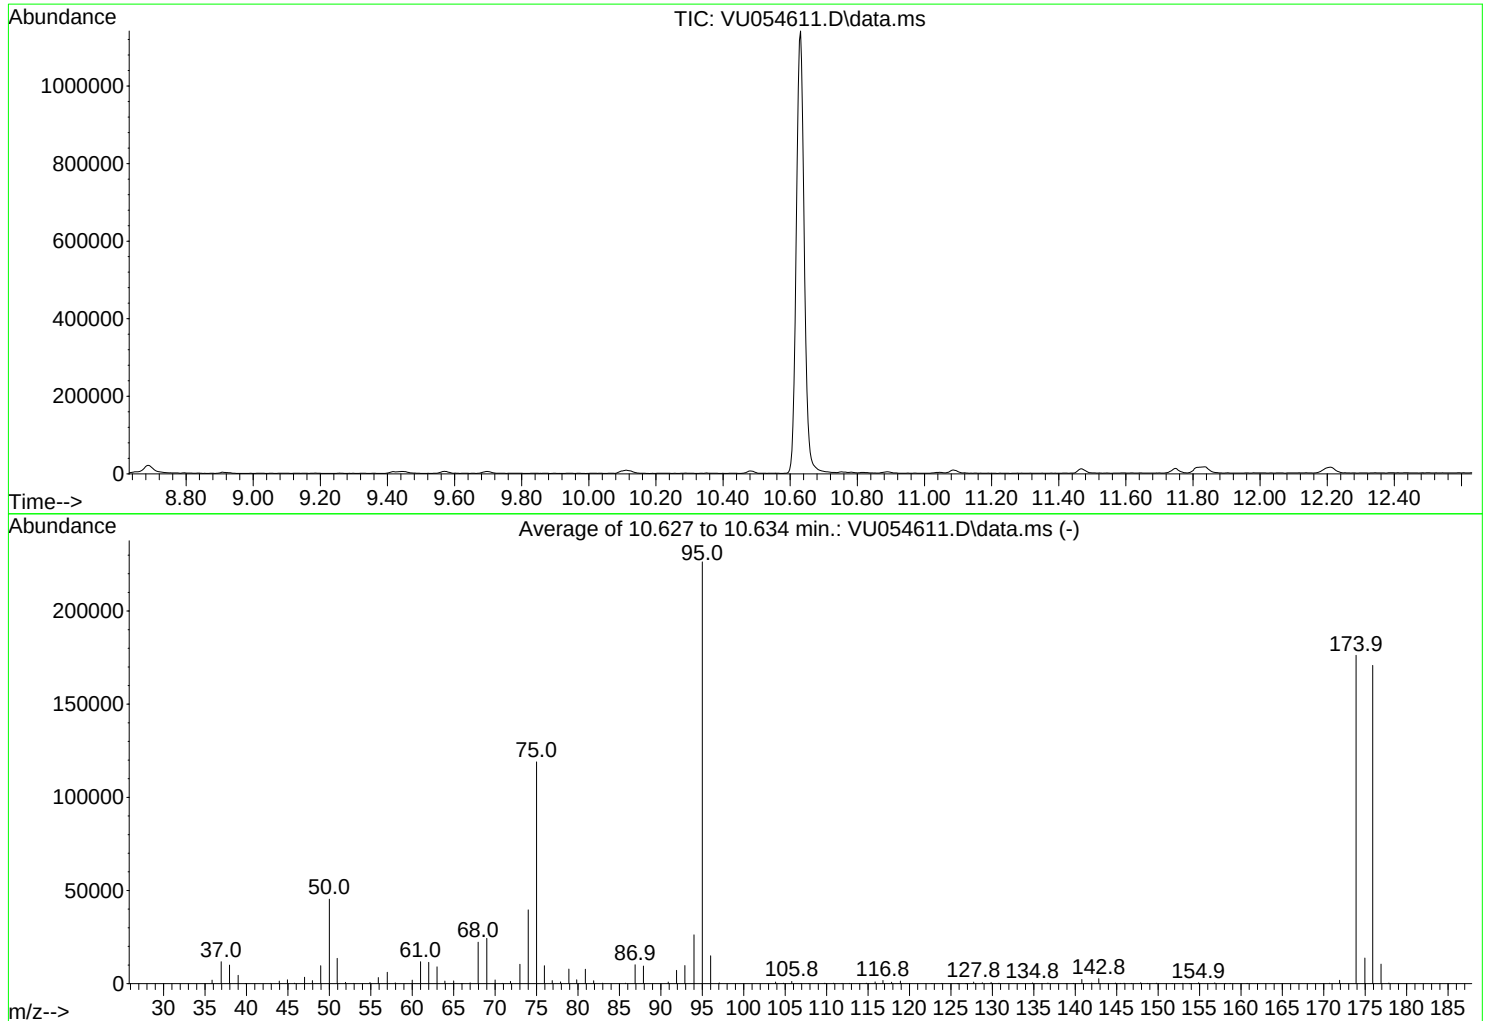

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	45328	PASS
75	95	30	80	52.6	119053	PASS
95	95	100	100	100.0	226411	PASS
96	95	5	9	6.6	14980	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.8	176213	PASS
175	174	5	9	7.8	13751	PASS
176	174	95	101	96.9	170795	PASS
177	176	5	9	6.2	10526	PASS

m/z	Abundance
35.90	226.0
39.90	305.0
42.90	143.0
44.00	1105.0
73.00	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	2096.0
37.00	12423.0
38.00	10356.0
39.00	4452.0
39.90	405.0
43.00	332.0
44.00	2500.0
44.90	2172.0
45.80	279.0
47.00	3521.0
47.90	1689.0
49.00	9714.0
50.00	46896.0
50.90	13965.0
51.90	721.0
53.00	153.0
54.90	622.0
55.90	3499.0
57.00	6277.0
58.00	574.0
60.00	1931.0
61.00	11863.0
62.00	11509.0
63.00	9410.0
64.00	1232.0
65.00	1321.0
65.90	127.0
67.90	22240.0
69.00	24280.0
70.00	2223.0
70.90	226.0
71.80	1197.0
73.00	11200.0
74.00	41032.0
75.00	120608.0
76.00	9962.0
76.90	1598.0
78.00	915.0
78.90	8218.0
79.90	1965.0
80.90	7716.0
81.90	1584.0
83.00	267.0
85.70	271.0
86.90	10273.0
87.90	10207.0
90.90	964.0
91.90	7125.0
92.90	9775.0
94.00	26064.0
95.00	231872.0
96.00	15377.0
97.10	419.0
103.80	927.0
104.80	287.0
105.80	1180.0
106.90	164.0
107.80	133.0
109.80	242.0
110.90	290.0
111.80	197.0
112.80	149.0
114.70	309.0
115.90	973.0
116.80	1699.0
117.80	849.0
118.90	1403.0
122.70	154.0
123.90	138.0
125.80	100.0
127.70	761.0
128.80	528.0
129.90	705.0
130.80	258.0
134.90	429.0
136.00	158.0
136.70	360.0
139.80	197.0
140.80	1973.0
142.00	323.0
142.90	2617.0
144.10	131.0
144.90	404.0
145.90	334.0
146.80	123.0
147.90	497.0
148.80	140.0
149.80	252.0
152.90	166.0
153.80	103.0
154.90	514.0
156.80	414.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

158.20	130.0
158.70	232.0
160.80	223.0
170.70	358.0
171.90	1793.0
173.90	173888.0
175.00	13575.0
175.90	167744.0
176.90	10614.0
177.90	340.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	2211.0
36.90	12090.0
37.90	10239.0
39.00	4570.0
39.90	332.0
42.90	384.0
43.90	2575.0
45.00	2093.0
45.80	250.0
47.00	3605.0
47.90	1654.0
49.00	9920.0
50.00	46624.0
50.90	14031.0
51.90	705.0
53.00	128.0
54.90	610.0
55.90	3309.0
57.00	6363.0
57.90	467.0
60.00	1924.0
61.00	12157.0
62.00	11747.0
63.00	9288.0
64.00	1396.0
65.00	1518.0
66.10	128.0
67.00	662.0
67.90	22920.0
69.00	25032.0
70.00	2089.0
70.90	208.0
71.90	1230.0
73.00	10947.0
74.00	40624.0
75.00	122416.0
76.00	9929.0
76.90	1622.0
77.90	967.0
78.90	7997.0
79.80	2109.0
80.90	8024.0
81.90	1575.0
83.00	257.0
85.80	297.0
86.90	10487.0
87.90	9554.0
90.90	857.0
91.90	7403.0
92.90	9898.0
94.00	26952.0
95.00	233728.0
96.00	15397.0
97.10	453.0
103.90	892.0
104.80	292.0
105.80	1312.0
106.90	163.0
107.90	145.0
109.80	312.0
110.80	251.0
111.80	171.0
112.70	142.0
114.80	283.0
115.90	938.0
116.80	1682.0
117.80	821.0
118.90	1449.0
122.70	122.0
123.90	189.0
127.80	916.0
128.80	521.0
129.90	660.0
130.80	260.0
134.90	433.0
136.00	140.0
136.70	327.0
139.80	243.0
140.80	2281.0
142.00	321.0
142.90	2756.0
144.00	124.0
144.90	314.0
145.40	271.0
145.90	307.0
146.80	151.0
147.90	596.0
148.70	145.0
149.90	259.0
151.70	106.0
152.90	167.0
154.90	485.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

156.90	451.0
158.20	135.0
158.70	193.0
160.70	223.0
170.70	307.0
171.90	1919.0
173.90	182208.0
174.90	14190.0
175.90	175872.0
176.90	10967.0
177.90	378.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

m/z	Abundance
35.90	2066.0
36.90	10708.0
37.90	9352.0
39.00	4442.0
39.90	340.0
42.90	365.0
43.90	2310.0
44.90	1884.0
45.80	266.0
47.00	3074.0
48.00	1499.0
48.90	9335.0
50.00	42464.0
51.00	12654.0
52.00	645.0
52.80	149.0
54.90	589.0
55.90	3055.0
57.00	5758.0
57.90	339.0
60.00	1804.0
61.00	11187.0
62.00	11045.0
63.00	8310.0
63.90	1390.0
65.00	1527.0
66.10	135.0
67.00	648.0
68.00	21512.0
69.00	23624.0
70.00	1755.0
70.80	165.0
71.90	1220.0
73.00	9479.0
74.00	37256.0
75.00	114136.0
75.90	9000.0
76.90	1594.0
77.80	1001.0
78.90	7188.0
79.80	2080.0
80.90	7568.0
81.90	1379.0
82.90	234.0
85.80	332.0
86.90	9753.0
87.90	8475.0
90.90	761.0
91.90	6825.0
92.90	9569.0
94.00	25624.0
95.00	213632.0
96.00	14165.0
97.00	376.0
103.90	889.0
104.80	279.0
105.80	1270.0
106.90	164.0
107.90	109.0
109.80	248.0
110.80	208.0
111.90	144.0
112.70	155.0
114.90	264.0
115.80	832.0
116.80	1716.0
117.90	753.0
118.90	1294.0
123.90	182.0
126.80	123.0
127.80	985.0
128.80	463.0
129.80	624.0
130.80	281.0
134.80	417.0
136.70	321.0
138.90	103.0
139.80	215.0
140.80	2362.0
142.00	331.0
142.80	2686.0
143.90	130.0
144.70	310.0
145.50	270.0
145.90	245.0
146.80	177.0
147.90	533.0
148.70	132.0
149.70	173.0
151.70	105.0
153.00	141.0
154.90	463.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022

156.90	423.0
158.10	121.0
158.70	219.0
160.70	206.0
170.60	187.0
171.90	1779.0
173.90	172544.0
174.90	13487.0
175.90	168768.0
176.90	9996.0
177.80	370.0

Instrument :
MSVOA_U
ClientSampleId :
BFB022