


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062118\
 Data File : VU024799.D
 Acq On : 21 Jun 2018 09:51
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260
 Last Update : Wed Jun 13 13:55:26 2018

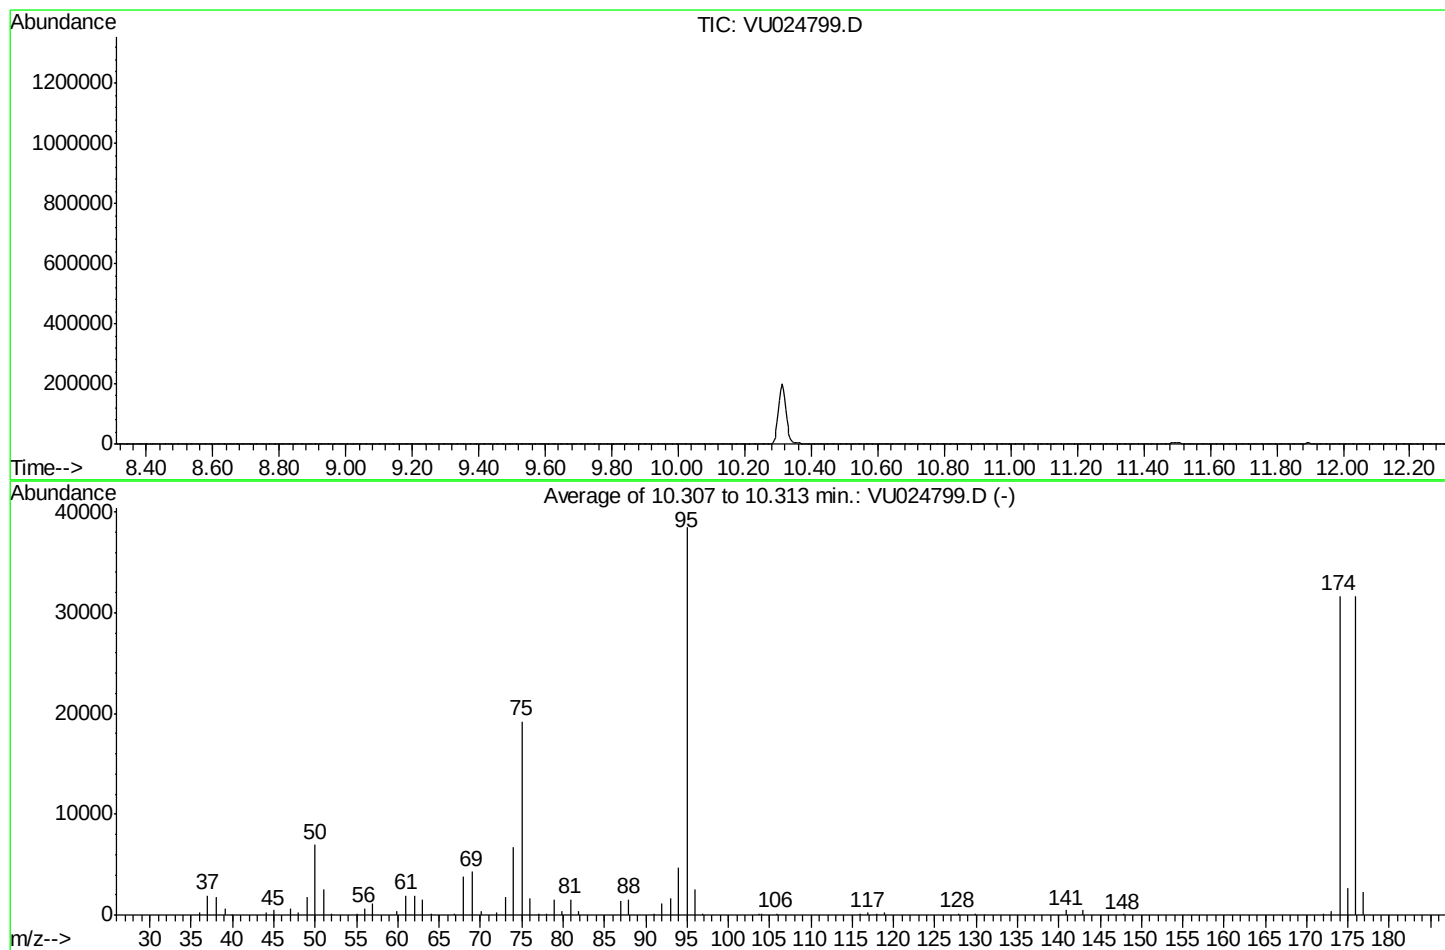

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	6960	PASS
75	95	30	60	50.0	19216	PASS
95	95	100	100	100.0	38461	PASS
96	95	5	9	6.7	2567	PASS
173	174	0.00	2	1.2	380	PASS
174	95	50	100	82.3	31650	PASS
175	174	5	9	8.5	2706	PASS
176	174	95	101	99.9	31610	PASS
177	176	5	9	7.1	2229	PASS