


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062121\
 Data File : VU044248.D
 Acq On : 21 Jun 2021 09:22
 Operator : SY/MD
 Sample : BFB46
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB146

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR062121WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Jun 22 01:35:06 2021

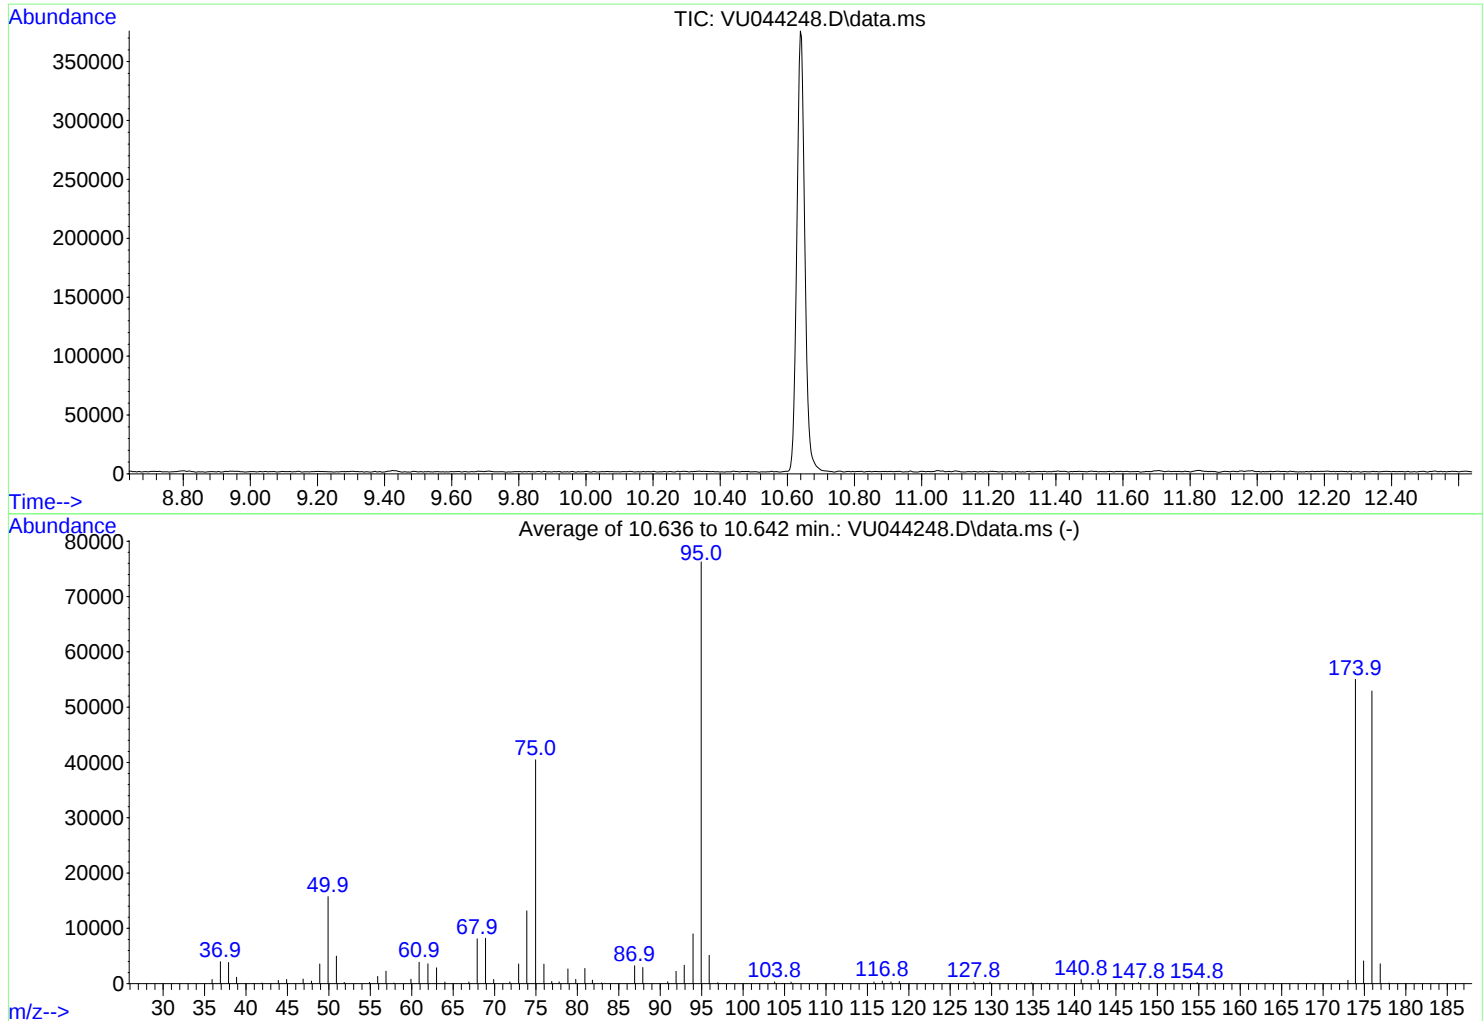

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	15753	PASS
75	95	30	80	53.1	40472	PASS
95	95	100	100	100.0	76280	PASS
96	95	5	9	6.7	5110	PASS
173	174	0.00	2	1.1	621	PASS
174	95	50	120	72.1	55035	PASS
175	174	5	9	7.5	4120	PASS
176	174	95	101	96.1	52912	PASS
177	176	5	9	6.8	3583	PASS

m/z	Abundance
38.80	133.0
39.80	175.0
40.90	199.0
42.90	223.0
43.90	552.0
55.00	241.0
56.00	143.0
57.00	112.0
68.90	124.0
70.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	737.0
36.90	3929.0
37.90	3769.0
38.90	1350.0
39.80	121.0
40.90	219.0
41.90	117.0
43.00	199.0
43.90	1139.0
44.90	789.0
46.90	847.0
47.90	440.0
48.90	3517.0
49.90	15752.0
50.90	4811.0
51.80	238.0
54.90	459.0
55.90	1476.0
56.90	2336.0
57.80	102.0
59.90	836.0
60.90	3868.0
62.00	3656.0
63.00	2852.0
64.00	270.0
66.90	301.0
67.90	8192.0
68.90	8341.0
69.90	792.0
71.80	336.0
72.90	3559.0
73.90	13196.0
75.00	40968.0
75.90	3347.0
76.90	428.0
77.80	339.0
78.80	2785.0
79.80	780.0
80.90	2788.0
81.80	677.0
82.90	149.0
86.90	3242.0
87.90	2836.0
90.90	352.0
91.90	2261.0
92.90	3337.0
94.00	8968.0
95.00	77040.0
95.90	5091.0
97.00	177.0
103.80	335.0
104.70	110.0
105.80	305.0
115.80	330.0
116.80	504.0
117.90	309.0
118.80	430.0
127.90	275.0
128.80	133.0
129.80	311.0
130.80	106.0
134.80	132.0
136.70	134.0
140.80	782.0
141.80	105.0
142.90	765.0
145.80	141.0
147.70	231.0
154.80	180.0
156.80	129.0
173.00	671.0
173.90	56840.0
174.90	4324.0
175.90	54800.0
176.90	3733.0
178.00	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	775.0
36.90	4070.0
37.90	3989.0
38.90	1299.0
39.80	136.0
40.90	219.0
41.90	124.0
43.00	236.0
43.90	1156.0
44.90	763.0
46.90	900.0
47.90	475.0
48.90	3674.0
49.90	16275.0
50.90	5147.0
51.90	236.0
54.90	464.0
55.90	1491.0
56.90	2427.0
57.90	101.0
59.90	854.0
60.90	3997.0
62.00	3679.0
63.00	2955.0
64.00	295.0
66.90	289.0
67.90	8307.0
68.90	8607.0
69.90	787.0
71.80	335.0
72.90	3657.0
73.90	13479.0
74.90	41736.0
75.90	3654.0
76.90	417.0
77.80	337.0
78.90	2723.0
79.80	831.0
80.90	2841.0
81.80	655.0
82.90	165.0
86.90	3371.0
87.90	3020.0
90.90	358.0
91.90	2276.0
92.90	3401.0
93.90	9308.0
95.00	78528.0
95.90	5251.0
97.00	173.0
103.80	333.0
104.80	113.0
105.80	301.0
110.90	104.0
115.80	322.0
116.80	477.0
117.80	334.0
118.90	393.0
127.90	298.0
128.80	124.0
129.80	280.0
134.80	131.0
136.70	135.0
140.80	771.0
142.90	743.0
145.80	106.0
147.70	200.0
154.80	203.0
156.80	126.0
173.00	655.0
173.90	56808.0
174.90	4244.0
175.90	54656.0
176.90	3697.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	747.0
36.90	3938.0
37.90	3721.0
38.90	1230.0
39.80	156.0
40.90	252.0
41.90	140.0
43.00	298.0
43.90	1118.0
44.90	712.0
46.90	812.0
47.90	462.0
48.90	3481.0
49.90	15233.0
50.90	5021.0
51.90	217.0
54.90	484.0
55.90	1355.0
56.90	2329.0
57.90	116.0
59.90	785.0
60.90	3738.0
61.90	3460.0
63.00	2793.0
64.00	299.0
66.90	273.0
67.90	7804.0
68.90	8072.0
69.90	682.0
71.90	301.0
72.90	3435.0
73.90	12828.0
74.90	38712.0
76.00	3568.0
76.90	402.0
77.80	277.0
78.90	2447.0
79.80	761.0
80.90	2651.0
81.80	604.0
82.90	147.0
86.90	3096.0
87.90	2939.0
90.90	324.0
91.90	2121.0
92.90	3256.0
93.90	8690.0
94.90	73272.0
95.90	4989.0
96.90	159.0
103.80	320.0
105.80	285.0
110.90	105.0
115.80	283.0
116.80	447.0
117.80	324.0
118.80	355.0
127.80	268.0
129.80	227.0
134.80	132.0
140.80	671.0
142.80	681.0
147.80	168.0
154.80	200.0
156.80	110.0
173.00	537.0
173.90	51456.0
174.90	3791.0
175.90	49280.0
176.90	3318.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146