

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
 Data File : VU049322.D
 Acq On : 21 Jun 2022 13:09
 Operator : SY/MD
 Sample : N3400-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AD1

Quant Time: Jun 22 01:47:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 22 01:47:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	144415	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	135856	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	67045	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	41947	3.324	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	66.400%	
7) Chloroethane-d5	1.915	69	33230	3.890	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	77.800%	
11) 1,1-Dichloroethene-d2	2.568	65	16131	3.178	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.600%	
20) 2-Butanone-d5	4.639	46	150213	44.583	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.160%	
24) Chloroform-d	5.066	84	82588	4.171	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.400%	
26) 1,2-Dichloroethane-d4	5.703	65	46631	4.294	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
32) Benzene-d6	5.729	84	156498	3.824	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	76.400%	
36) 1,2-Dichloropropane-d6	6.693	67	55393	3.988	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	79.800%	
41) Toluene-d8	7.899	98	129947	3.526	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	70.600%	
43) trans-1,3-Dichloroprop...	8.182	79	19671	3.188	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	63.800%	
46) 2-Hexanone-d5	8.635	63	99144	39.827	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.660%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	45275	4.071	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.400%	
66) 1,2-Dichlorobenzene-d4	12.192	152	52243	4.061	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	81.200%	
Target Compounds						
					Qvalue	
14) Carbon disulfide	2.793	76	11882	0.443	ug/L	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062122\
Data File : VU049322.D
Acq On : 21 Jun 2022 13:09
Operator : SY/MD
Sample : N3400-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AD1

Quant Time: Jun 22 01:47:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 22 01:47:02 2022
Response via : Initial Calibration

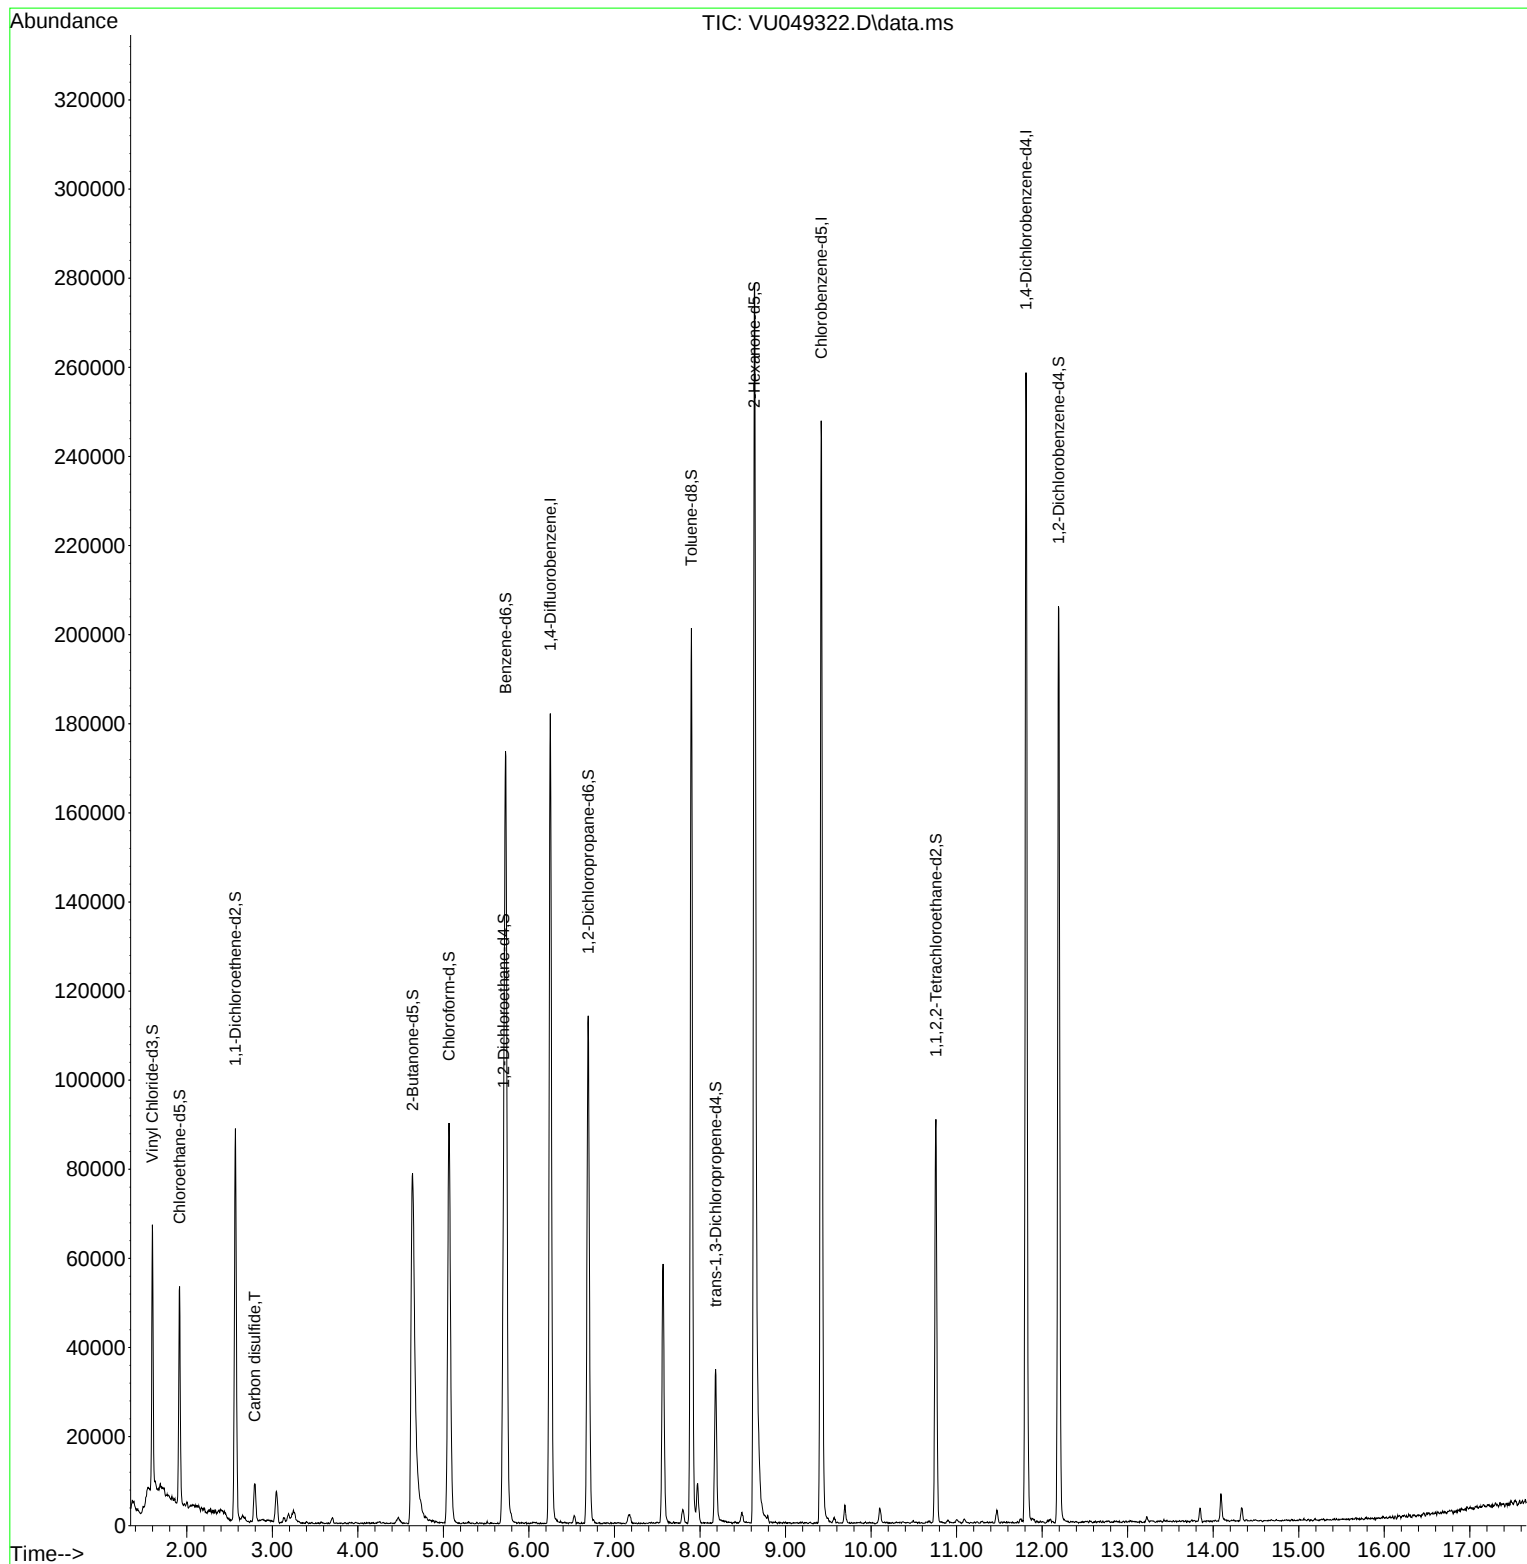

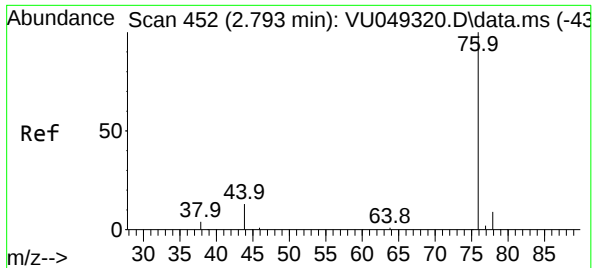

#14
Carbon disulfide
Concen: 0.443 ug/L
RT: 2.793 min Scan# 41
Delta R.T. -0.000 min
Lab File: VU049322.D
Acq: 21 Jun 2022 13:09

Instrument :
MSVOA_U
ClientSampleId :
C0AD1

Tgt Ion: 76 Resp: 11882
Ion Ratio Lower Upper
76 100
78 11.6 7.5 11.3#

